

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112718\
 Data File : P0051866.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Nov 2018 2:17
 Operator : SM/SJ
 Sample : J6071-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 112418-CHDE-F-D-M

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 10:46:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112618.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 27 01:06:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.301	3.309	15333653	4146520	23.505	17.563 #
2)	SA Decachlor...	9.912	8.025	9526668	4581601	22.846	23.157

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112718\
Data File : PO051866.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Nov 2018 2:17
Operator : SM/SJ
Sample : J6071-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
112418-CHDE-F-D-M

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 10:46:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112618.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 27 01:06:37 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

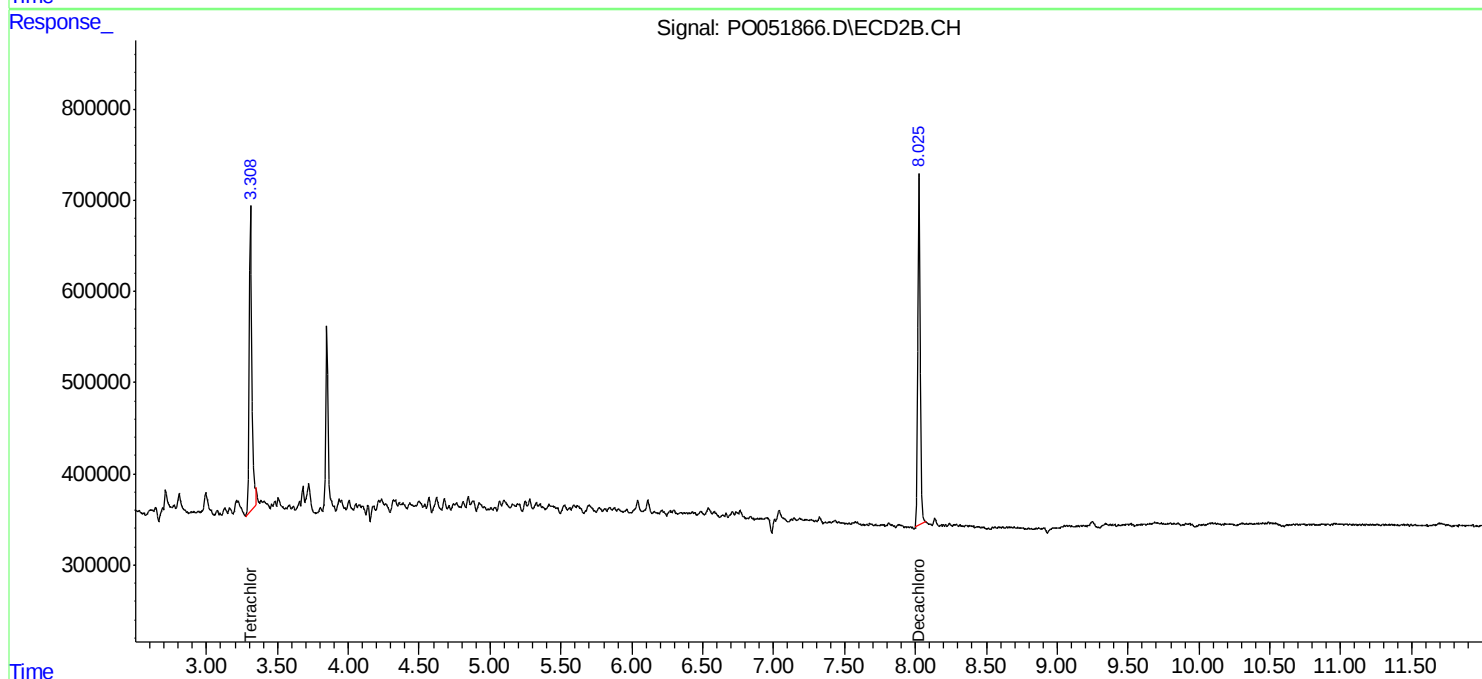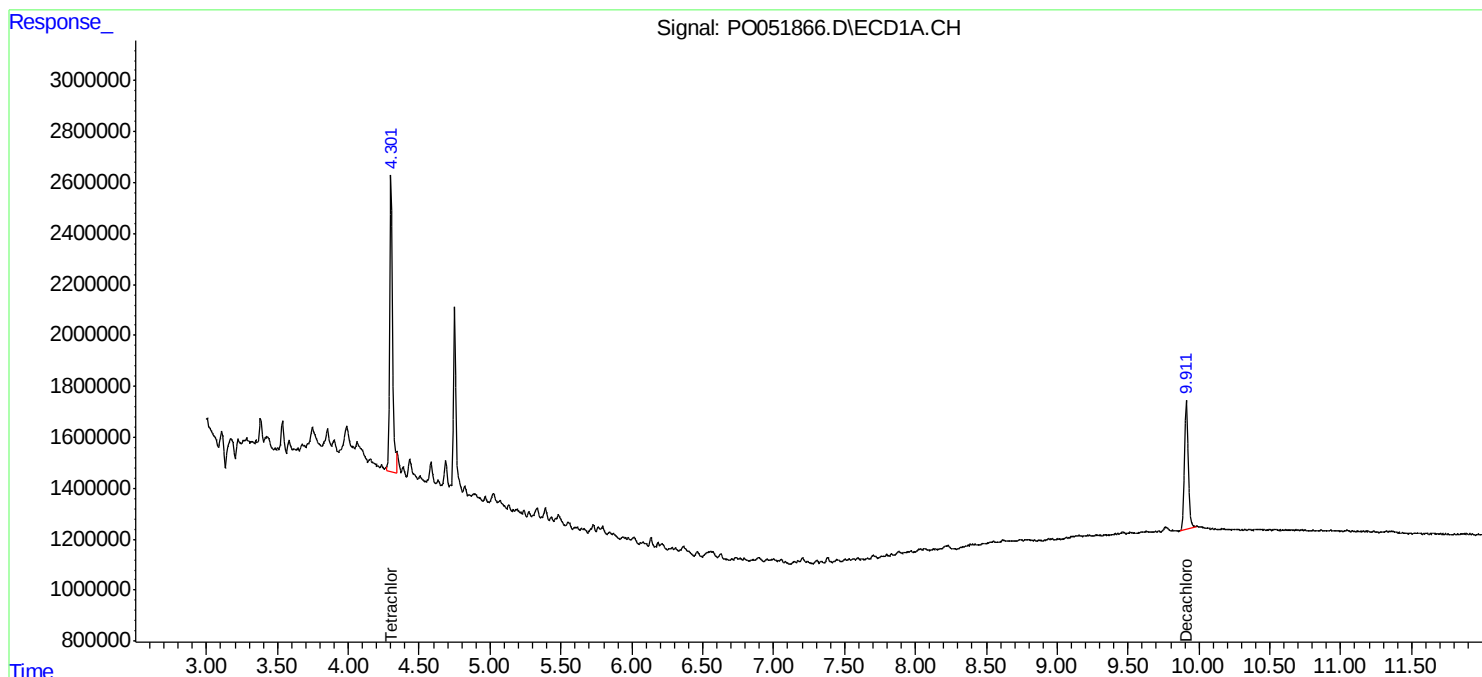


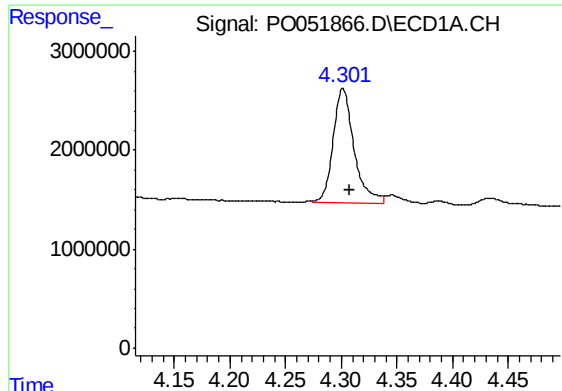

#1 Tetrachloro-m-xylene


R.T.: 4.301 min
Delta R.T.: -0.007 min
Response: 15333653
Conc: 23.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
112418-CHDE-F-D-M

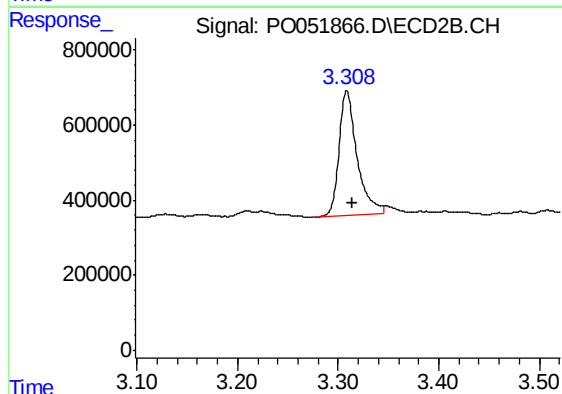


#1 Tetrachloro-m-xylene

R.T.: 3.309 min
Delta R.T.: -0.005 min
Response: 4146520
Conc: 17.56 ng/ml

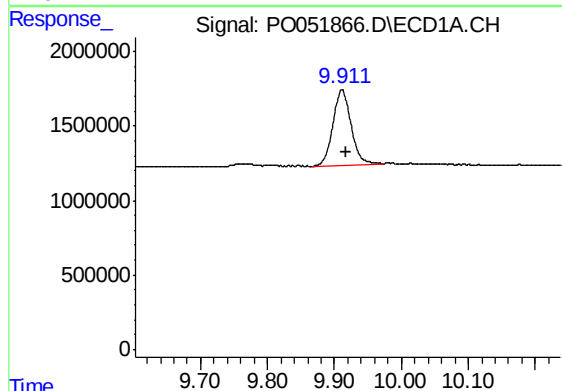

#2 Decachlorobiphenyl

R.T.: 9.912 min
Delta R.T.: -0.006 min
Response: 9526668
Conc: 22.85 ng/ml

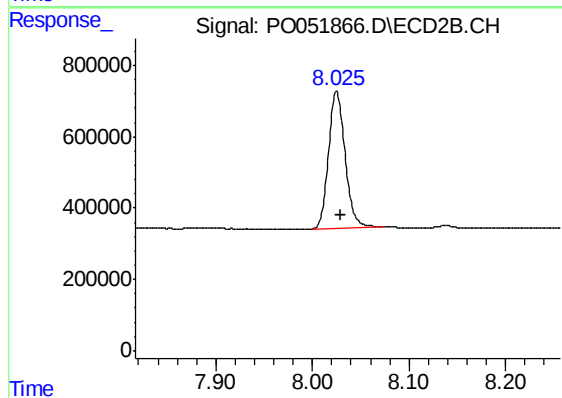

#2 Decachlorobiphenyl

R.T.: 8.025 min
Delta R.T.: -0.005 min
Response: 4581601
Conc: 23.16 ng/ml