

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112718\
 Data File : P0051883.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Nov 2018 7:05
 Operator : SM/SJ
 Sample : J6069-08
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 112318-TIPC-F-D-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 10:54:10 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112618.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 27 01:06:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.300	3.308	15050011	4385292	23.070	18.574
2)	SA Decachlor...	9.910	8.024	6965688	3384767	16.705	17.108

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112718\
Data File : P0051883.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Nov 2018 7:05
Operator : SM/SJ
Sample : J6069-08
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
112318-TIPC-F-D-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 10:54:10 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112618.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 27 01:06:37 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

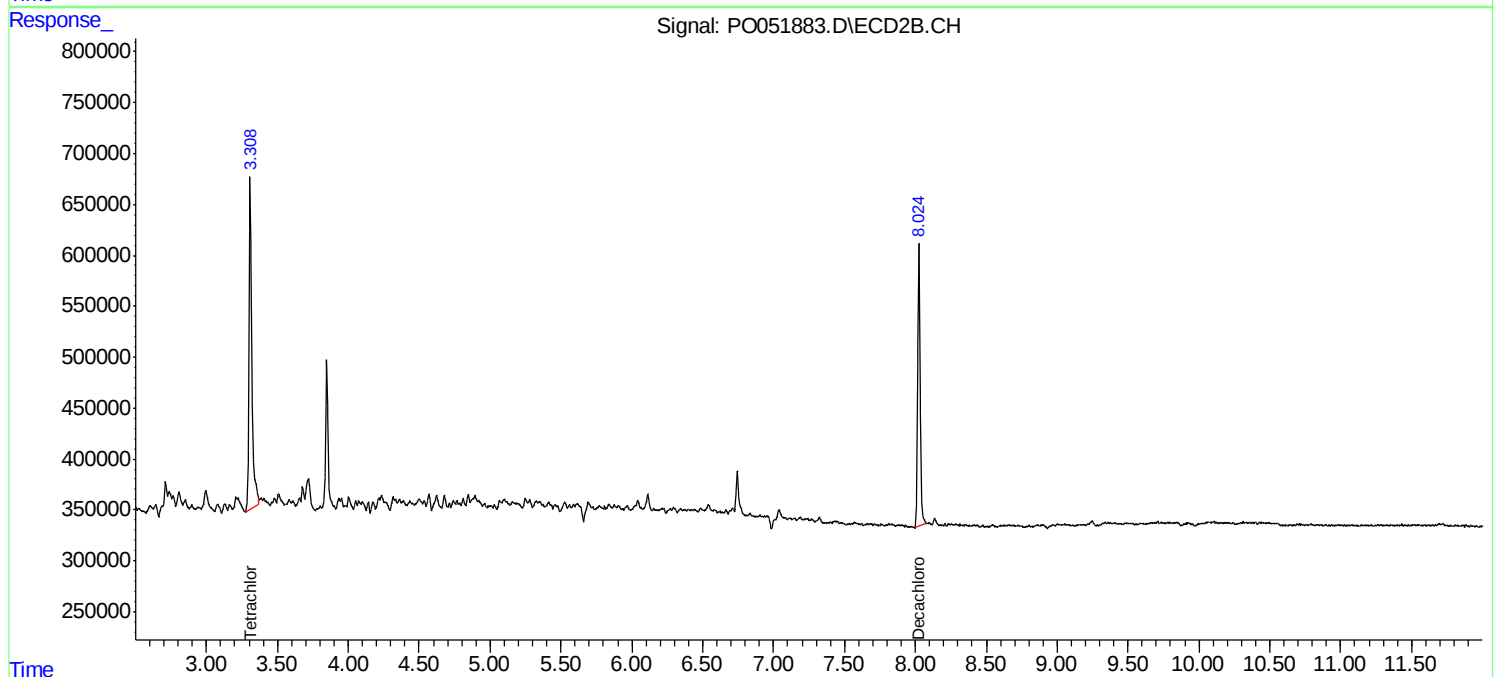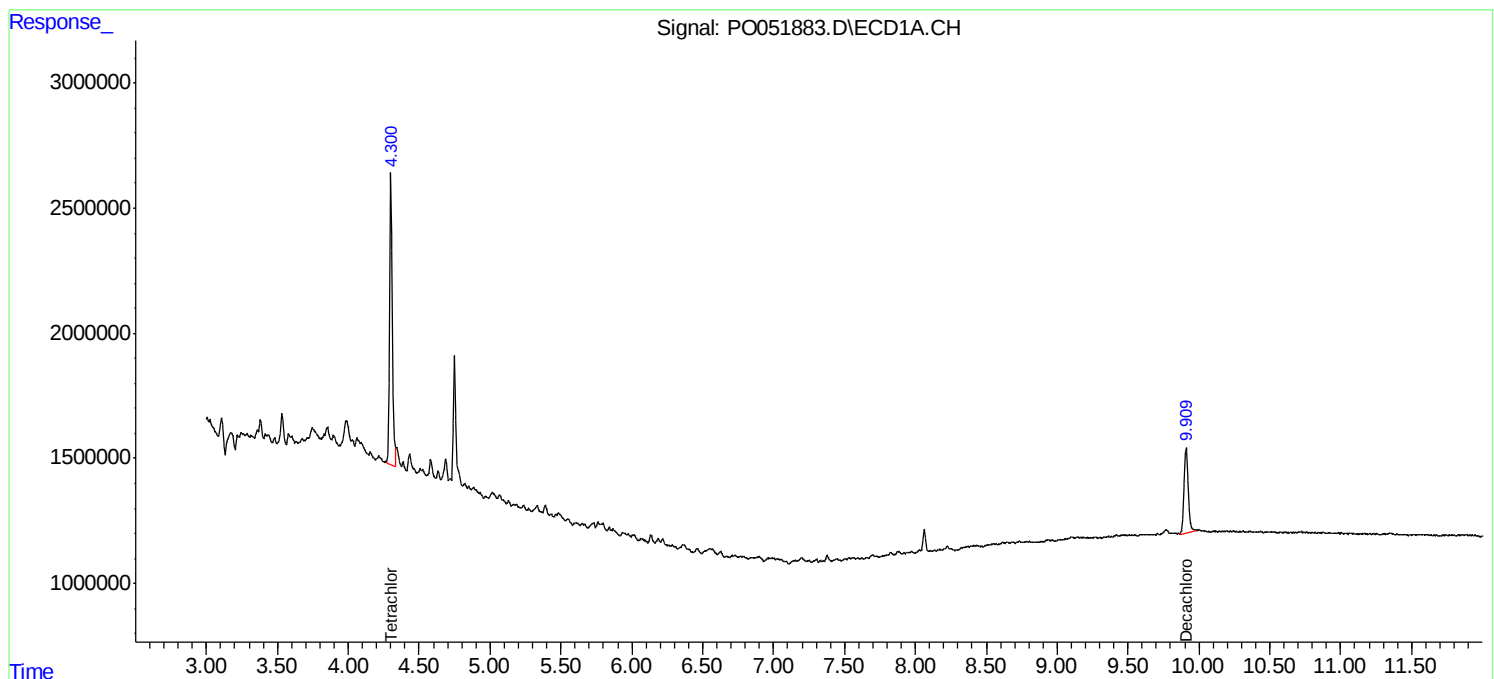


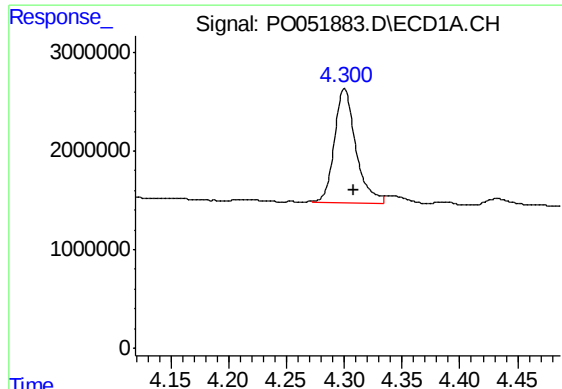

#1 Tetrachloro-m-xylene


R.T.: 4.300 min
Delta R.T.: -0.008 min
Response: 15050011
Conc: 23.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
112318-TIPC-F-D-S

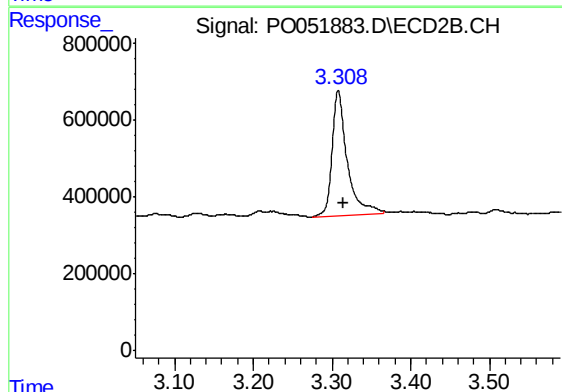


#1 Tetrachloro-m-xylene

R.T.: 3.308 min
Delta R.T.: -0.006 min
Response: 4385292
Conc: 18.57 ng/ml

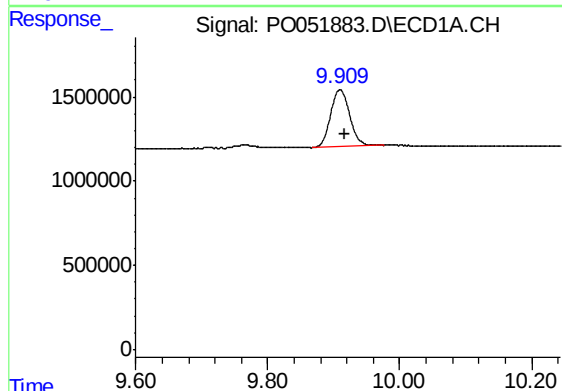

#2 Decachlorobiphenyl

R.T.: 9.910 min
Delta R.T.: -0.008 min
Response: 6965688
Conc: 16.70 ng/ml

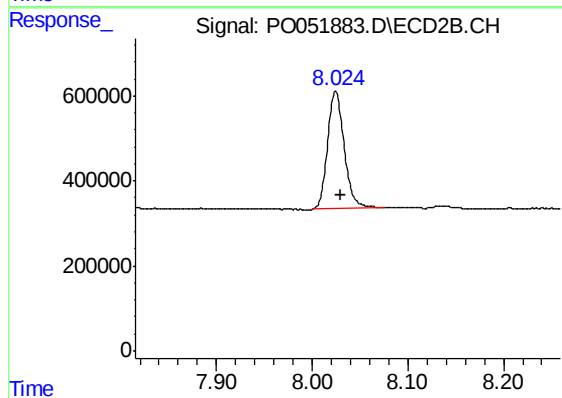

#2 Decachlorobiphenyl

R.T.: 8.024 min
Delta R.T.: -0.005 min
Response: 3384767
Conc: 17.11 ng/ml