

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112719\
Data File : P0064237.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Nov 2019 10:50
Operator : SM/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 00:39:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112719.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 28 01:28:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.313	3.562	743685	620740	25.111	26.098
2)	SA Decachlor...	9.939	8.523	721364	661292	17.601	16.188

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112719\
Data File : PO064237.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Nov 2019 10:50
Operator : SM/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 00:39:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112719.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 28 01:28:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

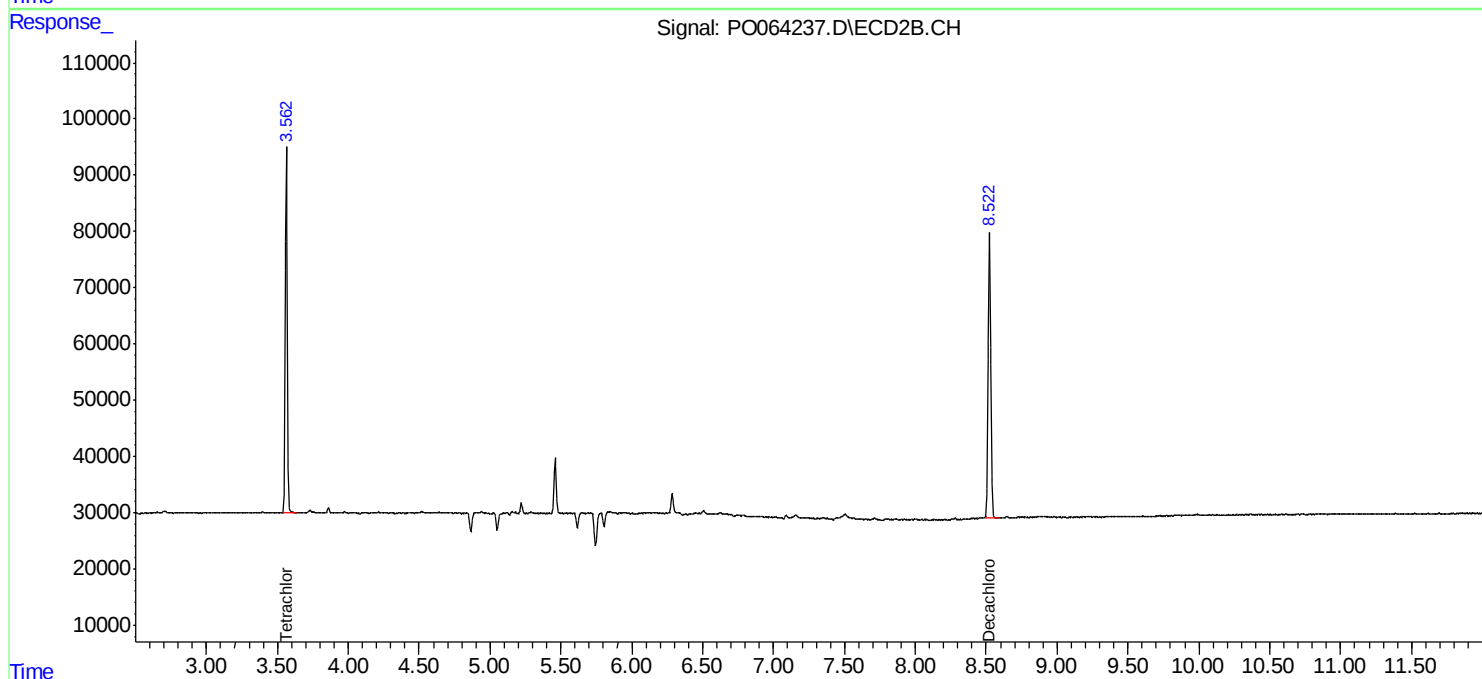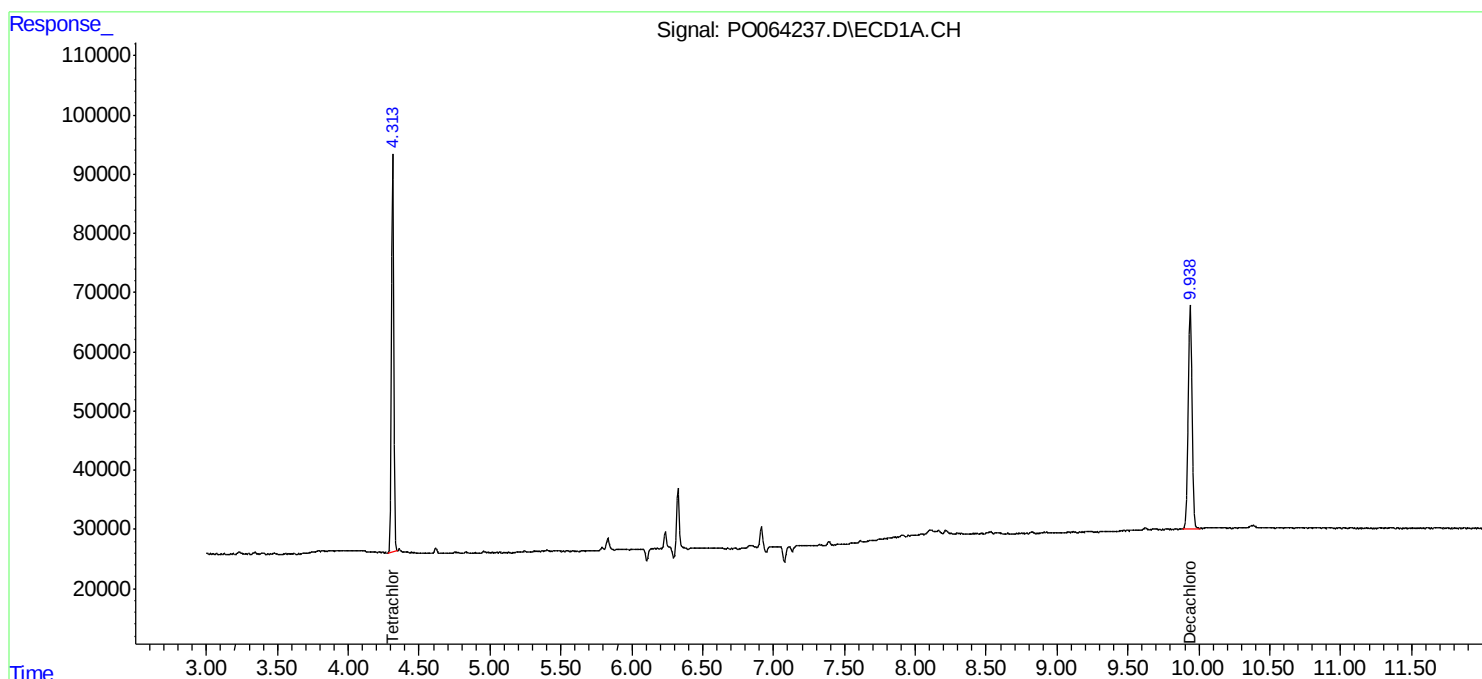


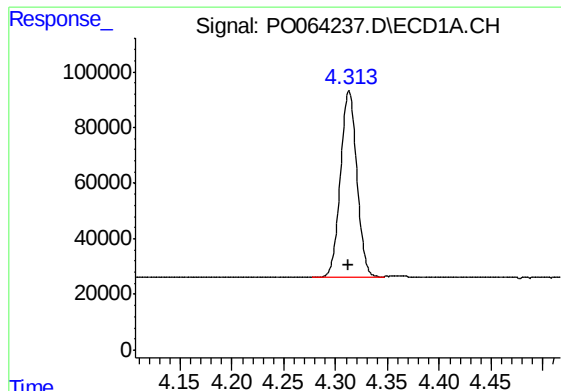

#1 Tetrachloro-m-xylene


R.T.: 4.313 min
Delta R.T.: 0.000 min
Response: 743685
Conc: 25.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

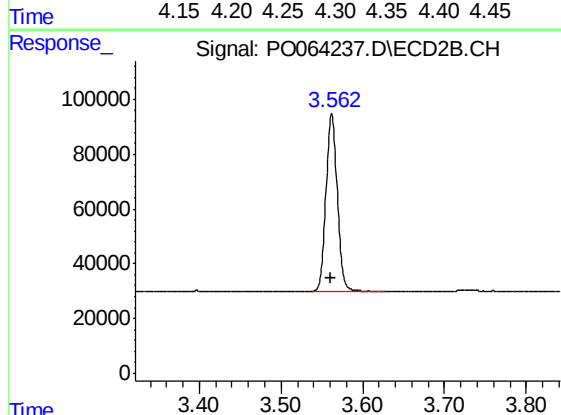


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 620740
Conc: 26.10 ng/ml

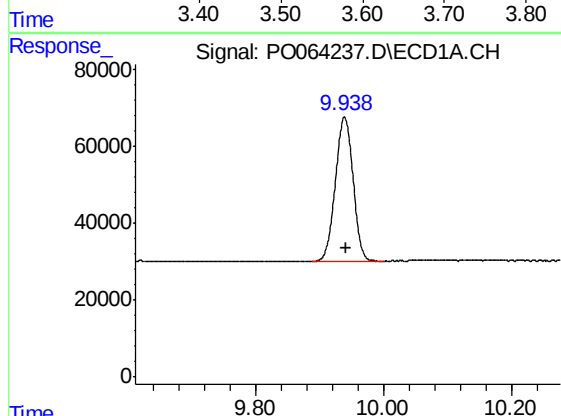

#2 Decachlorobiphenyl

R.T.: 9.939 min
Delta R.T.: -0.002 min
Response: 721364
Conc: 17.60 ng/ml

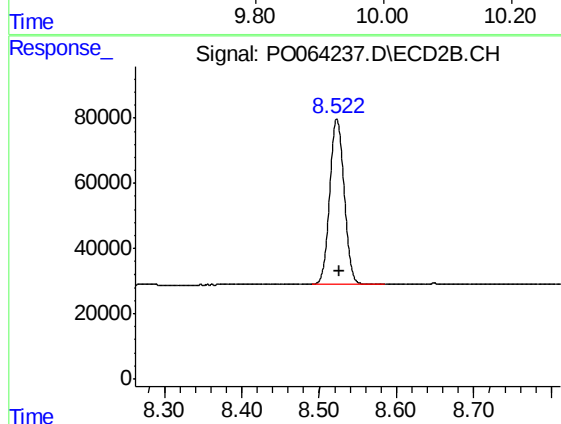

#2 Decachlorobiphenyl

R.T.: 8.523 min
Delta R.T.: -0.004 min
Response: 661292
Conc: 16.19 ng/ml