

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO112723\
 Data File : PO100080.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2023 12:47
 Operator : YP/AJ
 Sample : 05525-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 TWP13

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/28/2023
 Supervised By :Ankita Jodhani 11/28/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 13:08:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO112123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 21 15:58:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.480	3.705	36034400	29415131	21.112	19.611m
2) SA Decachlor...	10.366	8.802	18094472	26313864	24.912	23.516

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112723\
Data File : PO100080.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2023 12:47
Operator : YP/AJ
Sample : 05525-02
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TWP13


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/28/2023
Supervised By :Ankita Jodhani 11/28/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 13:08:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 21 15:58:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

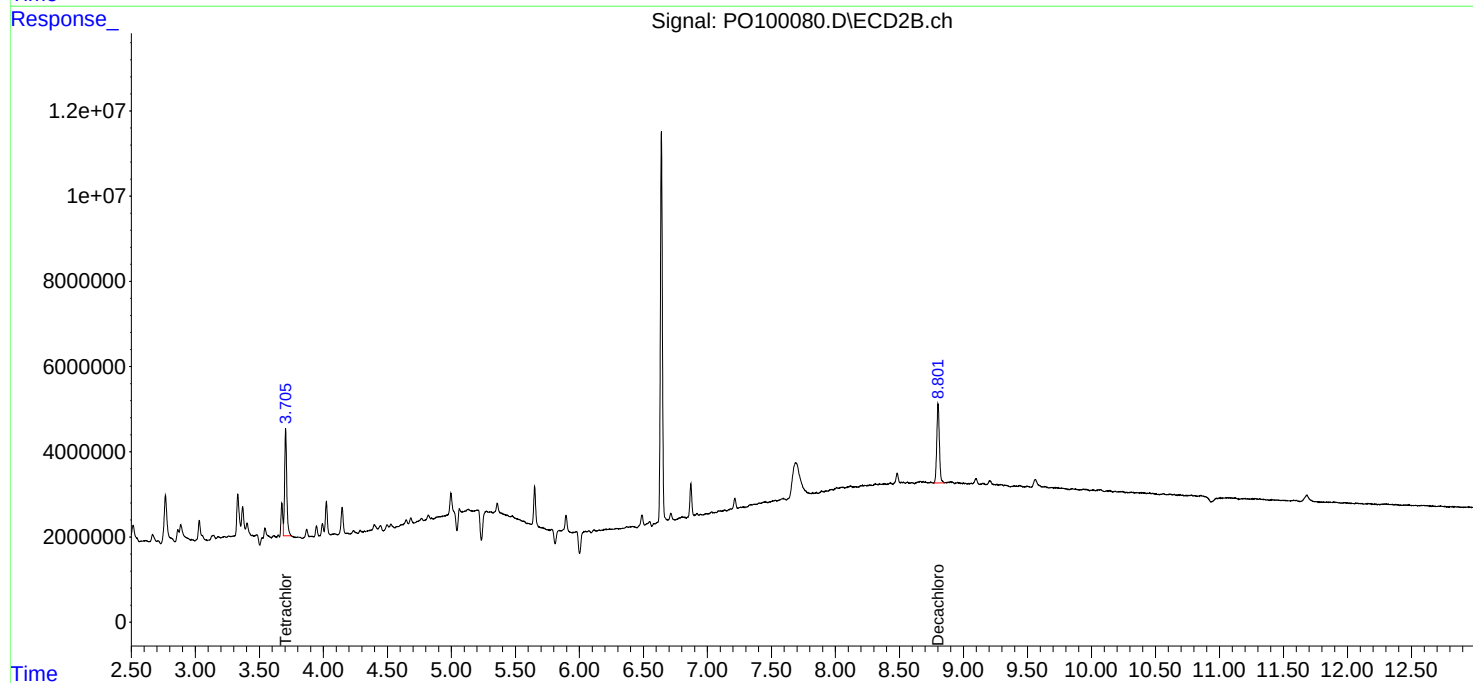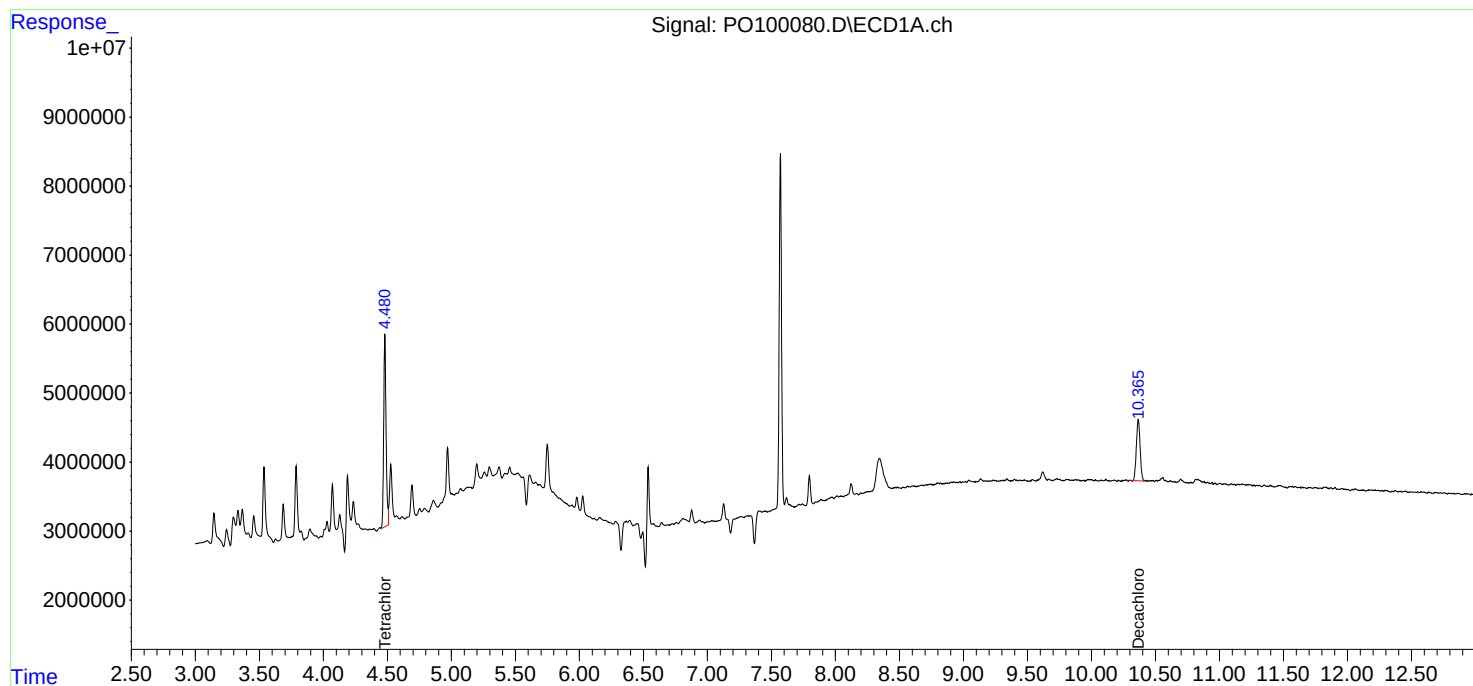

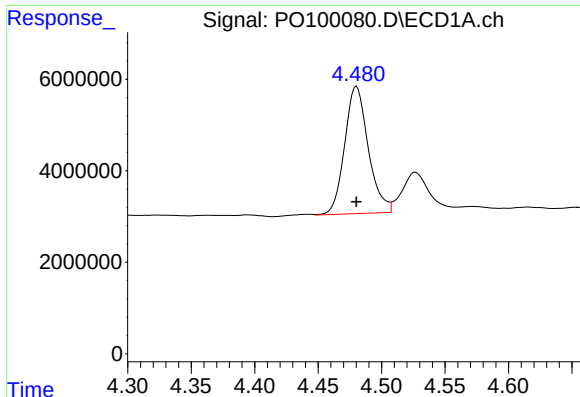


#1 Tetrachloro-m-xylene

R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 36034400
Conc: 21.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
TWP13


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/28/2023
Supervised By :Ankita Jodhani 11/28/2023

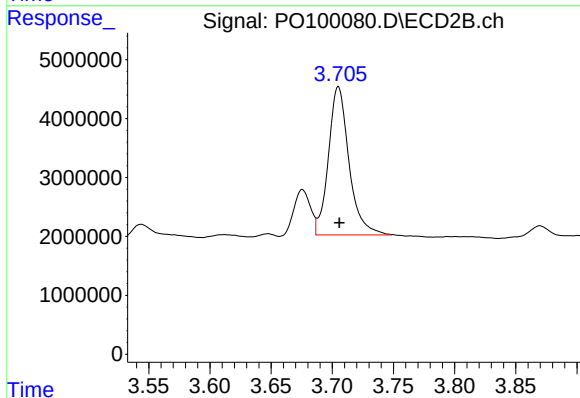


#1 Tetrachloro-m-xylene

R.T.: 3.705 min
Delta R.T.: -0.001 min
Response: 29415131
Conc: 19.61 ng/ml m

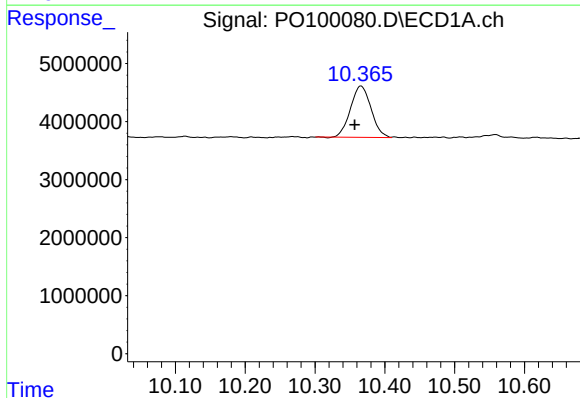

#2 Decachlorobiphenyl

R.T.: 10.366 min
Delta R.T.: 0.009 min
Response: 18094472
Conc: 24.91 ng/ml

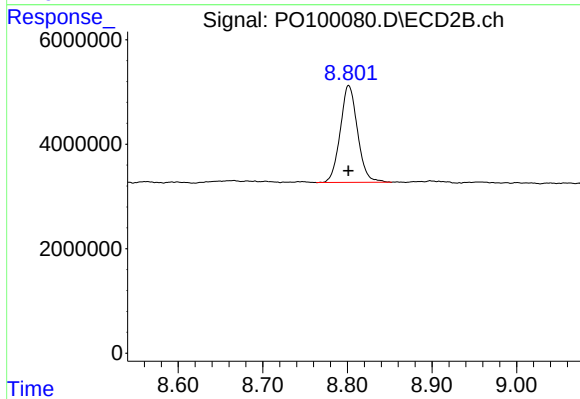

#2 Decachlorobiphenyl

R.T.: 8.802 min
Delta R.T.: 0.000 min
Response: 26313864
Conc: 23.52 ng/ml