

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0113018\
 Data File : P0052052.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Nov 2018 19:38
 Operator : SM/SJ
 Sample : J6085-01 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MH-720

Manual Integrations
 APPROVED

mohammad
 12/3/2018 1:44:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 07:52:17 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 30 03:43:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.279	3.287	2929615	832292	1.187m	0.930
2) SA Decachlor...	9.878	8.008	3392244	1387414	2.084	2.024

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO113018\
Data File : PO052052.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Nov 2018 19:38
Operator : SM/SJ
Sample : J6085-01 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MH-720


Manual Integrations
APPROVED

mohammad
12/3/2018 1:44:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 07:52:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112918.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 30 03:43:16 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

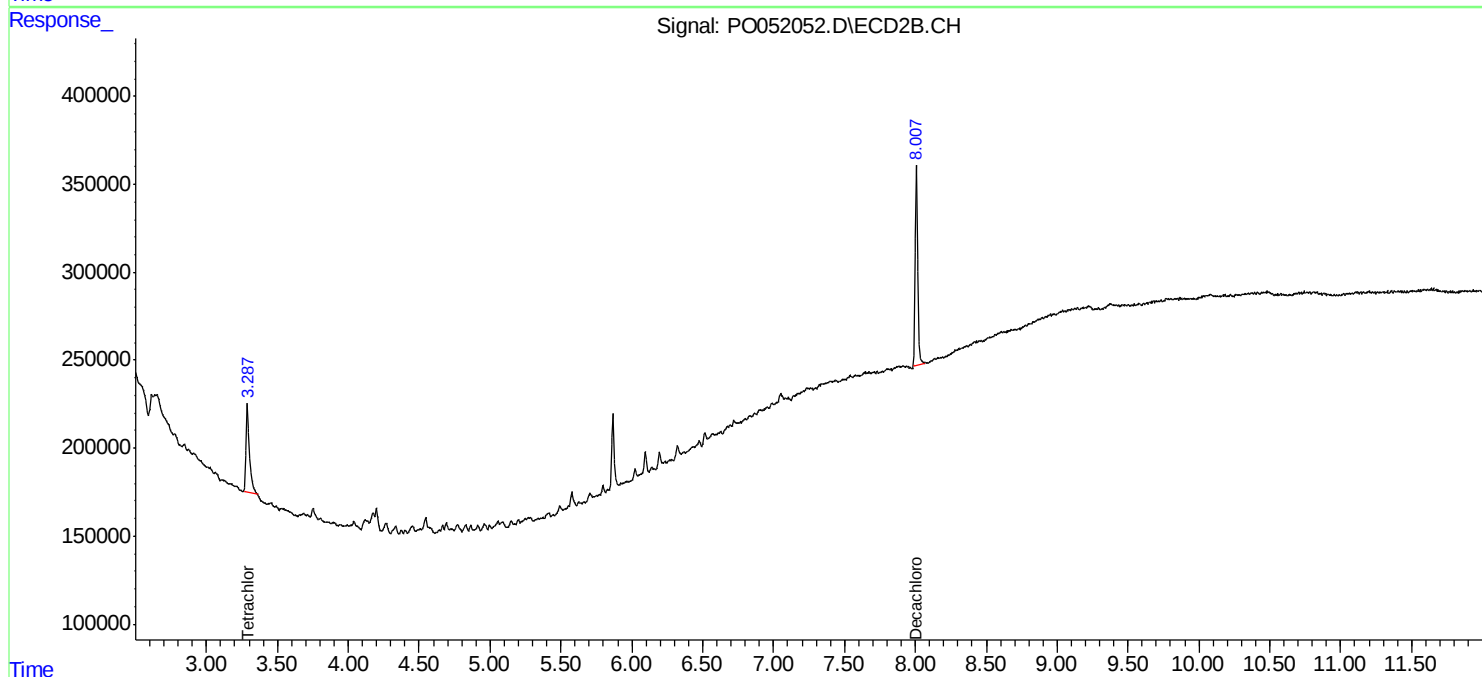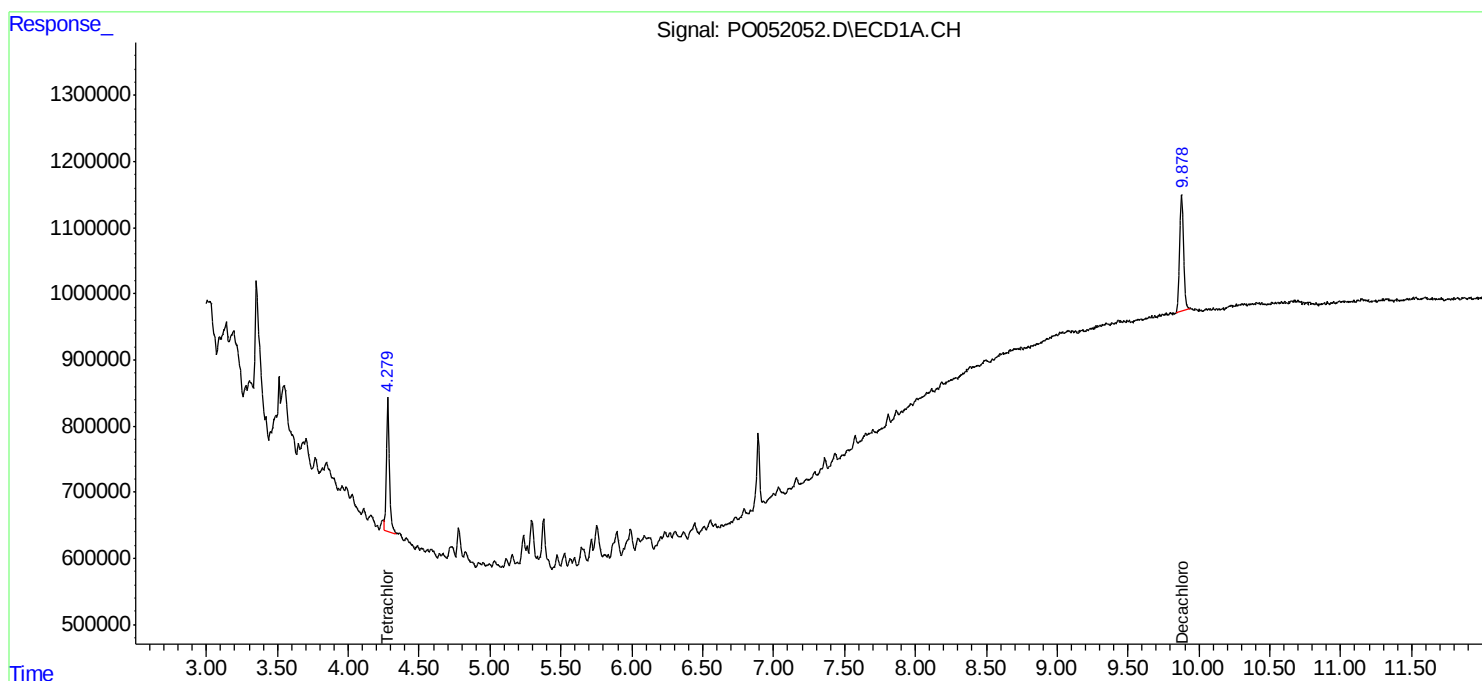

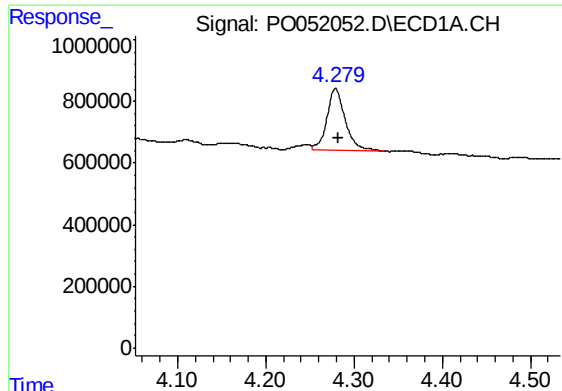


#1 Tetrachloro-m-xylene

R.T.: 4.279 min
Delta R.T.: -0.003 min
Response: 2929615
Conc: 1.19 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MH-720


Manual Integrations
APPROVED

mohammad
12/3/2018 1:44:55 PM

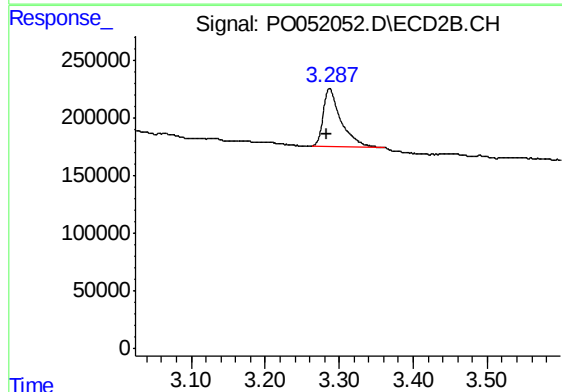


#1 Tetrachloro-m-xylene

R.T.: 3.287 min
Delta R.T.: 0.004 min
Response: 832292
Conc: 0.93 ng/ml

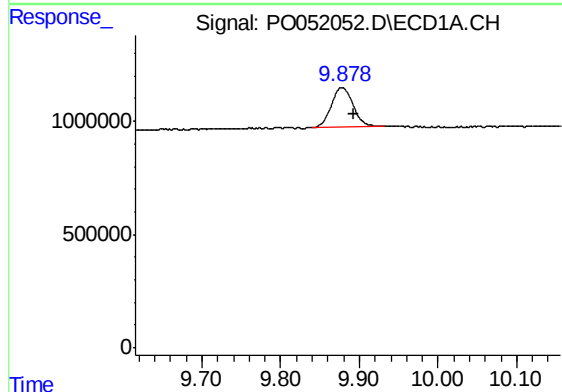

#2 Decachlorobiphenyl

R.T.: 9.878 min
Delta R.T.: -0.014 min
Response: 3392244
Conc: 2.08 ng/ml

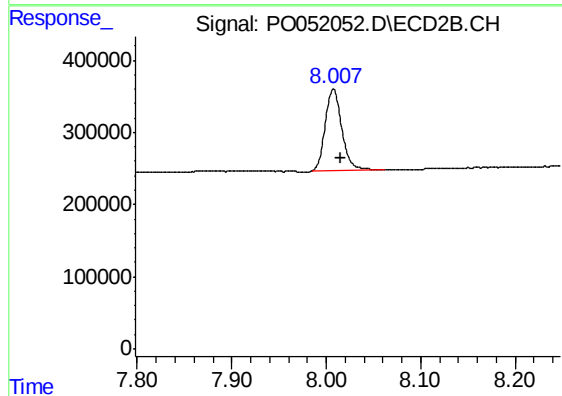

#2 Decachlorobiphenyl

R.T.: 8.008 min
Delta R.T.: -0.007 min
Response: 1387414
Conc: 2.02 ng/ml