

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO113018\
 Data File : P0052068.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Dec 2018 00:09
 Operator : SM/SJ
 Sample : J6128-05
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 112718-TIPC-F-D-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 03:16:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 30 03:43:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.277	3.283	50851962	14287504	20.604	15.960
2) SA Decachlor...	9.876	8.008	23921908	9868683	14.696	14.400

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO113018\
Data File : PO052068.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Dec 2018 00:09
Operator : SM/SJ
Sample : J6128-05
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
112718-TIPC-F-D-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 03:16:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112918.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 30 03:43:16 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

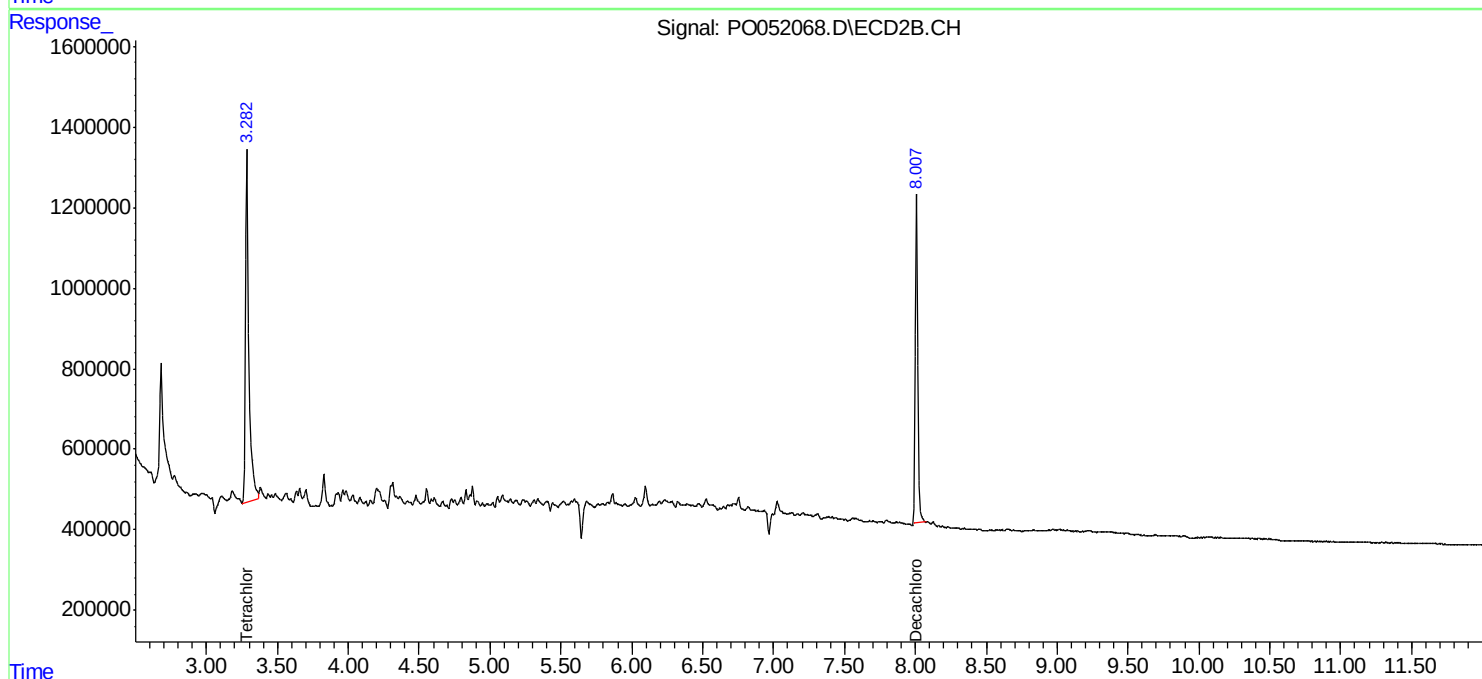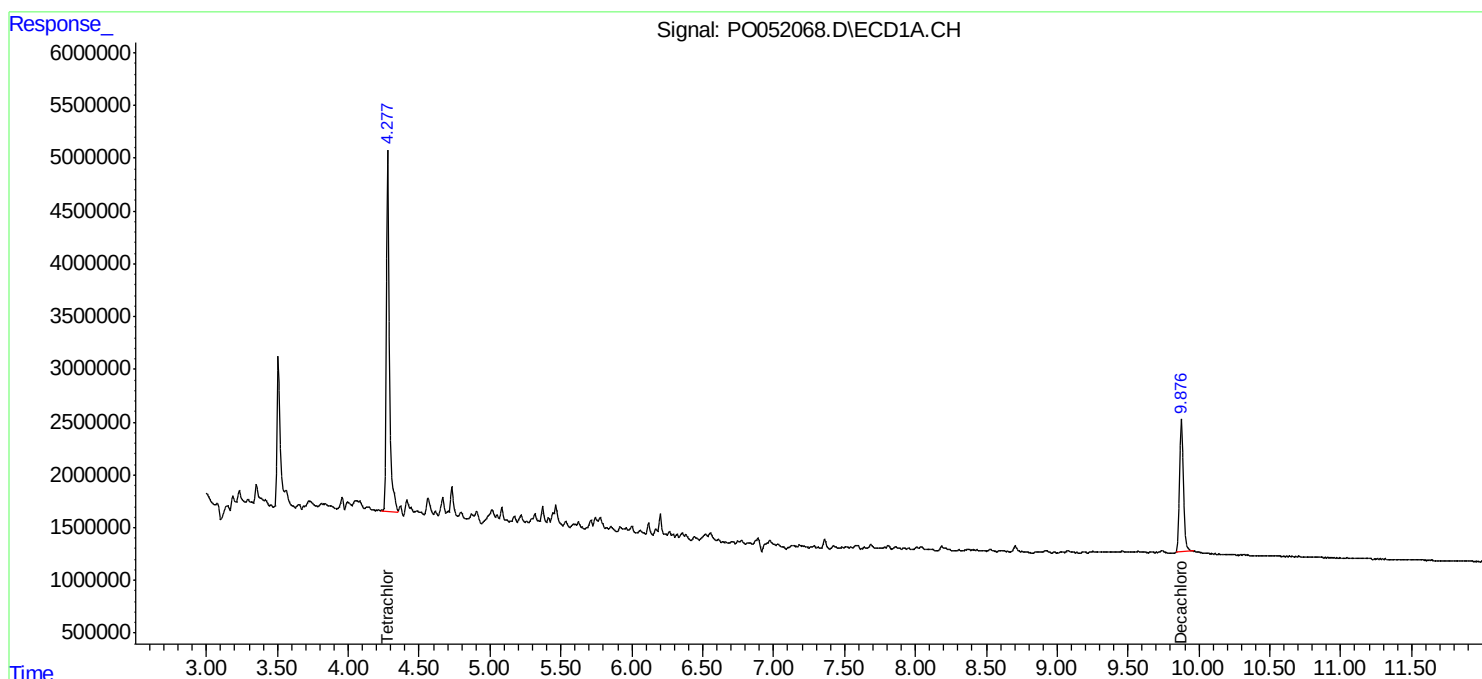


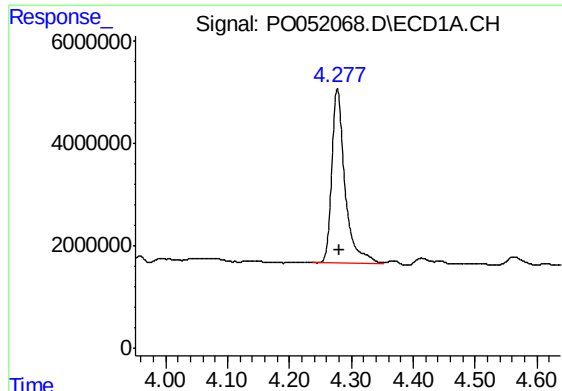

#1 Tetrachloro-m-xylene


R.T.: 4.277 min
Delta R.T.: -0.005 min
Response: 50851962
Conc: 20.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
112718-TIPC-F-D-B

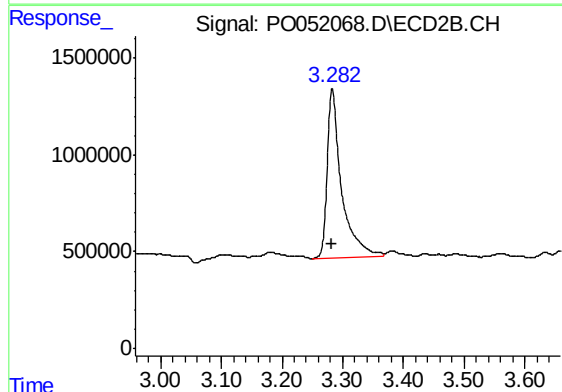


#1 Tetrachloro-m-xylene

R.T.: 3.283 min
Delta R.T.: 0.000 min
Response: 14287504
Conc: 15.96 ng/ml

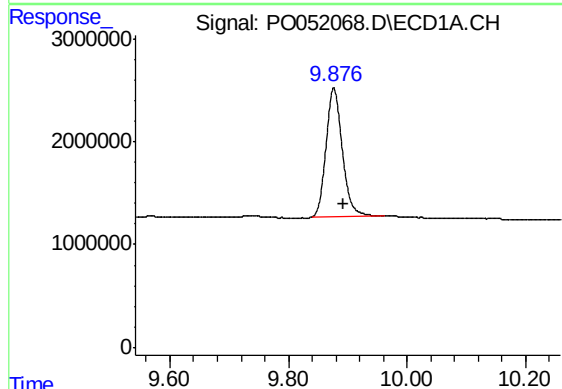

#2 Decachlorobiphenyl

R.T.: 9.876 min
Delta R.T.: -0.016 min
Response: 23921908
Conc: 14.70 ng/ml

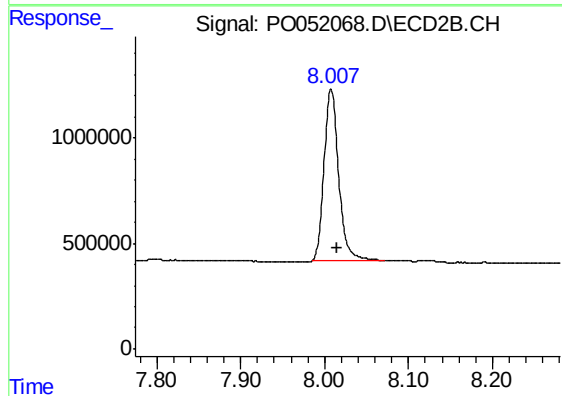

#2 Decachlorobiphenyl

R.T.: 8.008 min
Delta R.T.: -0.007 min
Response: 9868683
Conc: 14.40 ng/ml