

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO113021\
 Data File : PO083264.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Nov 2021 22:02
 Operator : AJ\MA
 Sample : M4850-06 10X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 22:49:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Nov 20 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.949	3.950	123466	46766	1.407	1.534
2)	SA Decachlor...	11.037	9.255	117716	46959	1.790	1.562
Target Compounds							
9)	L2 AR-1221-2	5.310	0.000	49299	0	73.322	N.D. #
28)	L6 AR-1254-3	7.832f	0.000	78107	0	18.185	N.D. #
30)	L6 AR-1254-5	8.531	0.000	6031	0	1.881	N.D. #
33)	L7 AR-1260-3	8.614	0.000	8089	0	2.827	N.D. #
34)	L7 AR-1260-4	8.871f	0.000	16538	0	5.120	N.D. #
35)	L7 AR-1260-5	9.182	0.000	4251	0	0.671	N.D. #
36)	L8 AR-1262-1	8.614	0.000	8089	0	2.169	N.D. #
37)	L8 AR-1262-2	9.182	0.000	4251	0	0.661	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO113021\
Data File : PO083264.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Nov 2021 22:02
Operator : AJ\MA
Sample : M4850-06 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 22:49:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Nov 20 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

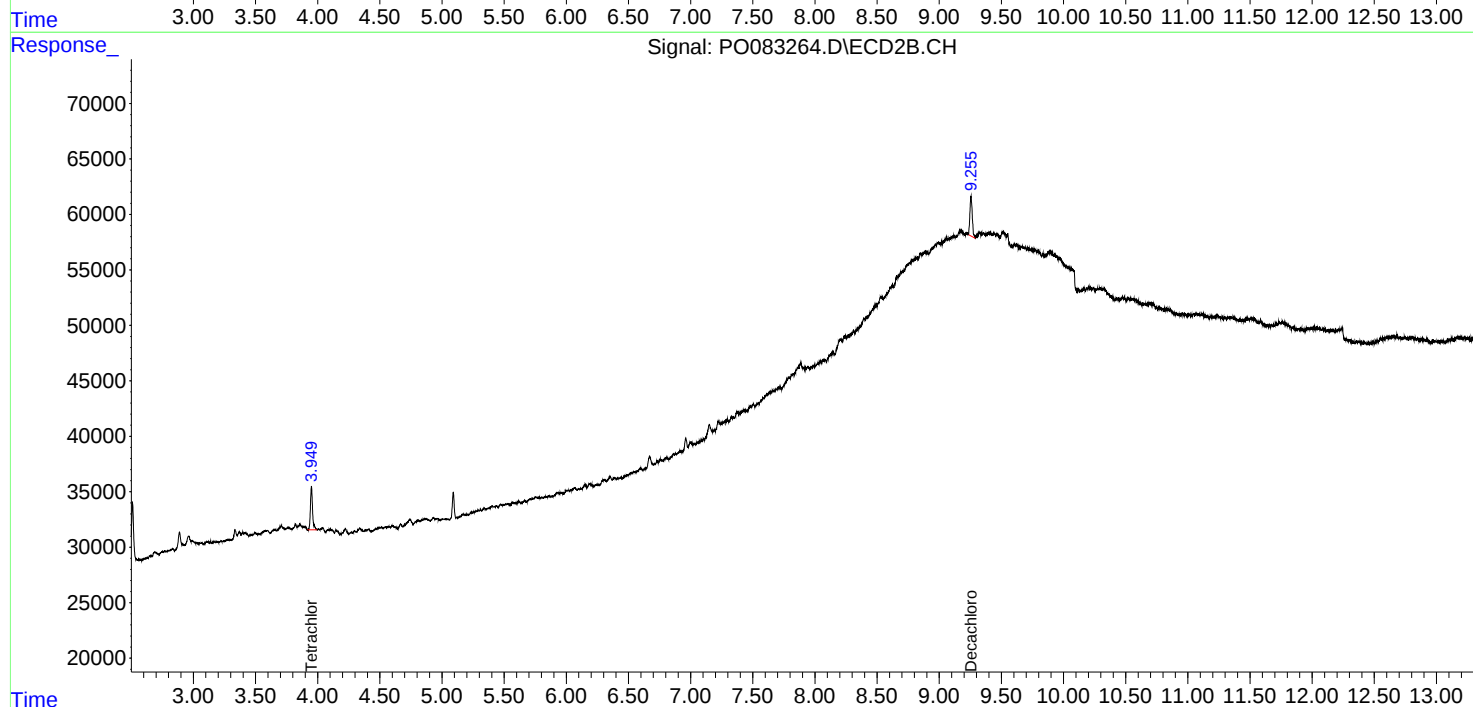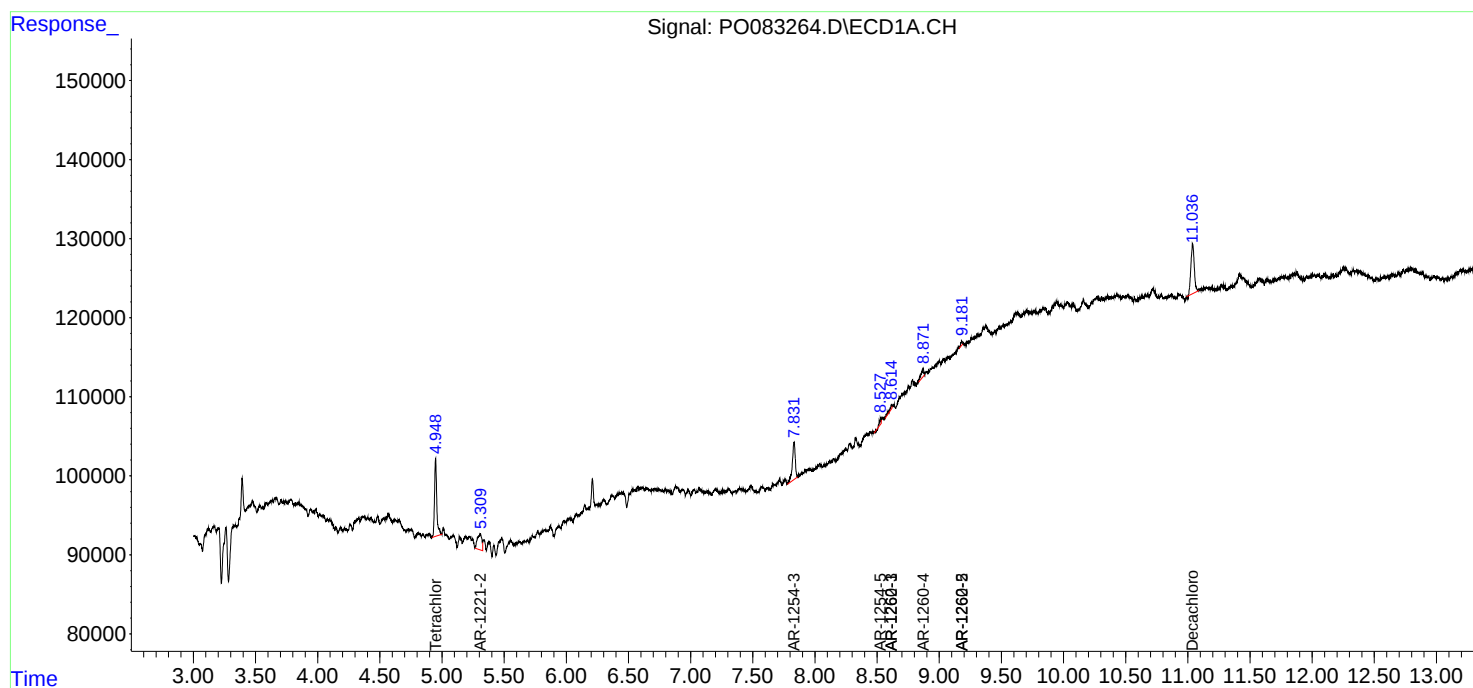


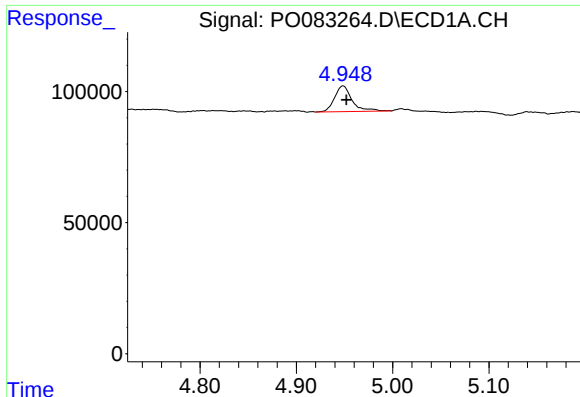

#1 Tetrachloro-m-xylene


R.T.: 4.949 min
Delta R.T.: -0.003 min
Response: 123466
Conc: 1.41 ng/ml

Instrument :
ECD_O
ClientSampleId :

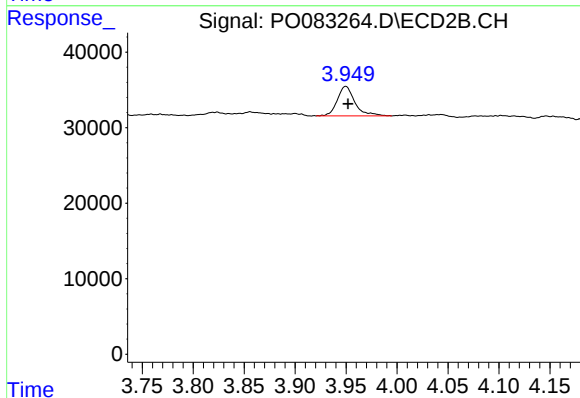


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: -0.002 min
Response: 46766
Conc: 1.53 ng/ml

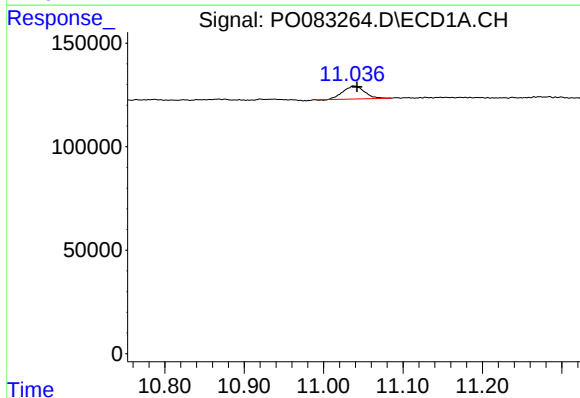


#2 Decachlorobiphenyl

R.T.: 11.037 min
Delta R.T.: -0.005 min
Response: 117716
Conc: 1.79 ng/ml

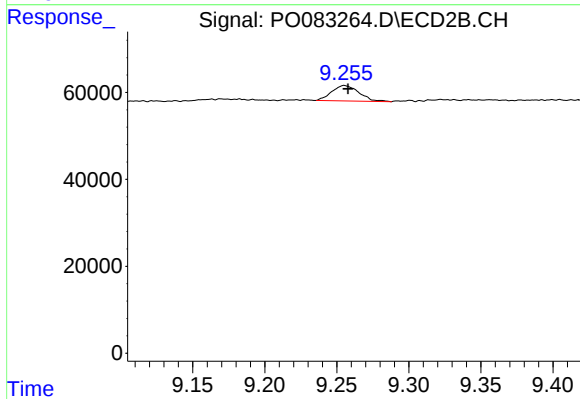

#2 Decachlorobiphenyl


R.T.: 9.255 min
Delta R.T.: -0.003 min
Response: 46959
Conc: 1.56 ng/ml

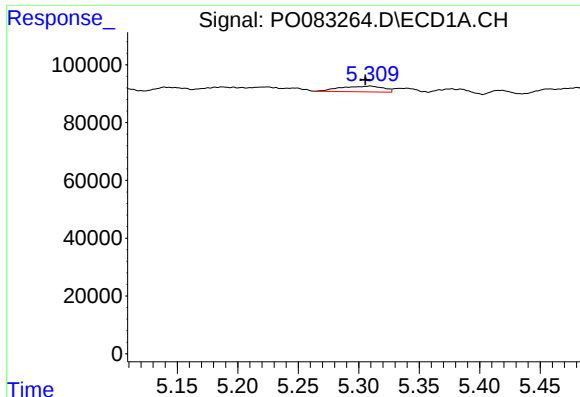

#9 AR-1221-2


R.T.: 5.310 min
Delta R.T.: 0.004 min
Response: 49299
Conc: 73.32 ng/ml

Instrument :
ECD_O
ClientSampleId :

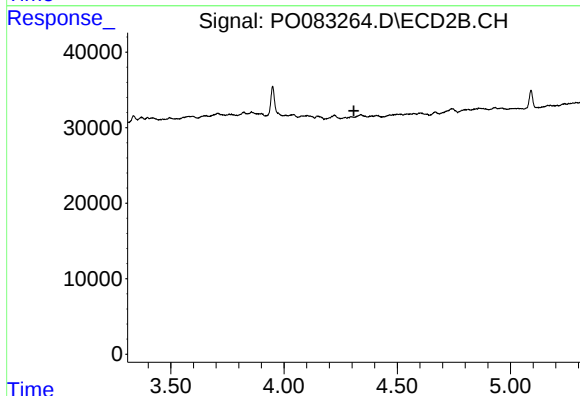


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.309 min
Response: 0
Conc: N.D.

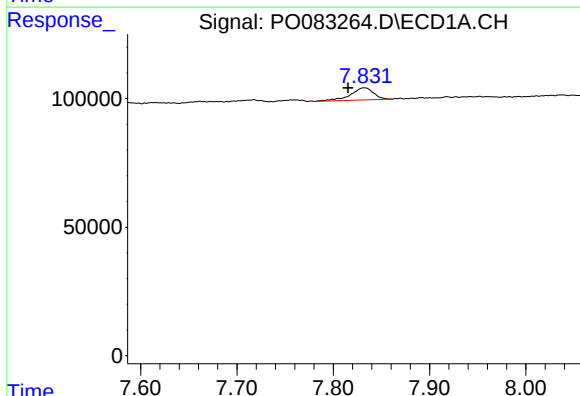


#28 AR-1254-3

R.T.: 7.832 min
Delta R.T.: 0.016 min
Response: 78107
Conc: 18.19 ng/ml

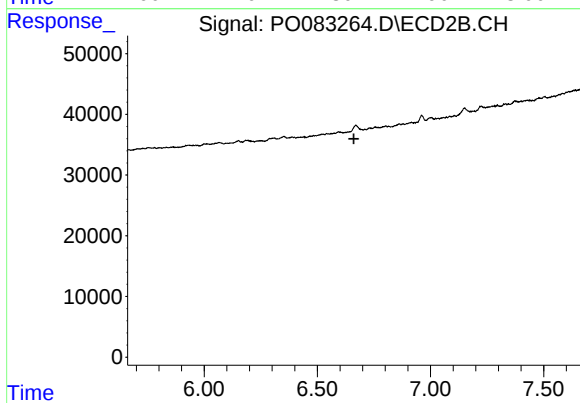

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.661 min
Response: 0
Conc: N.D.

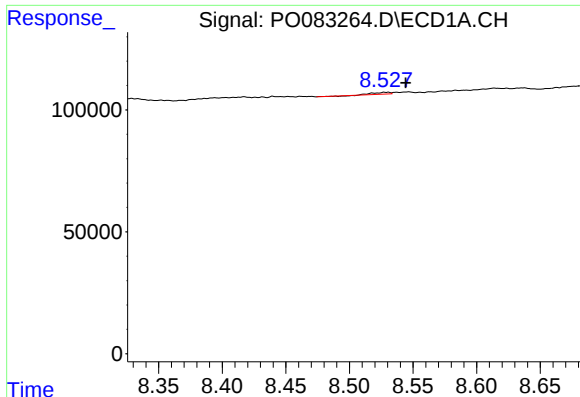

#30 AR-1254-5


R.T.: 8.531 min
Delta R.T.: -0.014 min
Response: 6031
Conc: 1.88 ng/ml

Instrument :
ECD_O
ClientSampleId :

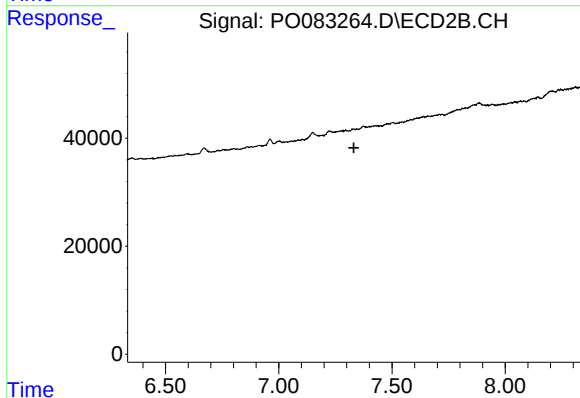


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.332 min
Response: 0
Conc: N.D.

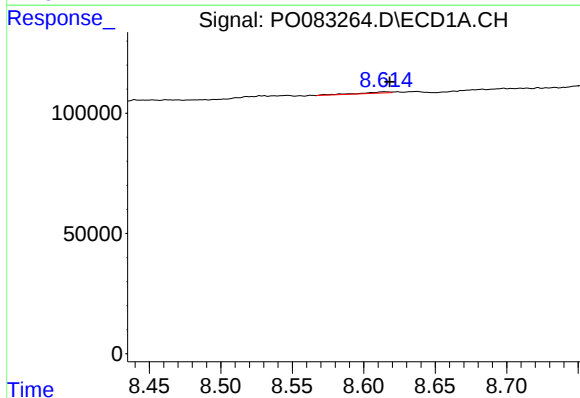


#33 AR-1260-3

R.T.: 8.614 min
Delta R.T.: -0.004 min
Response: 8089
Conc: 2.83 ng/ml

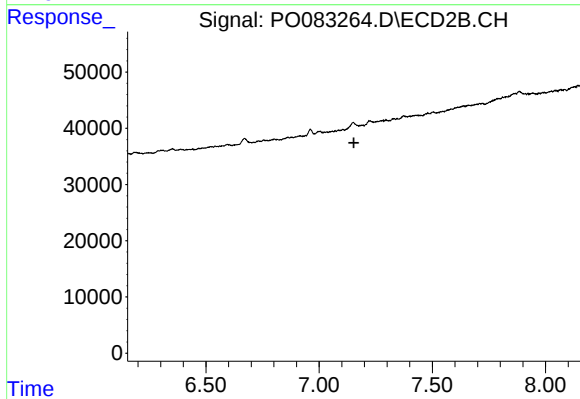

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.153 min
Response: 0
Conc: N.D.

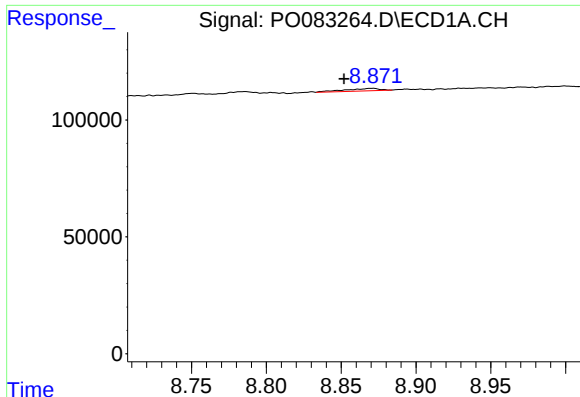

#34 AR-1260-4


R.T.: 8.871 min
Delta R.T.: 0.020 min
Response: 16538
Conc: 5.12 ng/ml

Instrument :
ECD_O
ClientSampleId :

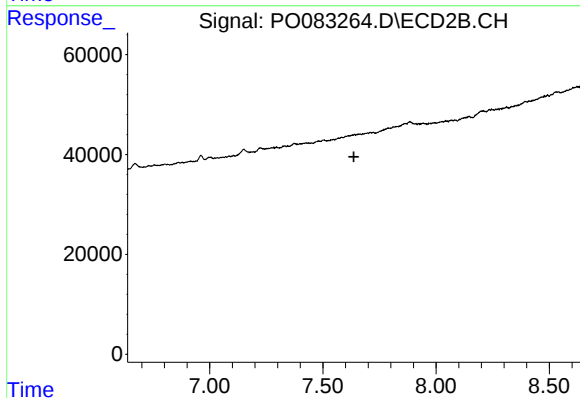


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.637 min
Response: 0
Conc: N.D.

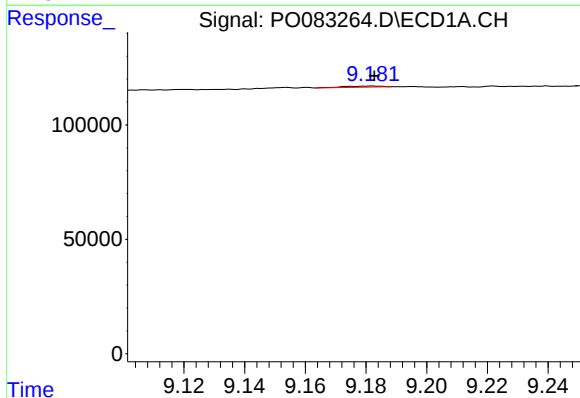


#35 AR-1260-5

R.T.: 9.182 min
Delta R.T.: 0.000 min
Response: 4251
Conc: 0.67 ng/ml

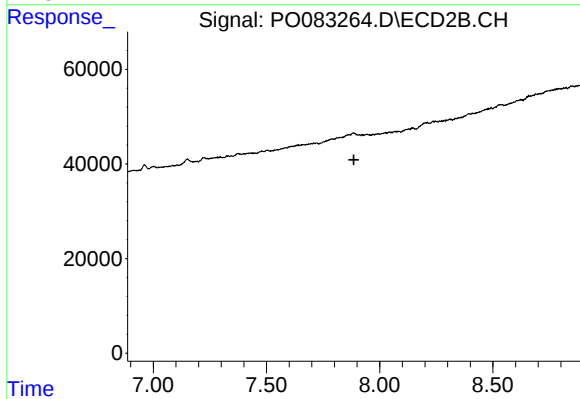

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.886 min
Response: 0
Conc: N.D.

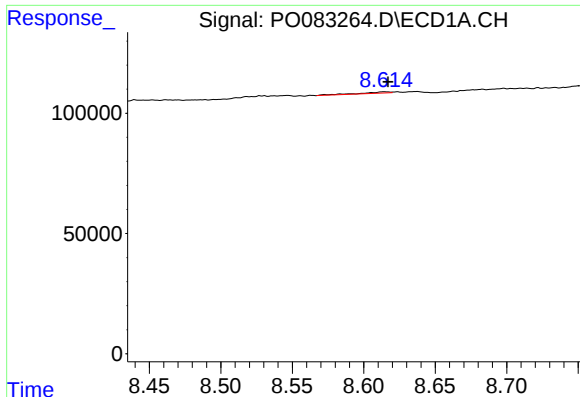

#36 AR-1262-1


R.T.: 8.614 min
Delta R.T.: -0.003 min
Response: 8089
Conc: 2.17 ng/ml

Instrument :
ECD_O
ClientSampleId :

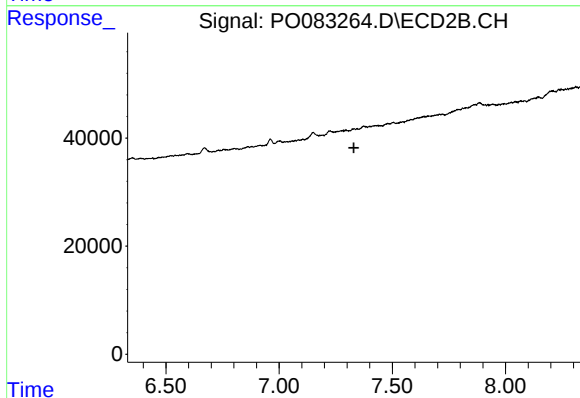


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.330 min
Response: 0
Conc: N.D.

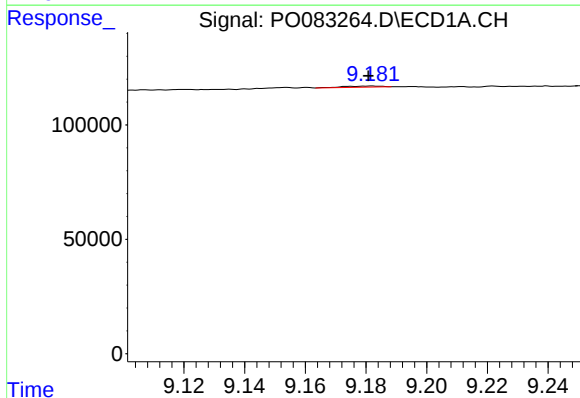

#37 AR-1262-2

R.T.: 9.182 min
Delta R.T.: 0.001 min
Response: 4251
Conc: 0.66 ng/ml

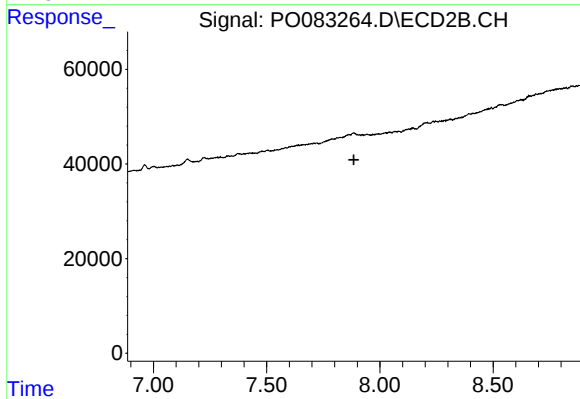

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.885 min
Response: 0
Conc: N.D.