

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO113021\
Data File : PO083255.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Nov 2021 19:27
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 22:45:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Nov 20 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.948	3.950	2051450	651624	23.376	21.377
2) SA Decachlor...	11.037	9.257	1513121	625084	23.011	20.793

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO113021\
Data File : PO083255.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Nov 2021 19:27
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 22:45:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Nov 20 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

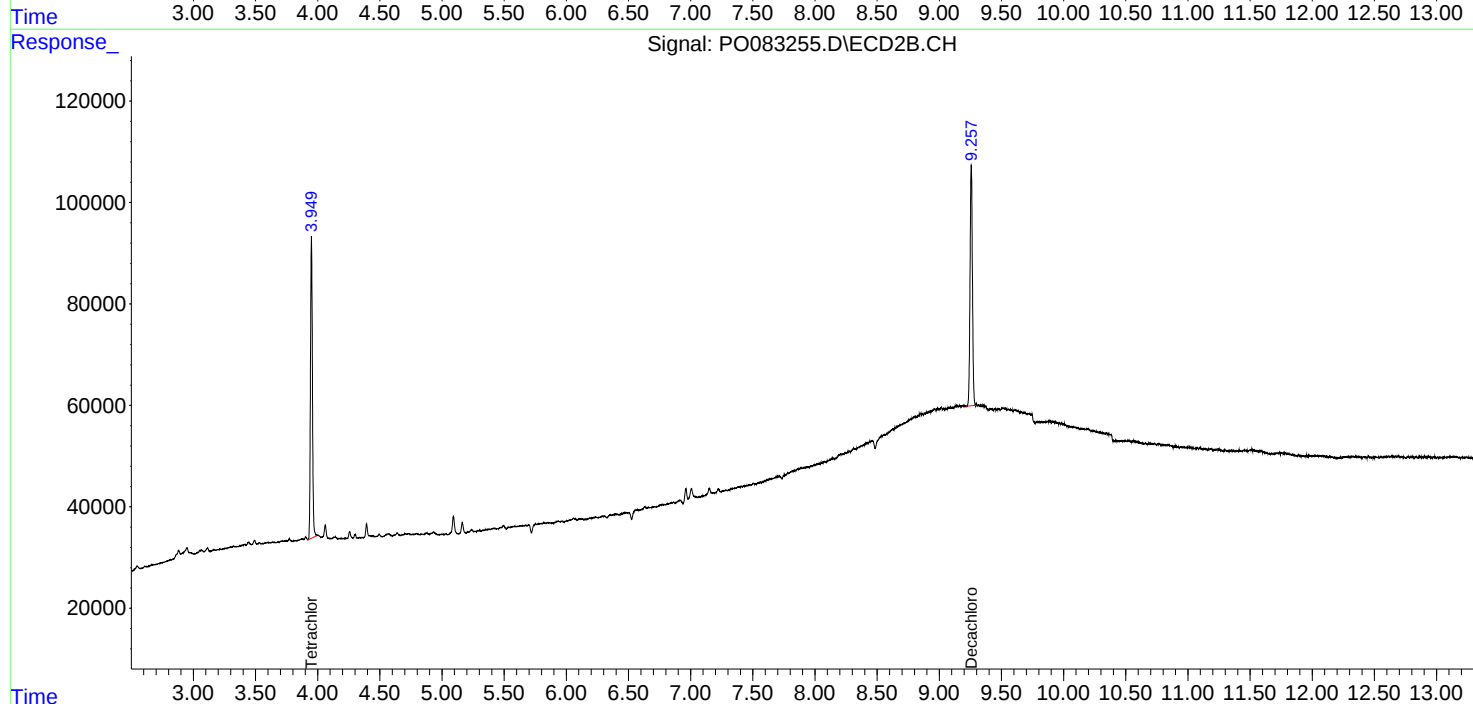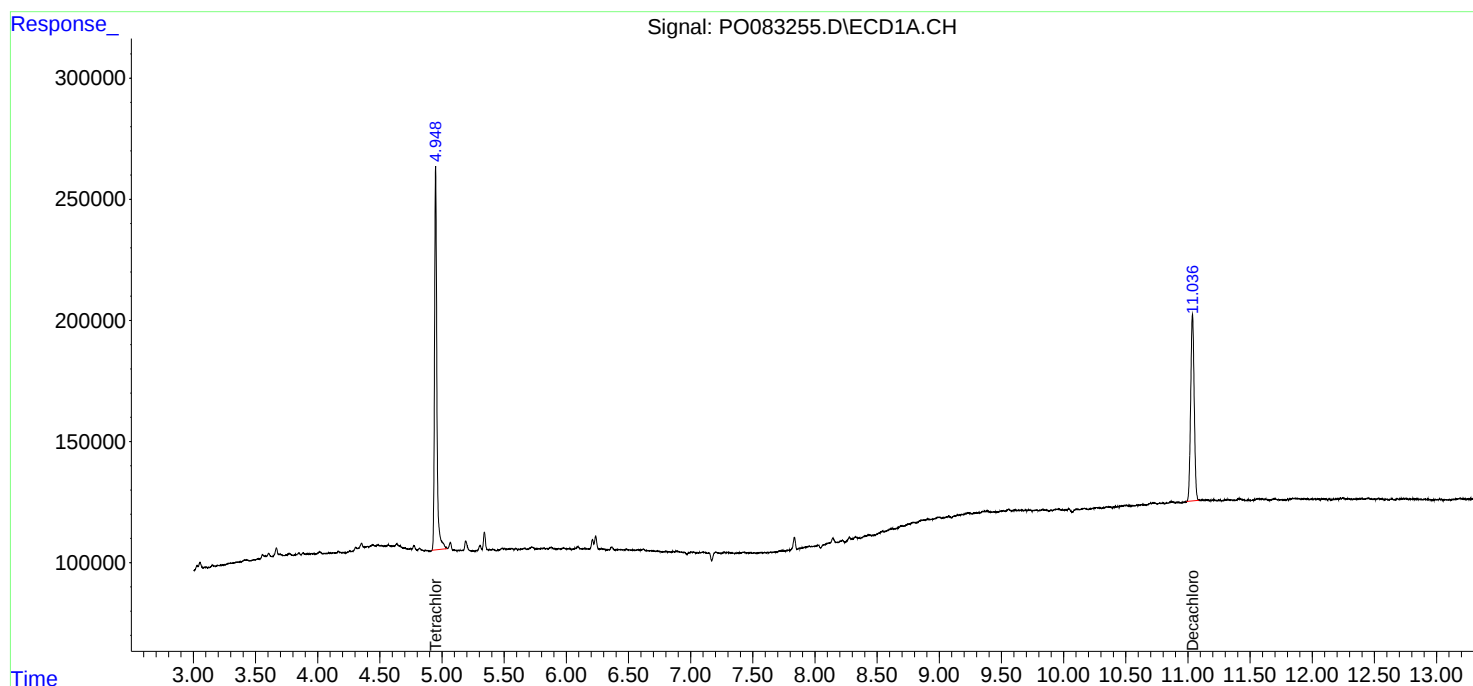


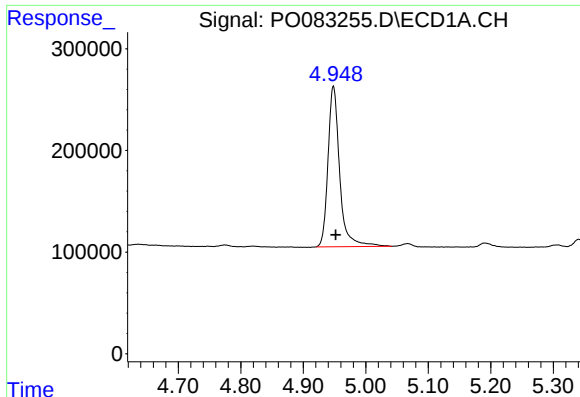

#1 Tetrachloro-m-xylene


R.T.: 4.948 min
Delta R.T.: -0.004 min
Response: 2051450
Conc: 23.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

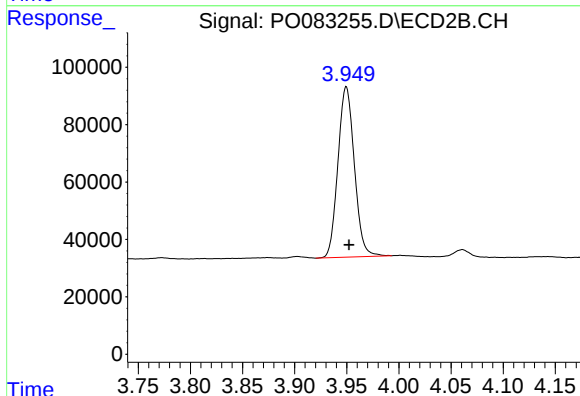


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: -0.002 min
Response: 651624
Conc: 21.38 ng/ml

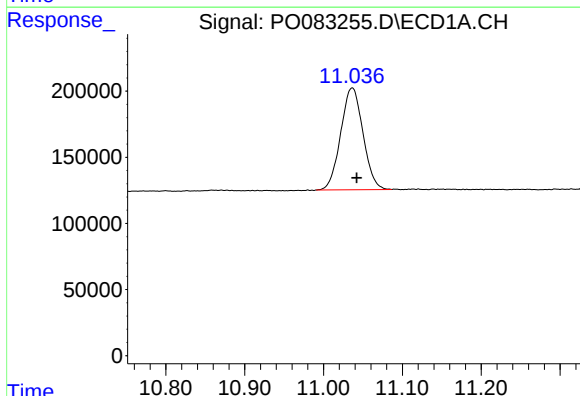

#2 Decachlorobiphenyl

R.T.: 11.037 min
Delta R.T.: -0.006 min
Response: 1513121
Conc: 23.01 ng/ml

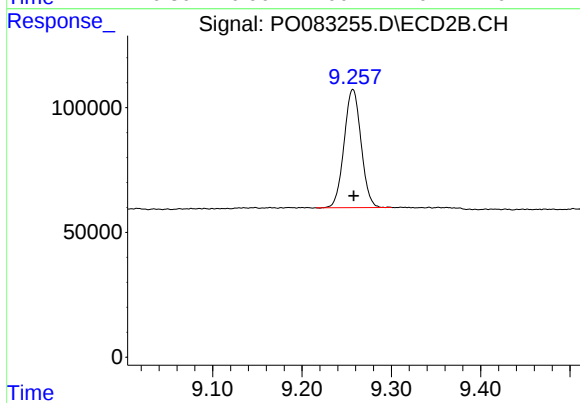

#2 Decachlorobiphenyl

R.T.: 9.257 min
Delta R.T.: 0.000 min
Response: 625084
Conc: 20.79 ng/ml