

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO113021\
 Data File : PO083283.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Dec 2021 4:04
 Operator : AJ\MA
 Sample : M4862-11
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CS-6B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 04:37:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Nov 20 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.947	3.949	1965481	644277	22.396	21.136
2)	SA Decachlor...	11.034	9.254	1484781	605409	22.580	20.139

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO113021\
Data File : PO083283.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Dec 2021 4:04
Operator : AJ\MA
Sample : M4862-11
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CS-6B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 04:37:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Nov 20 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

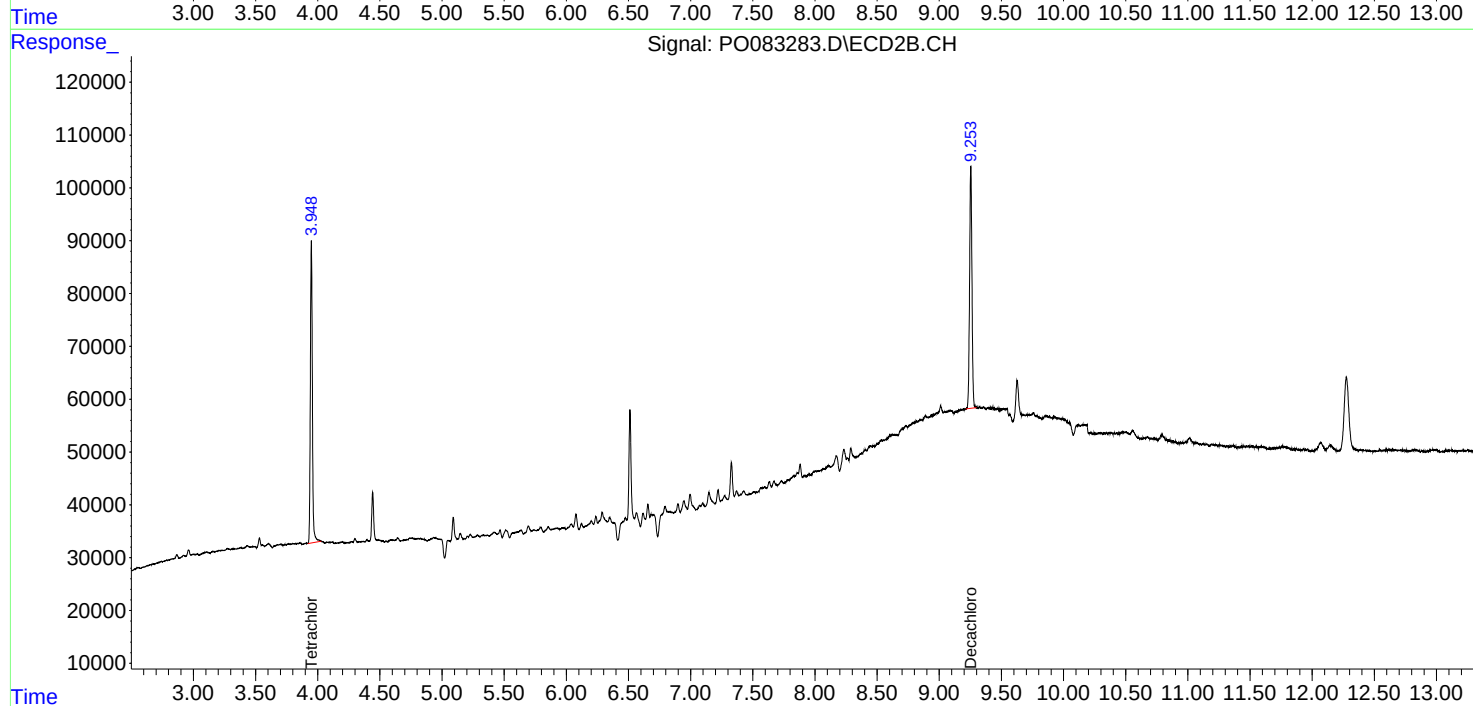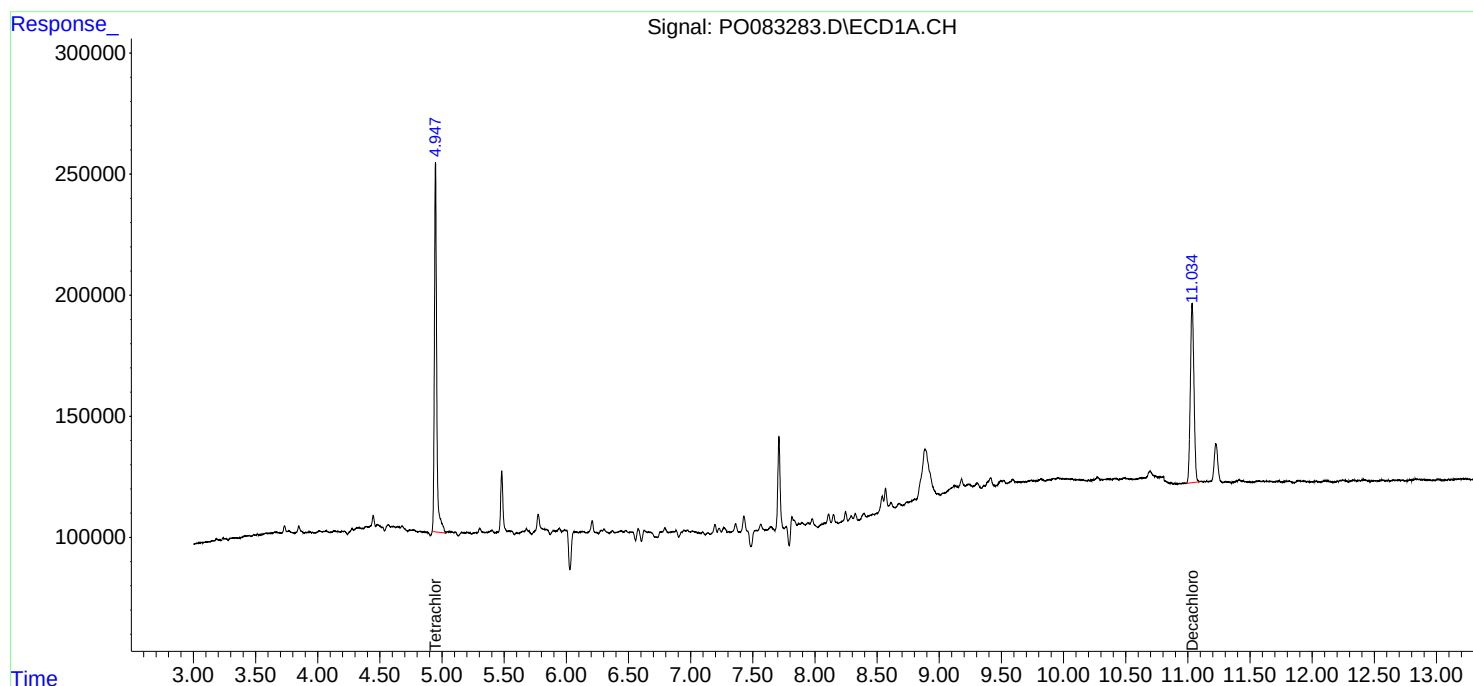


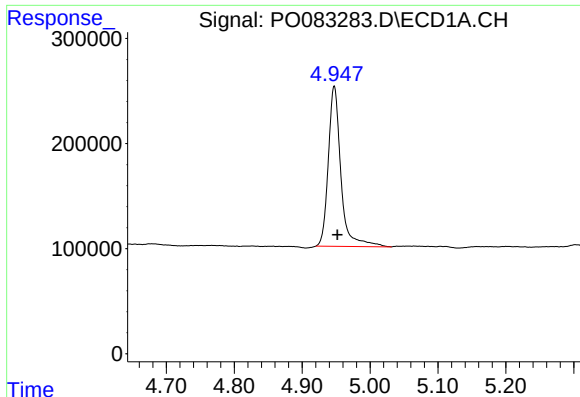

#1 Tetrachloro-m-xylene


R.T.: 4.947 min
Delta R.T.: -0.005 min
Response: 1965481
Conc: 22.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-6B

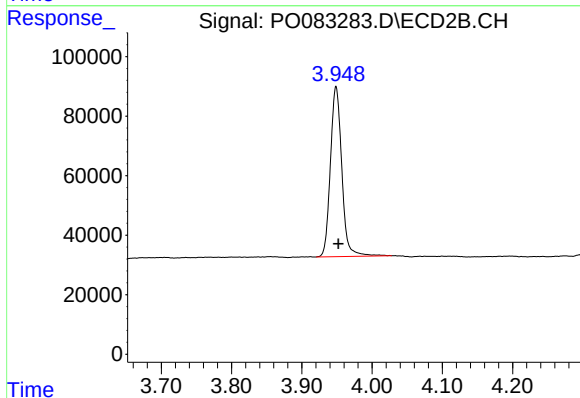


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: -0.003 min
Response: 644277
Conc: 21.14 ng/ml

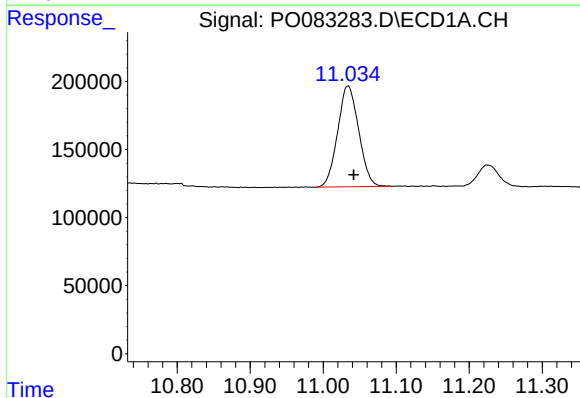

#2 Decachlorobiphenyl

R.T.: 11.034 min
Delta R.T.: -0.008 min
Response: 1484781
Conc: 22.58 ng/ml

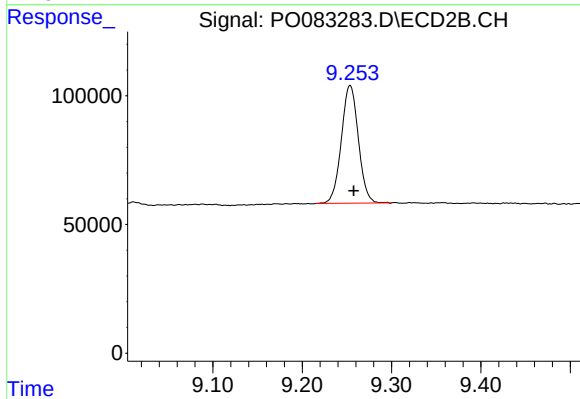

#2 Decachlorobiphenyl

R.T.: 9.254 min
Delta R.T.: -0.004 min
Response: 605409
Conc: 20.14 ng/ml