

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO113021\
 Data File : PO083285.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Dec 2021 4:38
 Operator : AJ\MA
 Sample : M4862-13
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CS-7B

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 12/01/2021
 Supervised By :mohammad ahmed 12/02/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 07:25:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Nov 20 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.947	3.949	2228972	731322	25.399m	23.992
2) SA Decachlor...	11.035	9.254	1666955	695493	25.351	23.136

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO113021\
Data File : PO083285.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Dec 2021 4:38
Operator : AJ\MA
Sample : M4862-13
Misc :
ALS Vial : 54 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CS-7B


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/01/2021
Supervised By :mohammad ahmed 12/02/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 07:25:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Nov 20 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

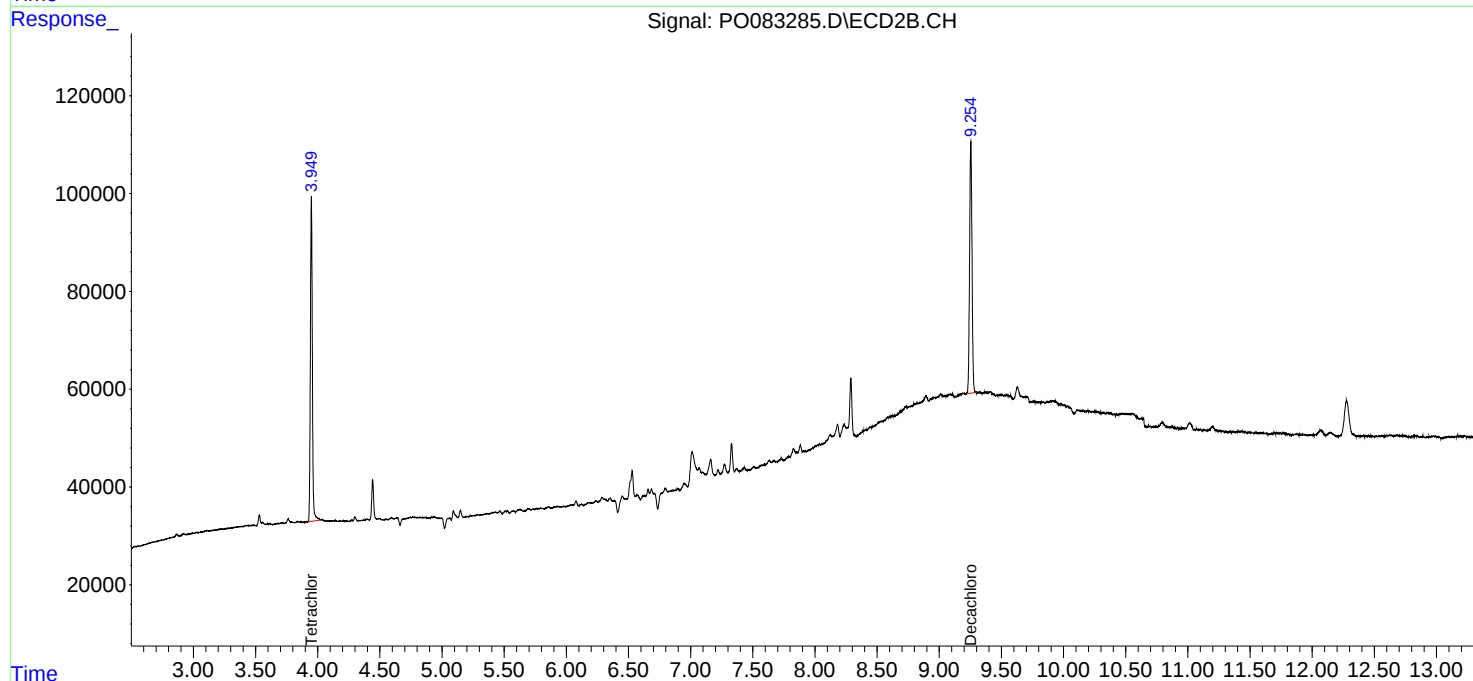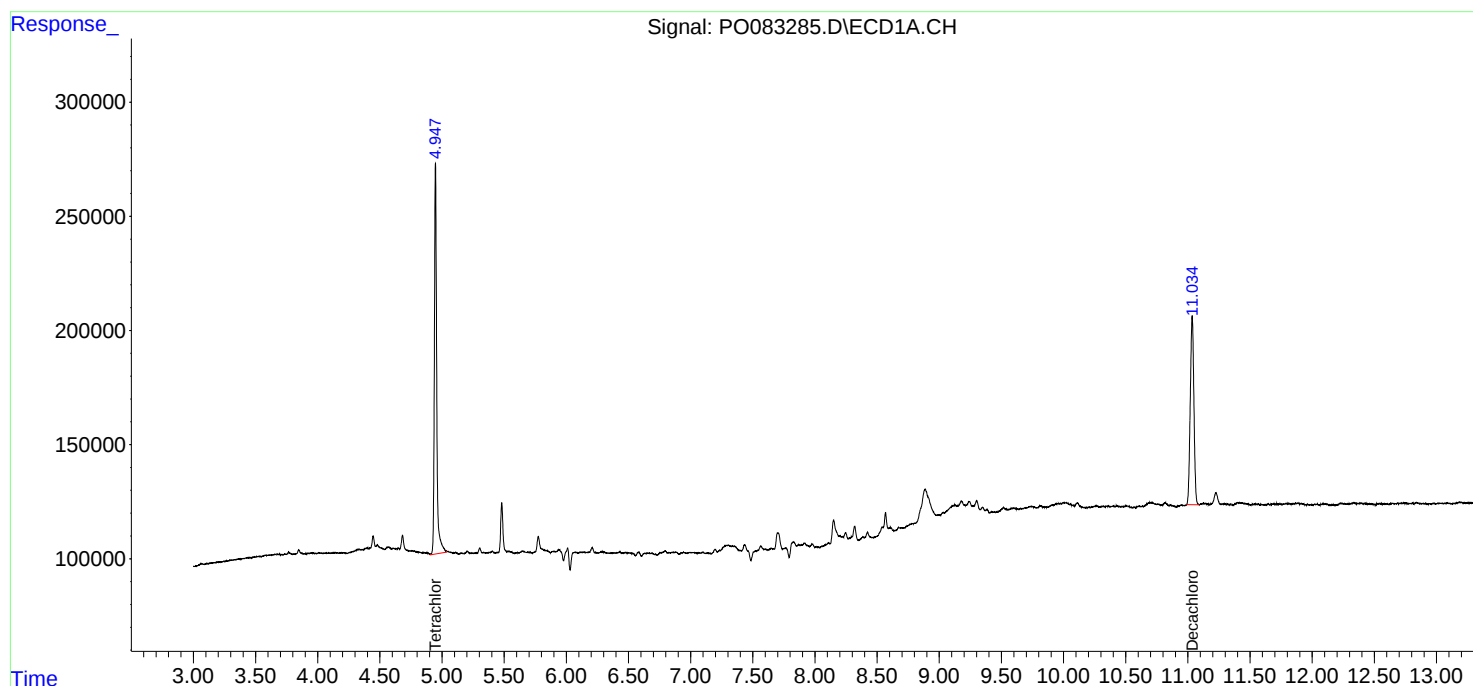

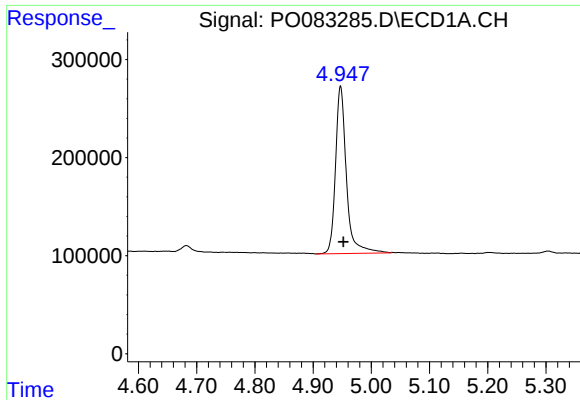


#1 Tetrachloro-m-xylene

R.T.: 4.947 min
Delta R.T.: -0.005 min
Response: 2228972
Conc: 25.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-7B


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/01/2021
Supervised By :mohammad ahmed 12/02/2021

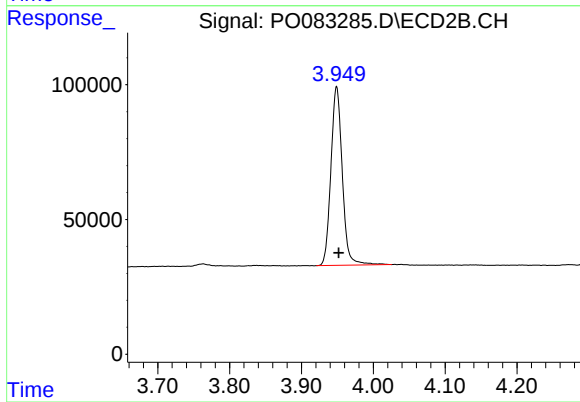


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: -0.003 min
Response: 731322
Conc: 23.99 ng/ml

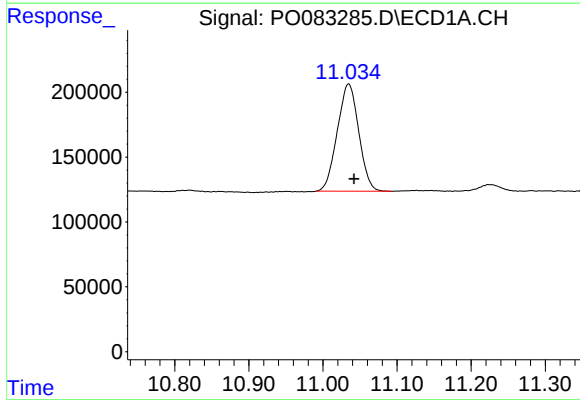

#2 Decachlorobiphenyl

R.T.: 11.035 min
Delta R.T.: -0.007 min
Response: 1666955
Conc: 25.35 ng/ml

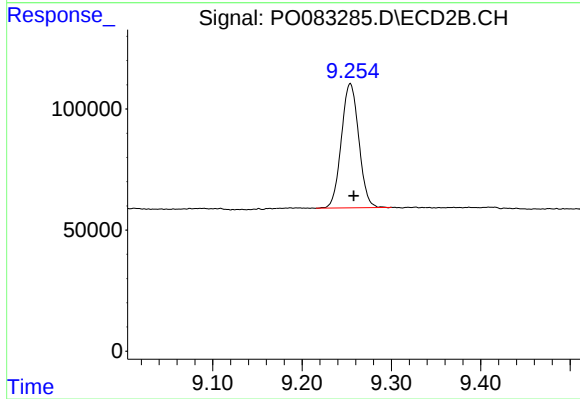

#2 Decachlorobiphenyl

R.T.: 9.254 min
Delta R.T.: -0.004 min
Response: 695493
Conc: 23.14 ng/ml