

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO113021\
 Data File : PO083296.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Dec 2021 8:23
 Operator : AJ\MA
 Sample : M4850-09 10X
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SEC-2021-57B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 13:03:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Nov 20 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.947	3.949	93503	37401	1.065	1.227
2)	SA Decachlor...	11.033	9.253	103337	48272	1.572	1.606

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO113021\
Data File : PO083296.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Dec 2021 8:23
Operator : AJ\MA
Sample : M4850-09 10X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SEC-2021-57B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 13:03:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Nov 20 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

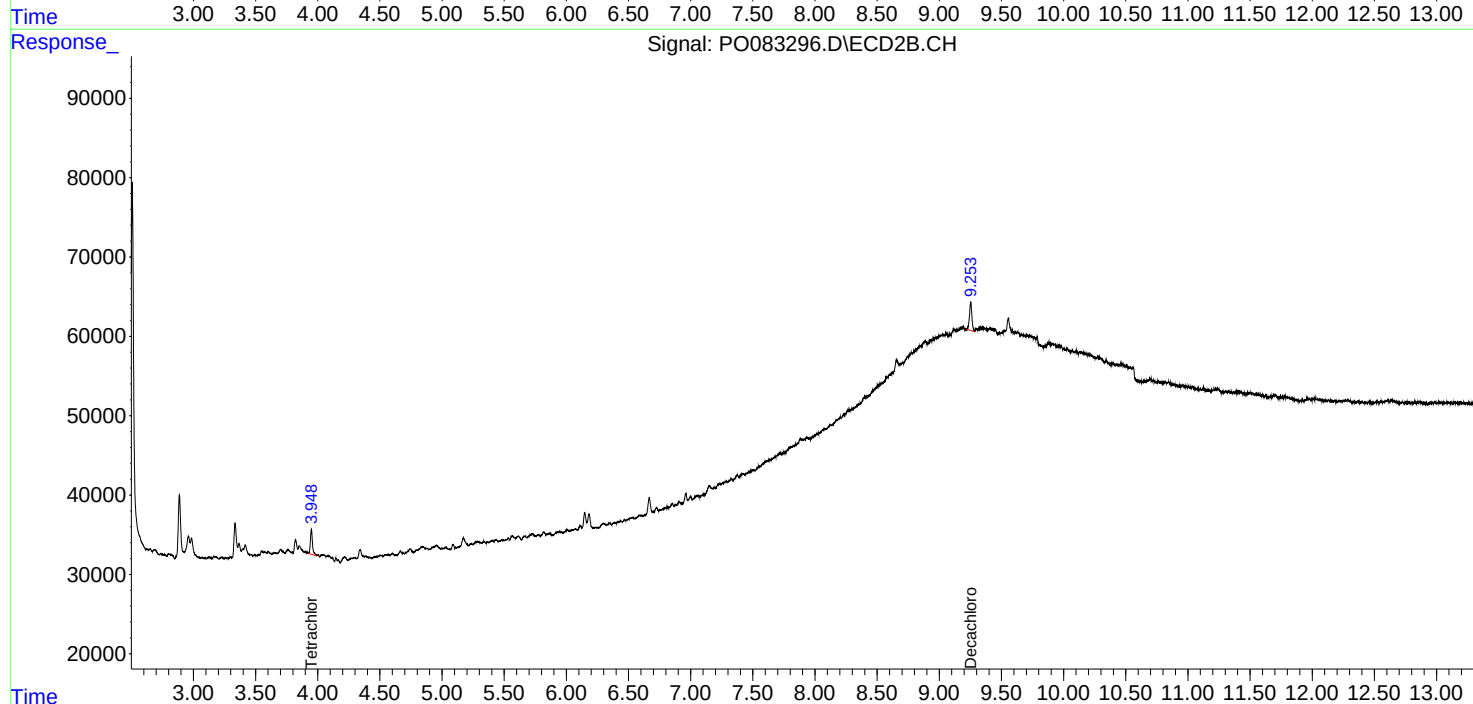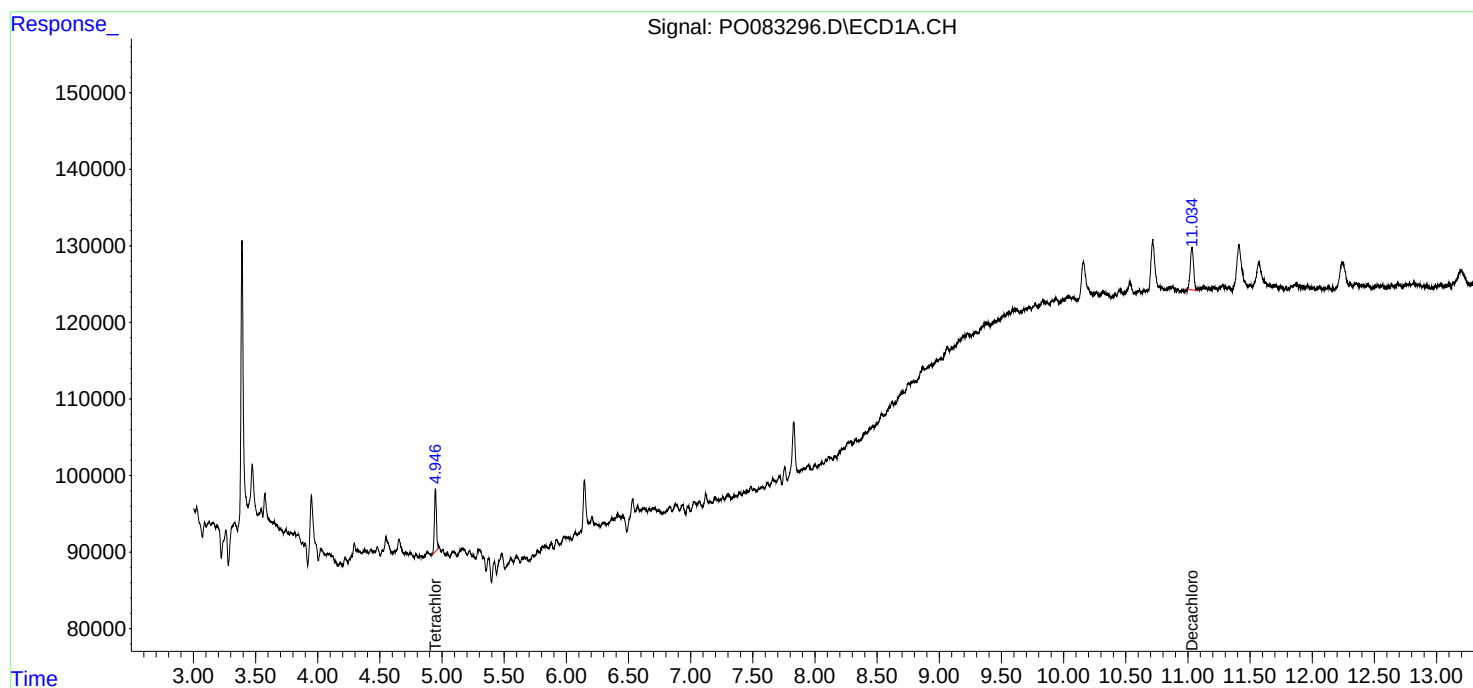


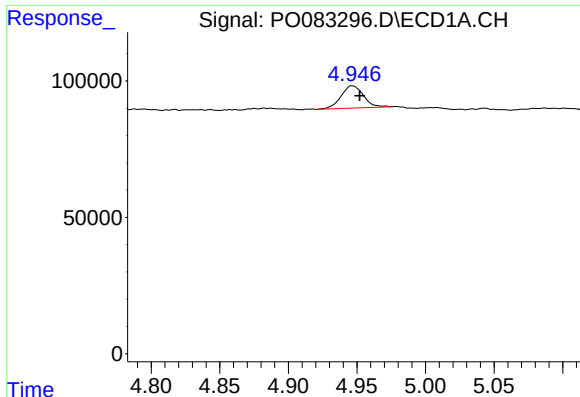

#1 Tetrachloro-m-xylene


R.T.: 4.947 min
Delta R.T.: -0.005 min
Response: 93503
Conc: 1.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-57B

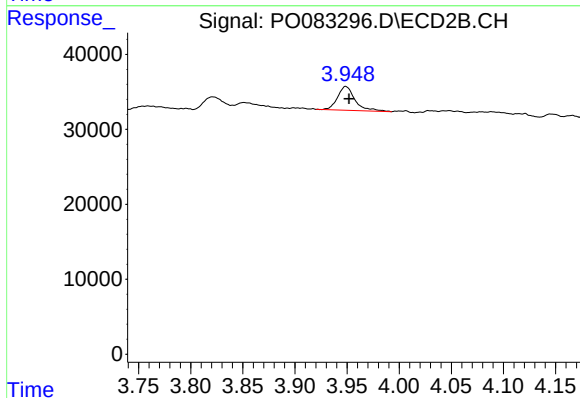


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: -0.003 min
Response: 37401
Conc: 1.23 ng/ml

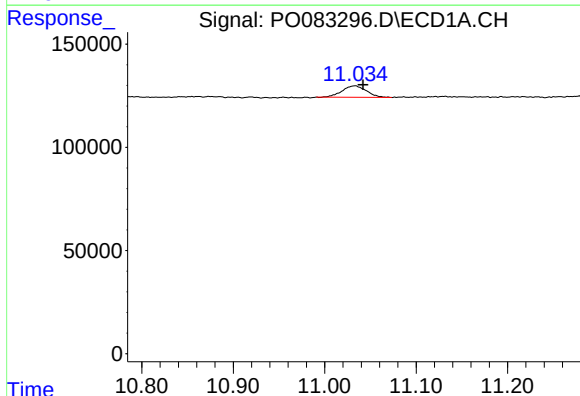

#2 Decachlorobiphenyl

R.T.: 11.033 min
Delta R.T.: -0.009 min
Response: 103337
Conc: 1.57 ng/ml

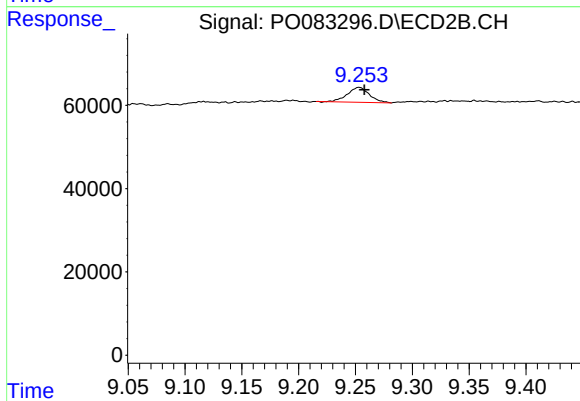

#2 Decachlorobiphenyl

R.T.: 9.253 min
Delta R.T.: -0.005 min
Response: 48272
Conc: 1.61 ng/ml