

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO113023\
 Data File : PO100180.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2023 17:19
 Operator : YP/AJ
 Sample : 05578-03 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC271332-LOZ-END-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/01/2023
 Supervised By :Ankita Jodhani 12/01/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 21:43:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 21 15:58:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.478	3.702	2904881	2659473	1.702	1.773m
2) SA Decachlor...	10.357	8.797	2035150	2126729	2.802m	1.901m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO113023\
Data File : PO100180.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2023 17:19
Operator : YP/AJ
Sample : 05578-03 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC271332-LOZ-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/01/2023
Supervised By :Ankita Jodhani 12/01/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 21:43:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 21 15:58:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

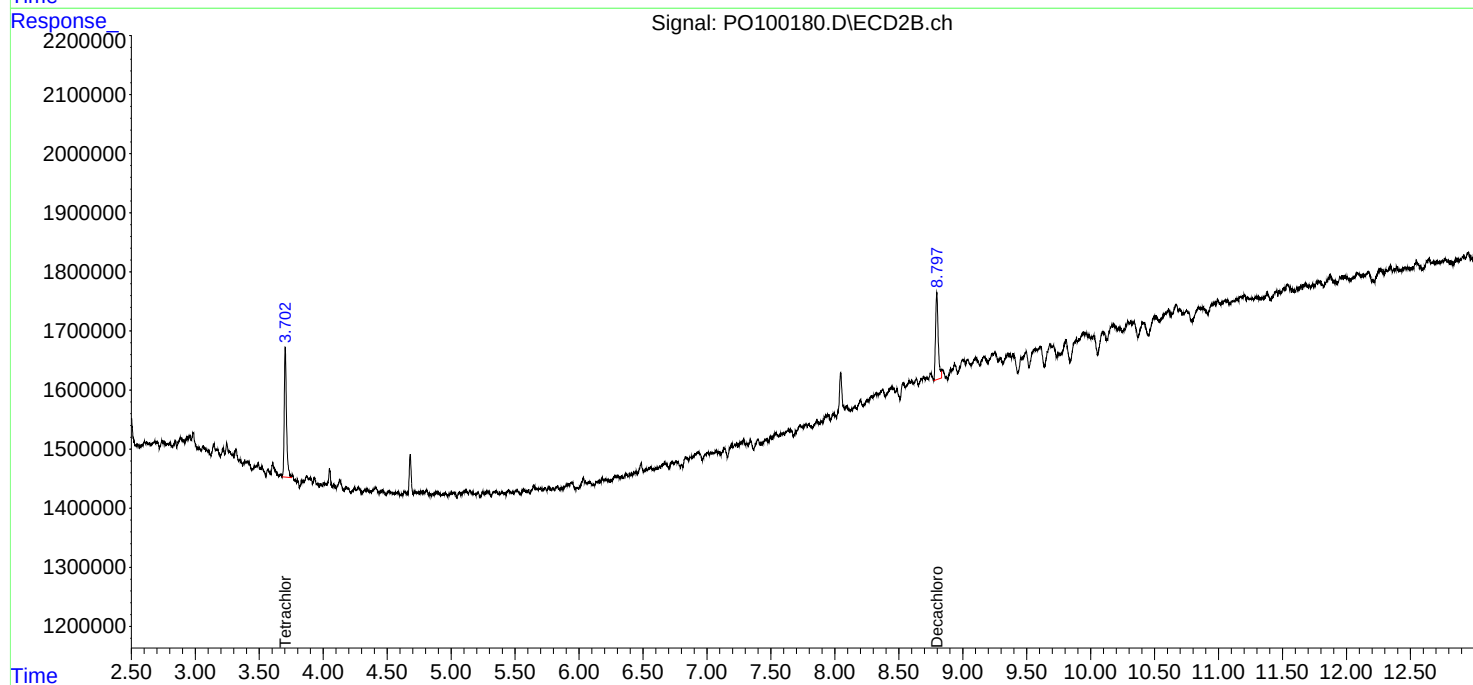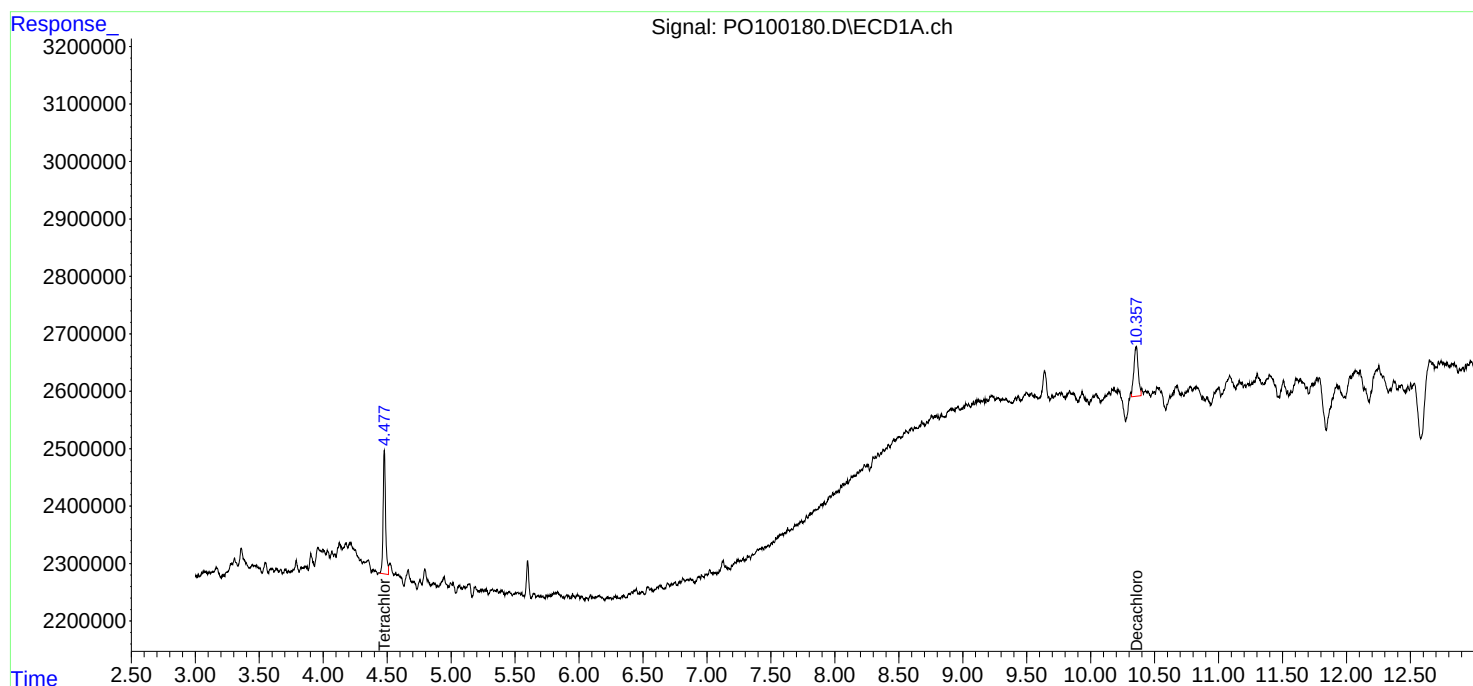

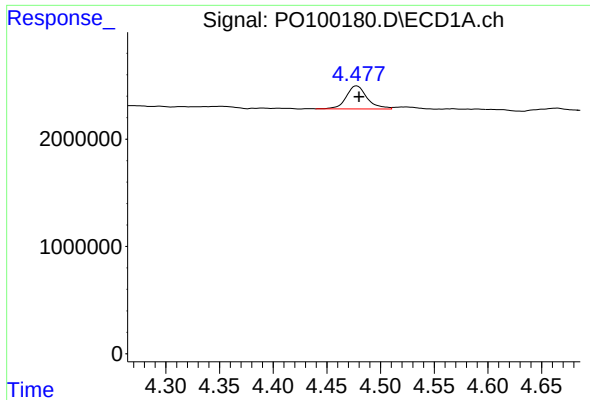


#1 Tetrachloro-m-xylene

R.T.: 4.478 min
Delta R.T.: -0.002 min
Response: 2904881
Conc: 1.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC271332-LOZ-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/01/2023
Supervised By :Ankita Jodhani 12/01/2023

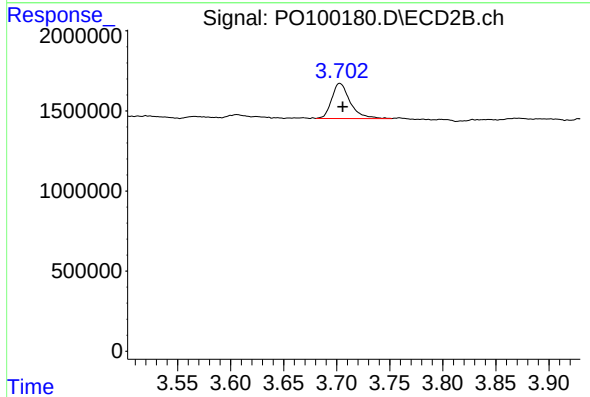


#1 Tetrachloro-m-xylene

R.T.: 3.702 min
Delta R.T.: -0.003 min
Response: 2659473
Conc: 1.77 ng/ml m

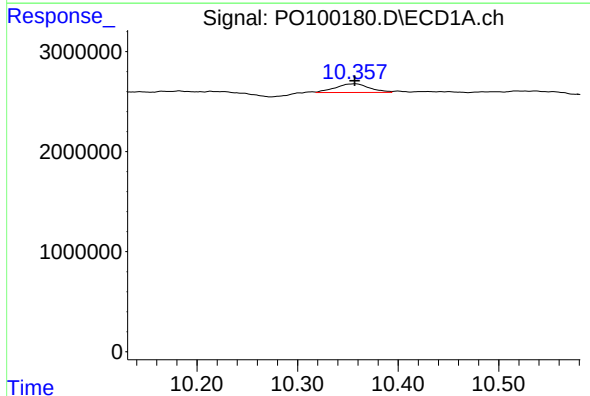

#2 Decachlorobiphenyl

R.T.: 10.357 min
Delta R.T.: 0.000 min
Response: 2035150
Conc: 2.80 ng/ml m

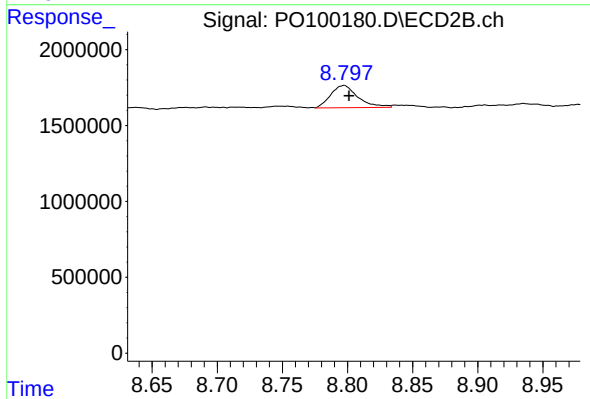

#2 Decachlorobiphenyl

R.T.: 8.797 min
Delta R.T.: -0.004 min
Response: 2126729
Conc: 1.90 ng/ml m