

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO113023\
 Data File : PO100197.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2023 22:49
 Operator : YP/AJ
 Sample : 05576-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TR-04-112923

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/01/2023
 Supervised By :Ankita Jodhani 12/01/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 03:17:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 21 15:58:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.477	3.703	29445882	26009376	17.252m	17.341m
2) SA Decachlor...	10.355	8.794	18159735	26010376	25.001	23.244

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO113023\
Data File : PO100197.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2023 22:49
Operator : YP/AJ
Sample : 05576-01
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TR-04-112923


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/01/2023
Supervised By :Ankita Jodhani 12/01/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 03:17:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 21 15:58:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

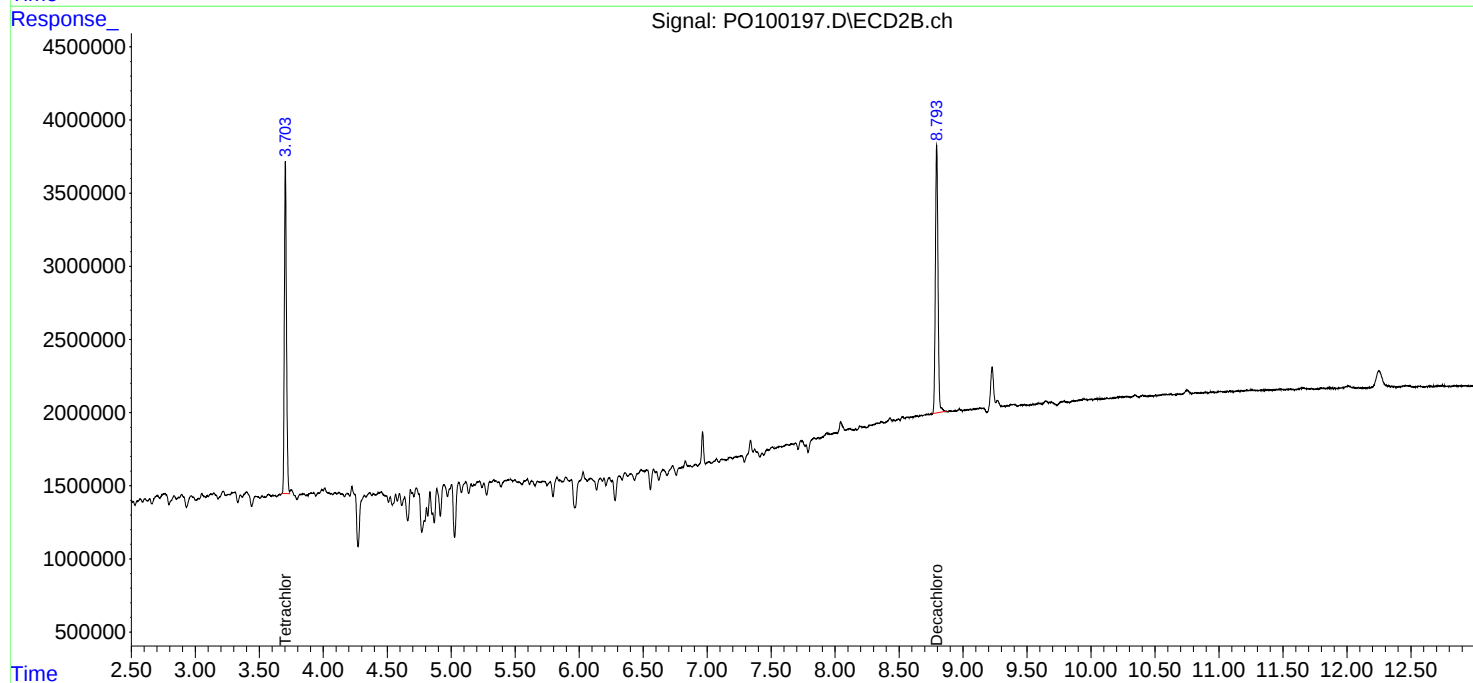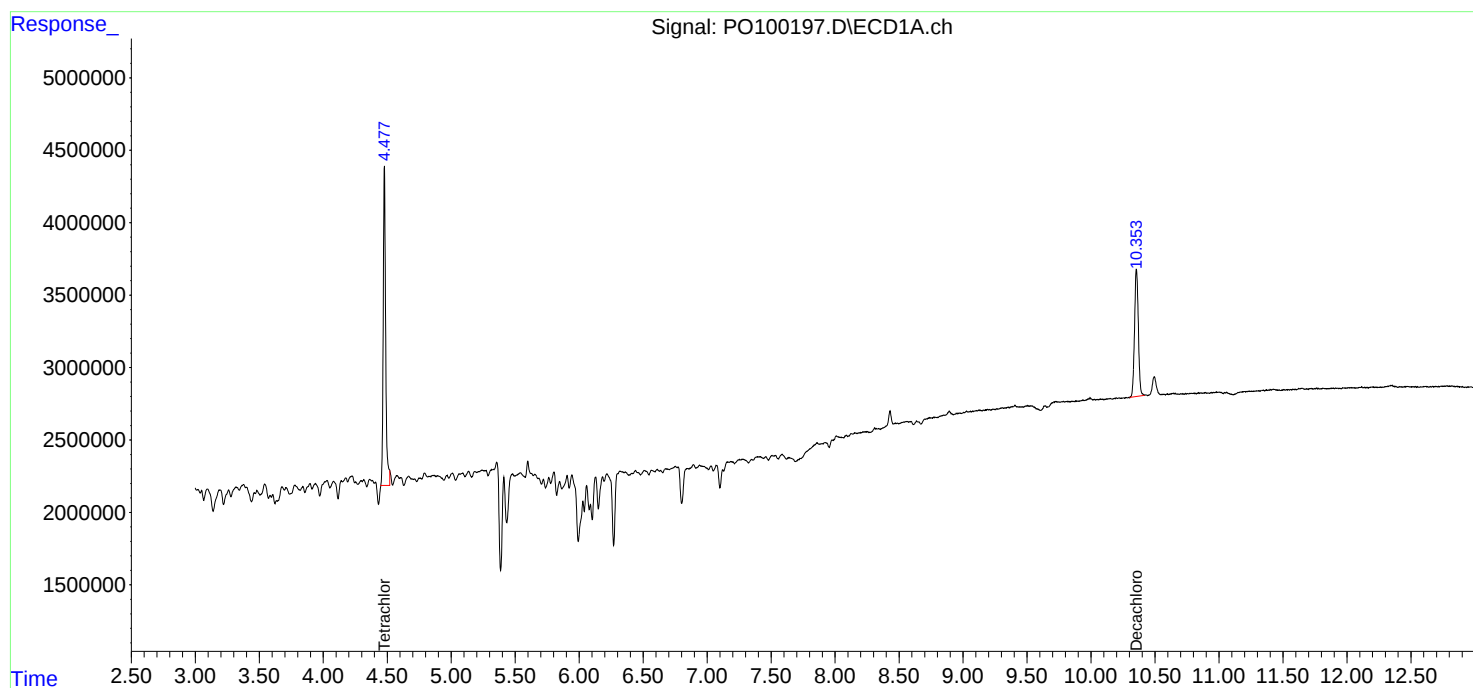

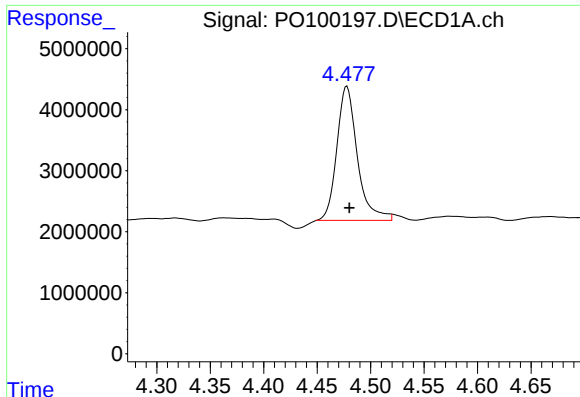


#1 Tetrachloro-m-xylene

R.T.: 4.477 min
Delta R.T.: -0.003 min
Response: 29445882
Conc: 17.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
TR-04-112923


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/01/2023
Supervised By :Ankita Jodhani 12/01/2023

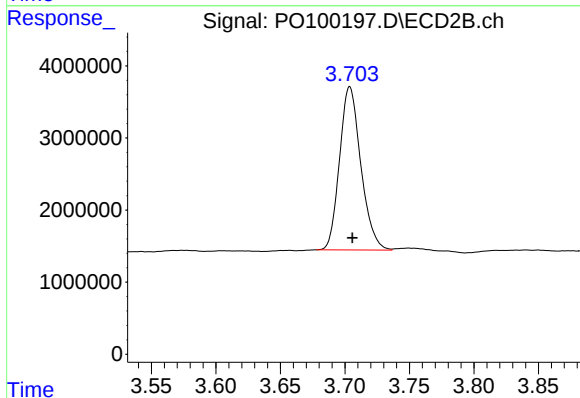


#1 Tetrachloro-m-xylene

R.T.: 3.703 min
Delta R.T.: -0.002 min
Response: 26009376
Conc: 17.34 ng/ml m

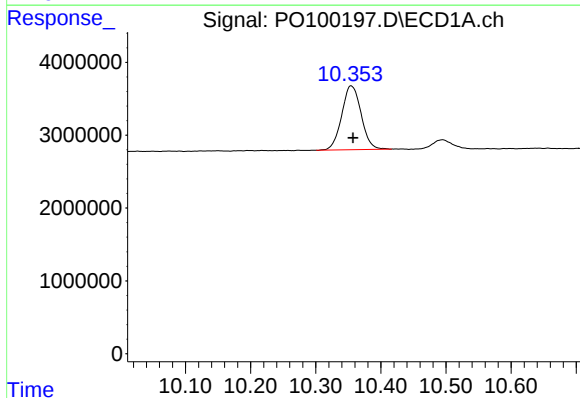

#2 Decachlorobiphenyl

R.T.: 10.355 min
Delta R.T.: -0.002 min
Response: 18159735
Conc: 25.00 ng/ml

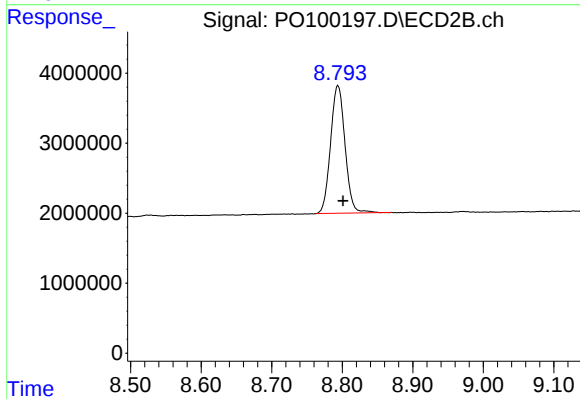

#2 Decachlorobiphenyl

R.T.: 8.794 min
Delta R.T.: -0.007 min
Response: 26010376
Conc: 23.24 ng/ml