

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO113023\
 Data File : PO100198.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2023 23:06
 Operator : YP/AJ
 Sample : 05577-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EO-03-112923

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/01/2023
 Supervised By :Ankita Jodhani 12/01/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 03:18:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 21 15:58:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.477	3.704	17889142	17434780	10.481m	11.624
2) SA Decachlor...	10.354	8.795	11158187	15111936	15.362	13.505

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO113023\
Data File : PO100198.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2023 23:06
Operator : YP/AJ
Sample : 05577-01
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
EO-03-112923


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/01/2023
Supervised By :Ankita Jodhani 12/01/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 03:18:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 21 15:58:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

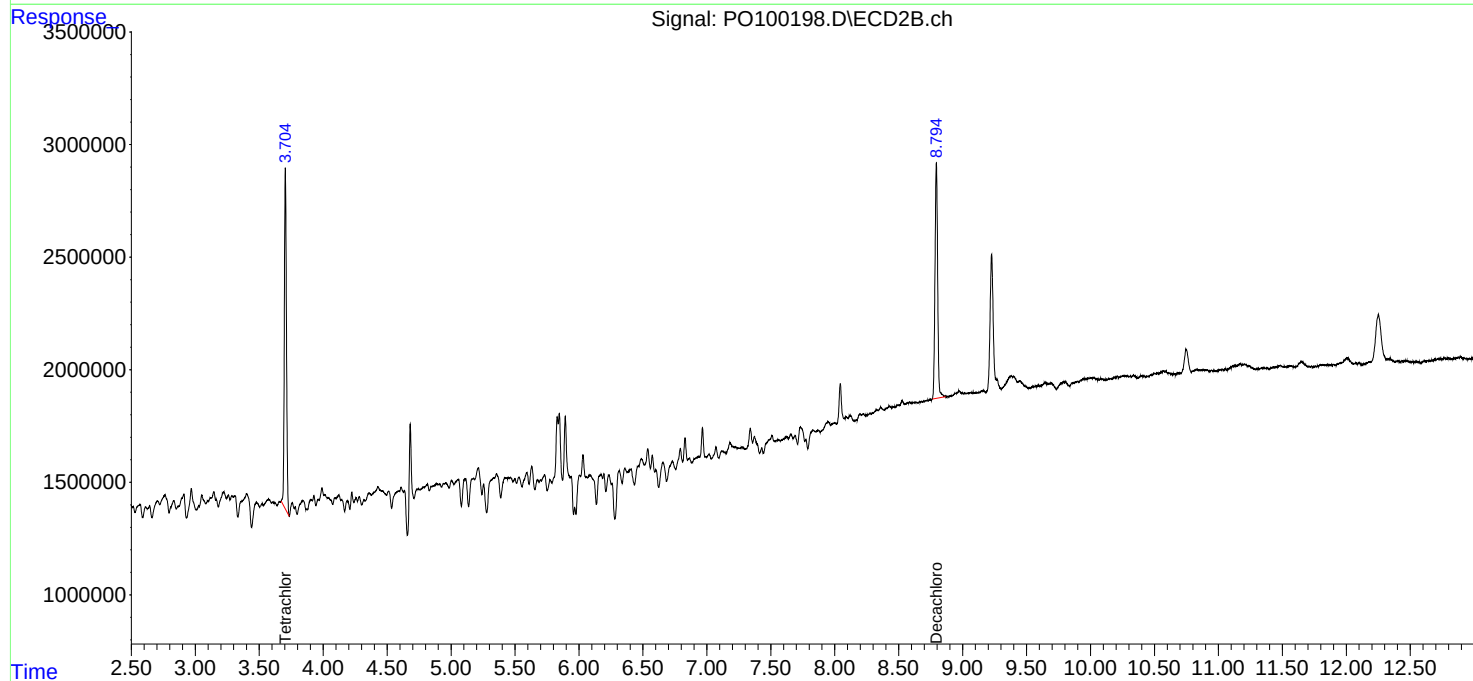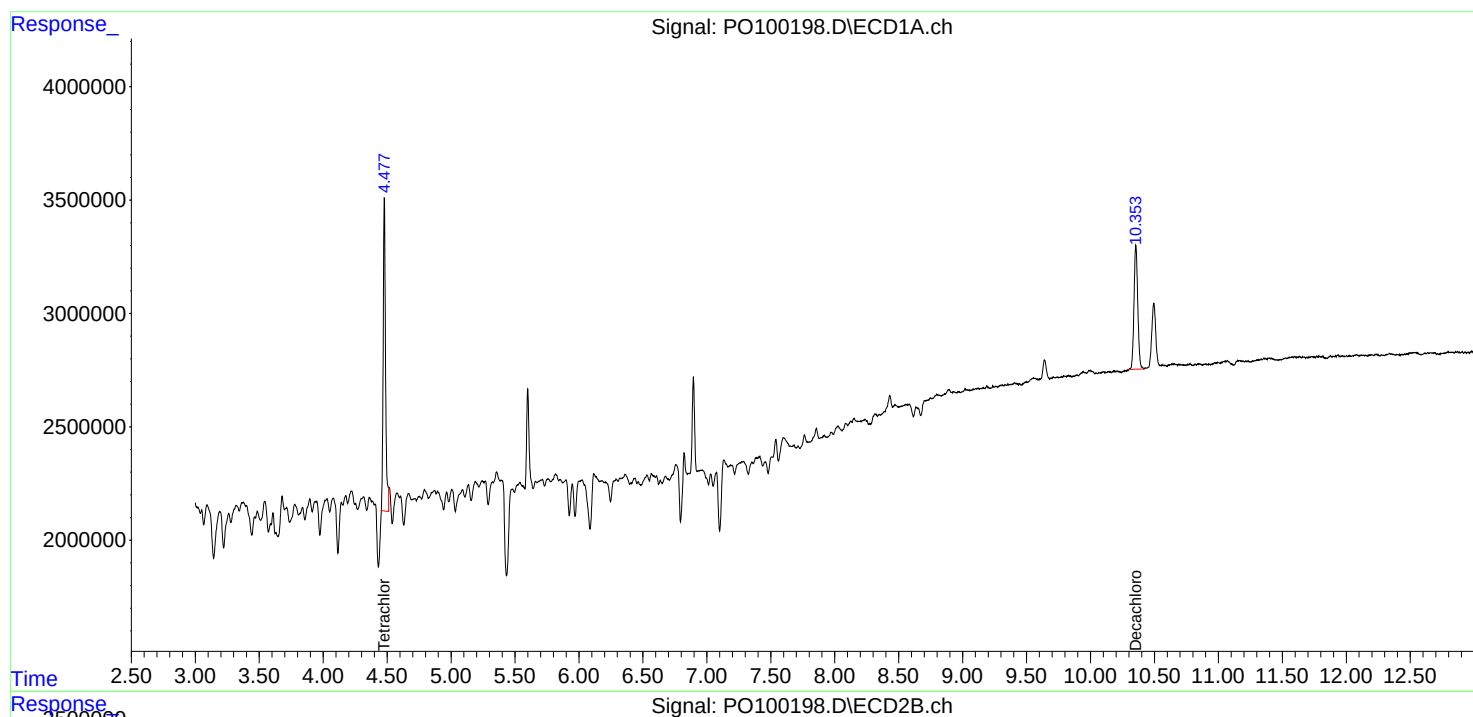

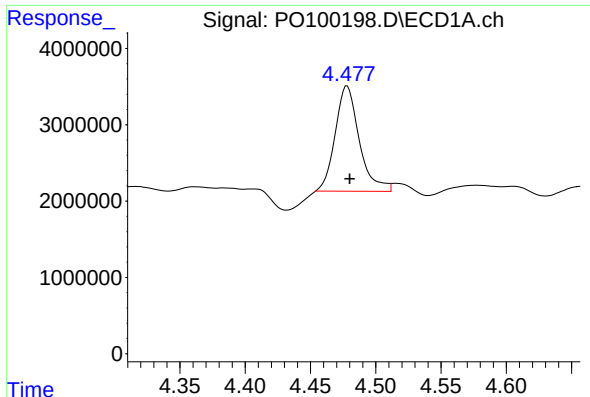


#1 Tetrachloro-m-xylene

R.T.: 4.477 min
Delta R.T.: -0.003 min
Response: 17889142
Conc: 10.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
EO-03-112923


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/01/2023
Supervised By :Ankita Jodhani 12/01/2023

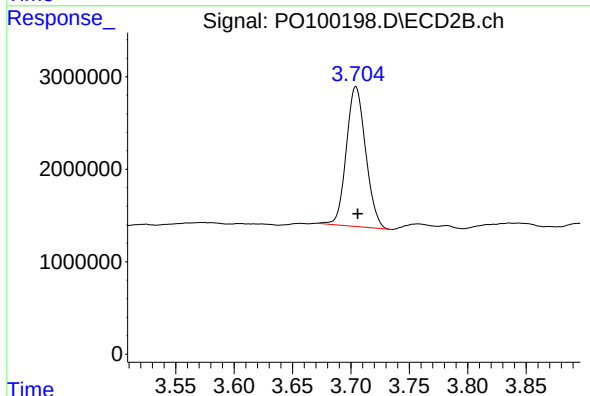


#1 Tetrachloro-m-xylene

R.T.: 3.704 min
Delta R.T.: -0.002 min
Response: 17434780
Conc: 11.62 ng/ml

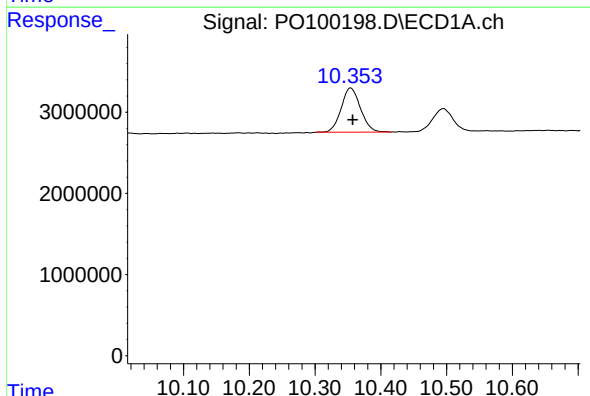

#2 Decachlorobiphenyl

R.T.: 10.354 min
Delta R.T.: -0.003 min
Response: 11158187
Conc: 15.36 ng/ml

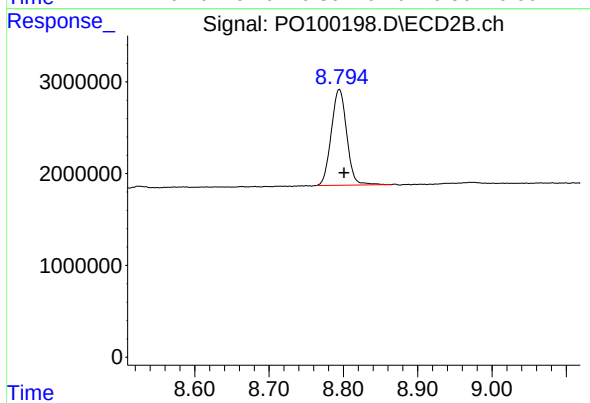

#2 Decachlorobiphenyl

R.T.: 8.795 min
Delta R.T.: -0.007 min
Response: 15111936
Conc: 13.50 ng/ml