

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO113023\
 Data File : PO100199.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2023 23:23
 Operator : YP/AJ
 Sample : 05579-05
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 3330

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/01/2023
 Supervised By :Ankita Jodhani 12/01/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 03:18:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 21 15:58:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.485	3.713	25023511	17721763	14.661	11.815m
2) SA Decachlor...	10.355	8.795	19687411	23820394	27.105	21.287

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO113023\
Data File : PO100199.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2023 23:23
Operator : YP/AJ
Sample : 05579-05
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
3330


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/01/2023
Supervised By :Ankita Jodhani 12/01/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 03:18:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 21 15:58:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

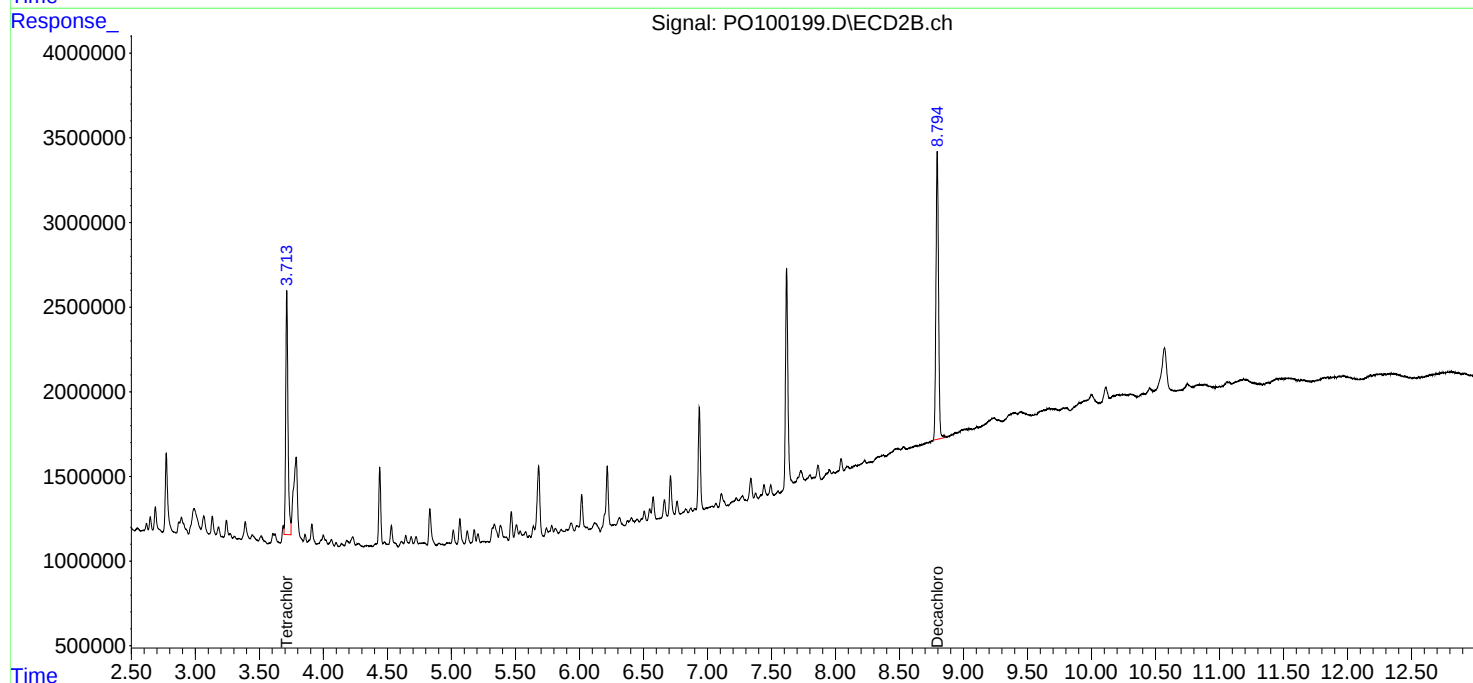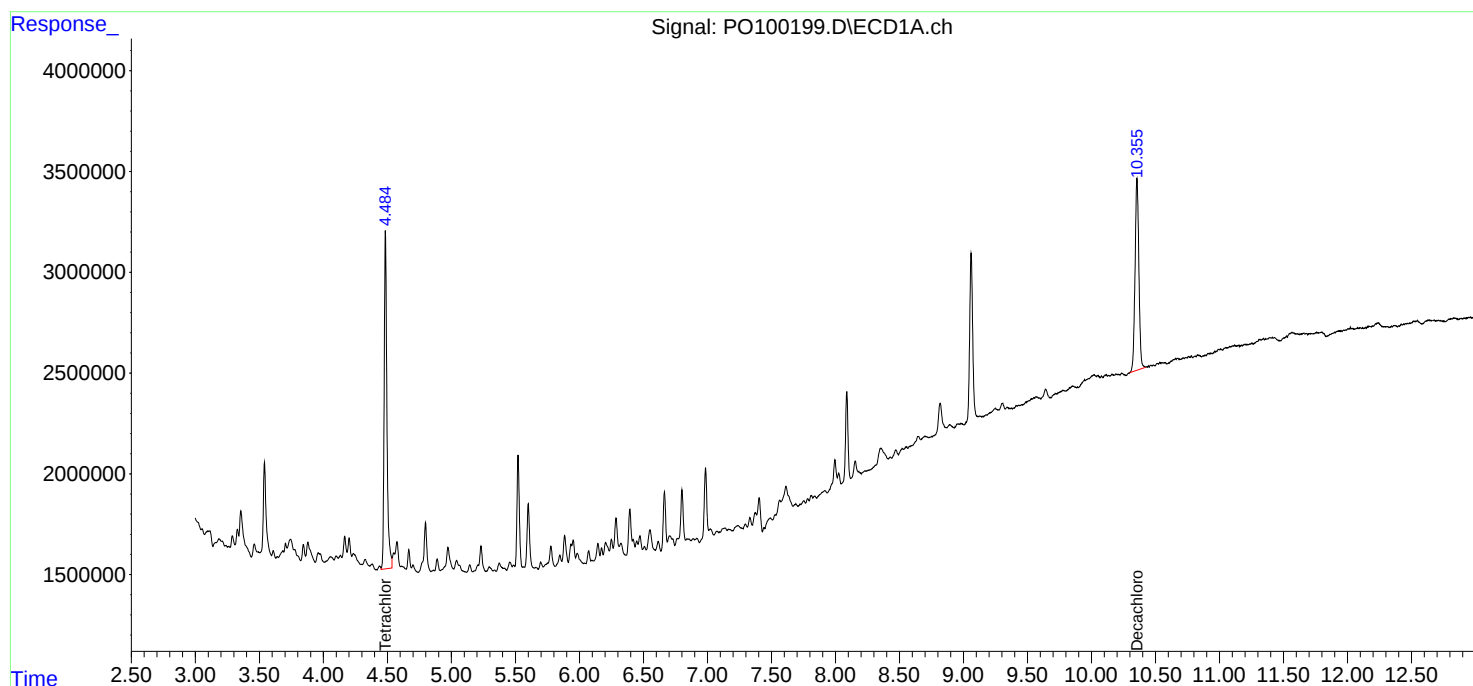

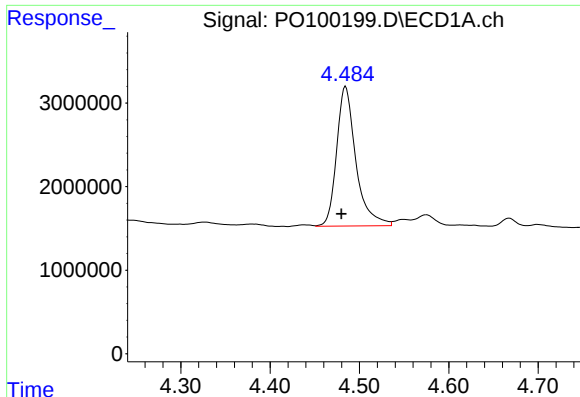


#1 Tetrachloro-m-xylene

R.T.: 4.485 min
Delta R.T.: 0.005 min
Response: 25023511
Conc: 14.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
3330


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/01/2023
Supervised By :Ankita Jodhani 12/01/2023

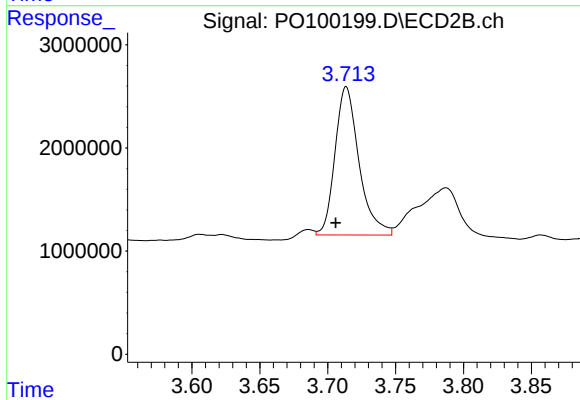


#1 Tetrachloro-m-xylene

R.T.: 3.713 min
Delta R.T.: 0.007 min
Response: 17721763
Conc: 11.82 ng/ml m

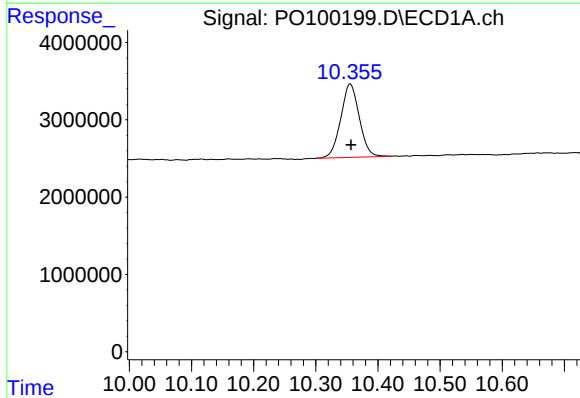

#2 Decachlorobiphenyl

R.T.: 10.355 min
Delta R.T.: -0.002 min
Response: 19687411
Conc: 27.10 ng/ml

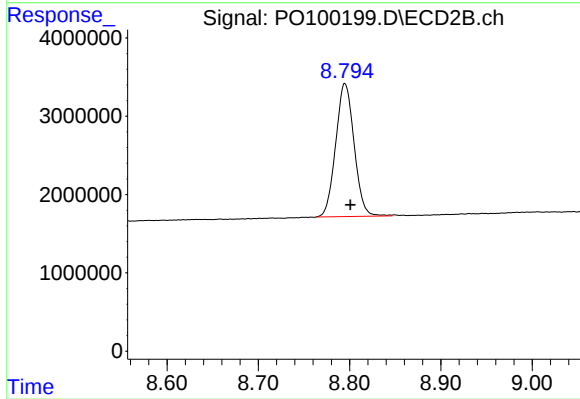

#2 Decachlorobiphenyl

R.T.: 8.795 min
Delta R.T.: -0.006 min
Response: 23820394
Conc: 21.29 ng/ml