

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO120121\  
Data File : PO083322.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 01 Dec 2021 16:32  
Operator : AJ\MA  
Sample : M4068-08  
Misc : AR1254 LOQ 50 PPB  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
LOQ-WATER-02-QT4-2021

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 01 23:53:03 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO111921.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Sat Nov 20 02:49:51 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

-----  
System Monitoring Compounds

Target Compounds  
-----


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO120121\  
Data File : P0083322.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 01 Dec 2021 16:32  
Operator : AJ\MA  
Sample : M4068-08  
Misc : AR1254 LOQ 50 PPB  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
LOQ-WATER-02-QT4-2021

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 01 23:53:03 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO111921.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Sat Nov 20 02:49:51 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

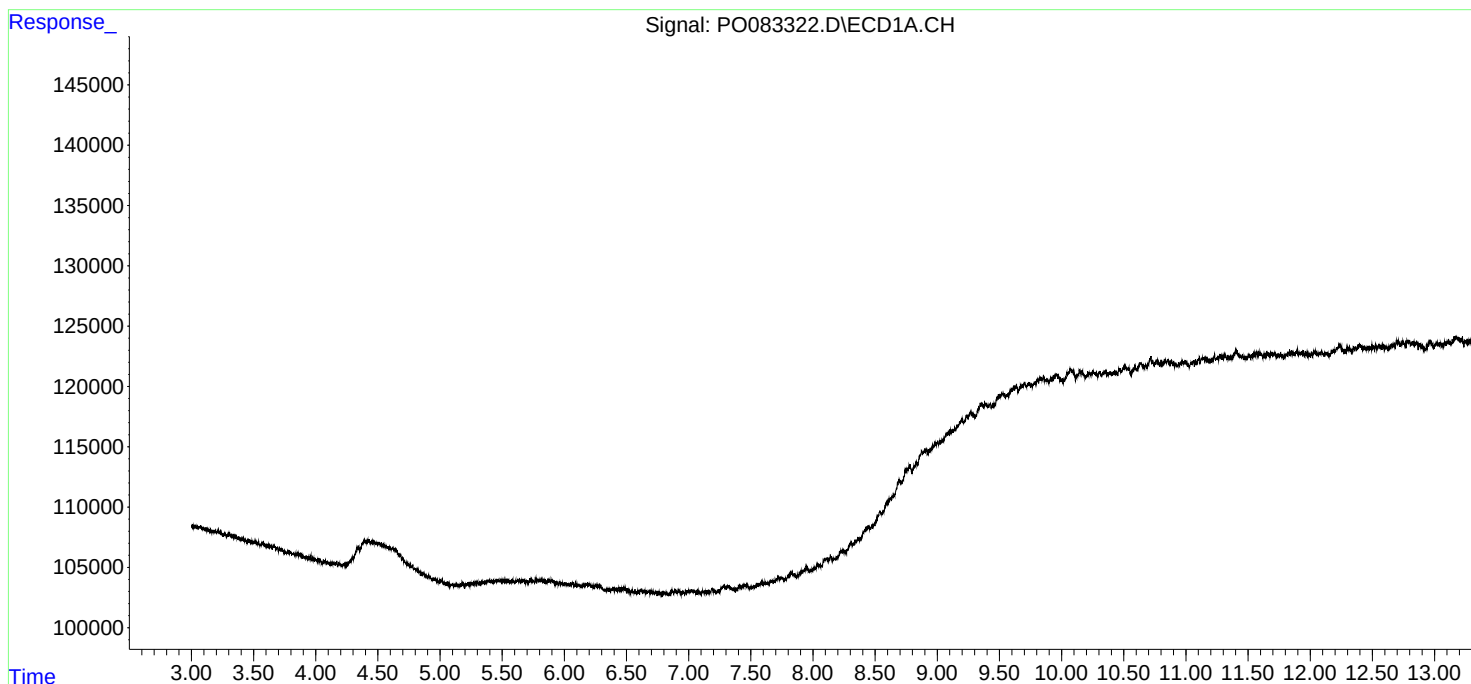


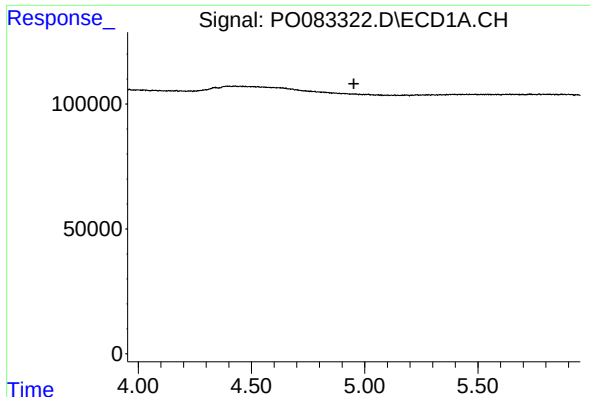

#1 Tetrachloro-m-xylene


R.T.: 0.000 min  
Exp R.T. : 4.952 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_O  
ClientSampleId :  
LOQ-WATER-02-QT4-2021

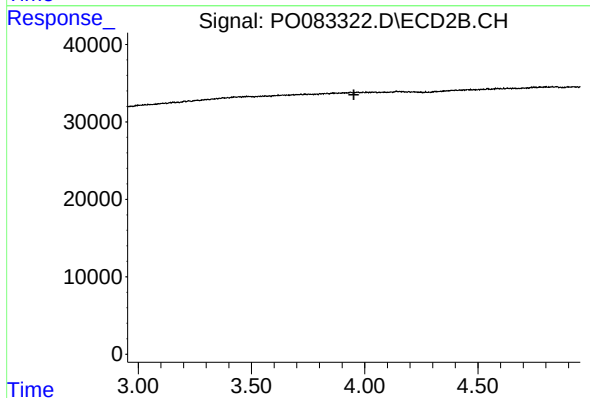


#1 Tetrachloro-m-xylene

R.T.: 0.000 min  
Exp R.T. : 3.952 min  
Response: 0  
Conc: N.D.

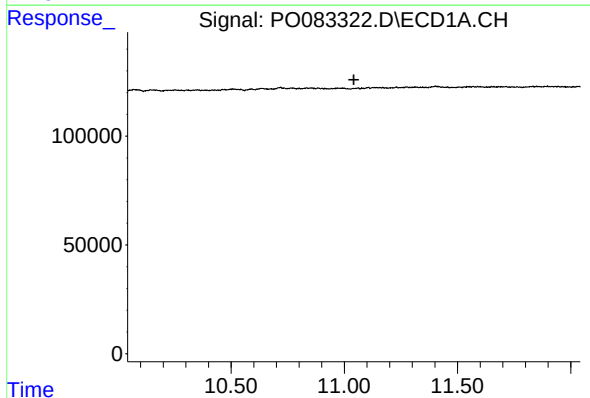

#2 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 11.042 min  
Response: 0  
Conc: N.D.

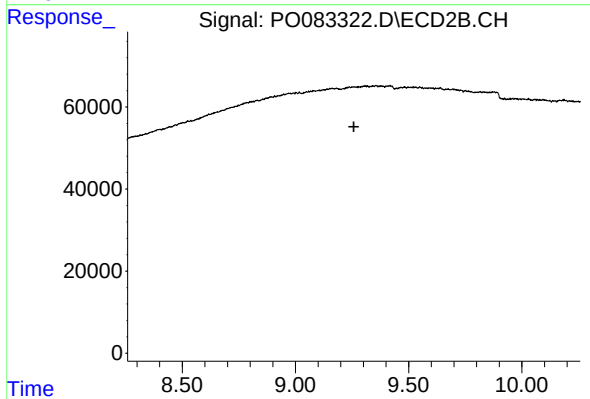

#2 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 9.258 min  
Response: 0  
Conc: N.D.