

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120121\
 Data File : PO083342.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Dec 2021 22:16
 Operator : AJ\MA
 Sample : M4068-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT4-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 00:00:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Nov 20 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.945	3.948	1848144	640274	21.059	21.005
2) SA Decachlor...	11.029	9.251	1506391	672591	22.909	22.374
Target Compounds						
26) L6 AR-1254-1	7.193	6.076	70231	45767	25.236	23.537
27) L6 AR-1254-2	7.425	6.236	111002	41317	26.682	24.556
28) L6 AR-1254-3	7.810	6.656	125223	57680	29.155	22.562
29) L6 AR-1254-4	8.107	6.897	78771	49836	25.466	27.318
30) L6 AR-1254-5	8.539	7.327	71998	47359	22.458	20.352



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120121\
Data File : P0083342.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Dec 2021 22:16
Operator : AJ\MA
Sample : M4068-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 00:00:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Nov 20 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

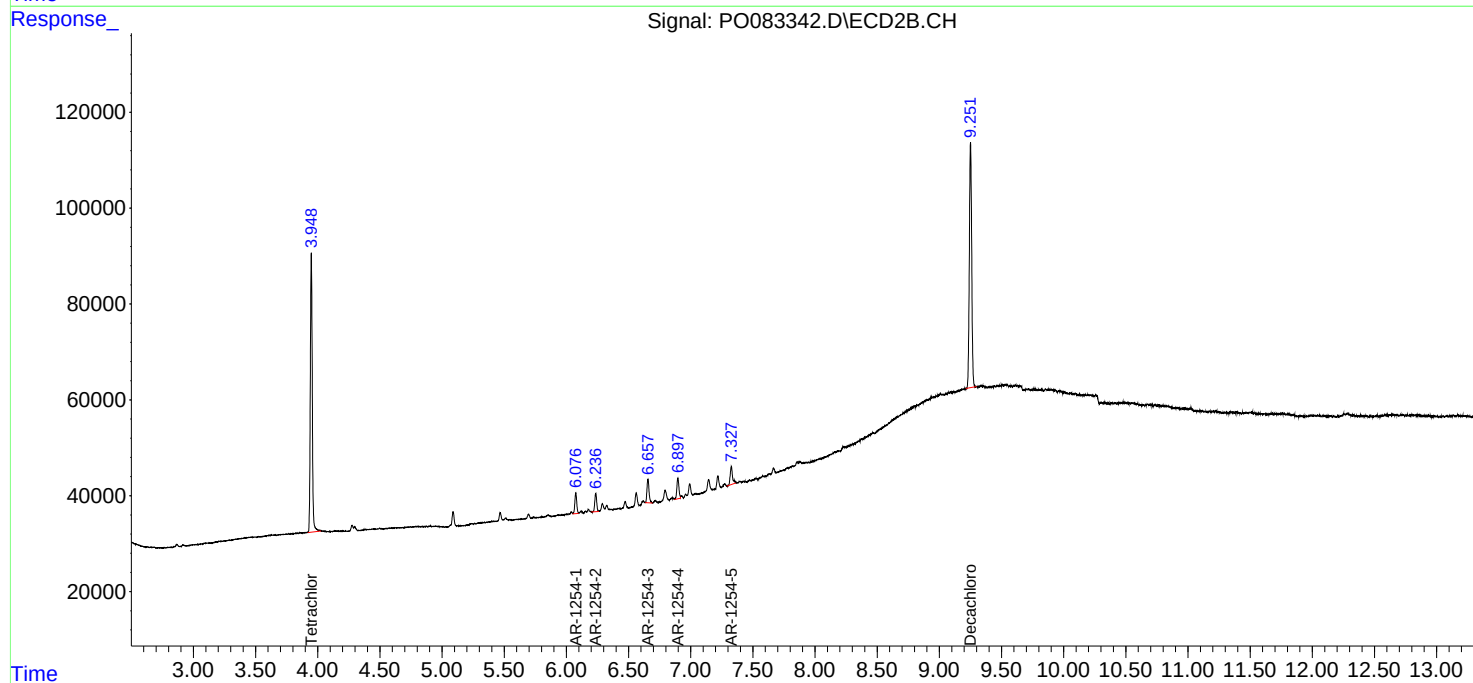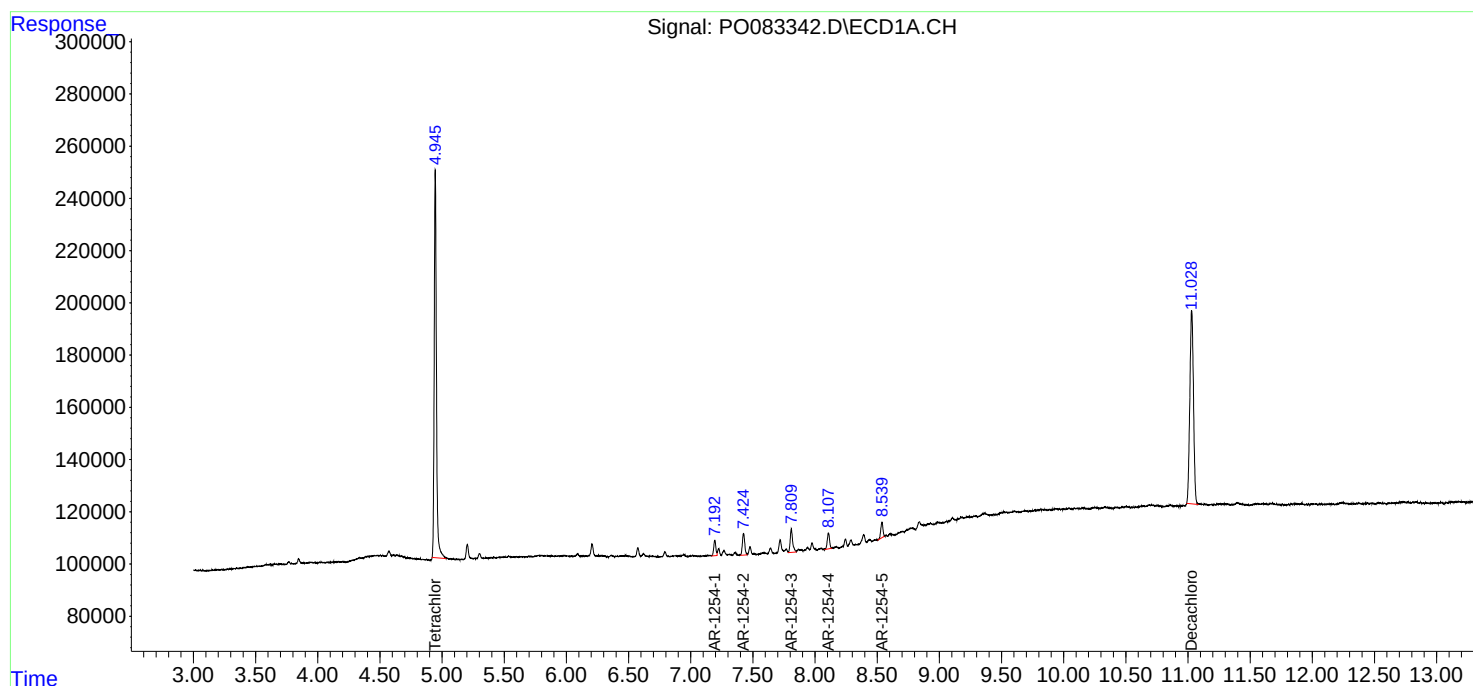


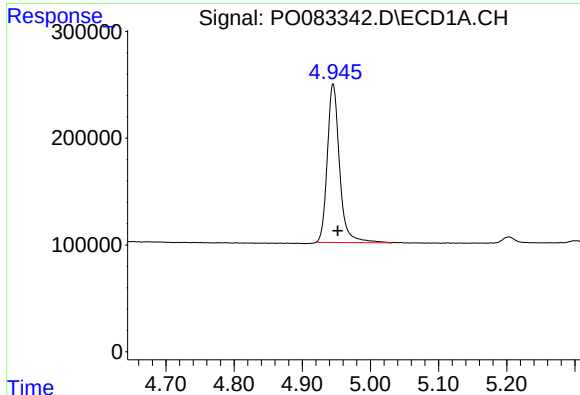

#1 Tetrachloro-m-xylene


R.T.: 4.945 min
Delta R.T.: -0.007 min
Response: 1848144
Conc: 21.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2021

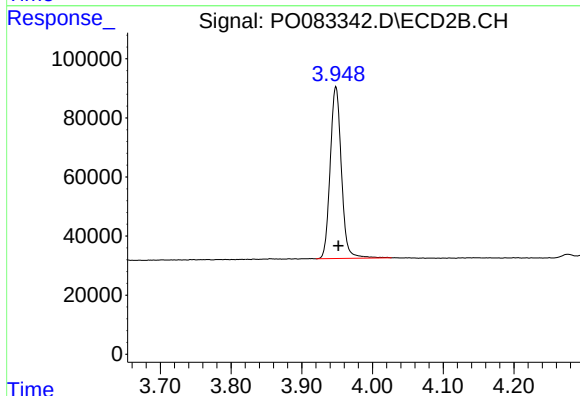


#1 Tetrachloro-m-xylene

R.T.: 3.948 min
Delta R.T.: -0.004 min
Response: 640274
Conc: 21.01 ng/ml

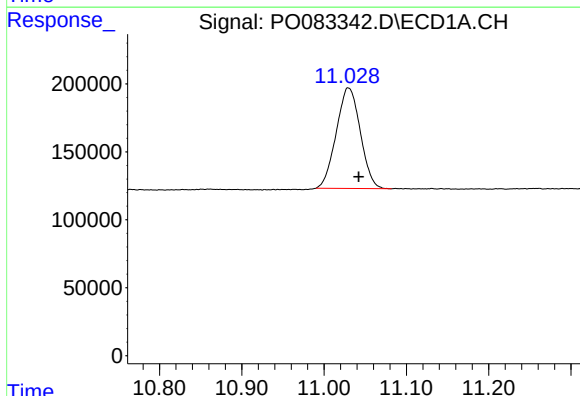


#2 Decachlorobiphenyl

R.T.: 11.029 min
Delta R.T.: -0.013 min
Response: 1506391
Conc: 22.91 ng/ml

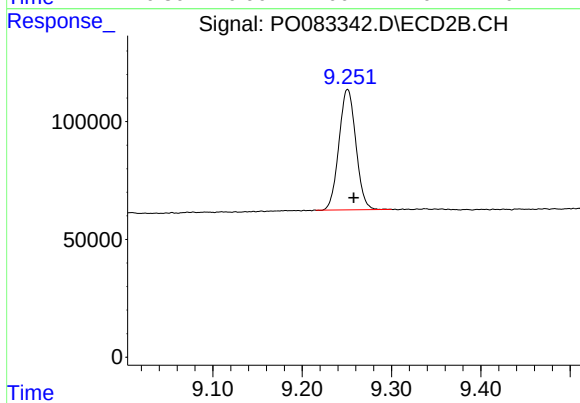

#2 Decachlorobiphenyl


R.T.: 9.251 min
Delta R.T.: -0.007 min
Response: 672591
Conc: 22.37 ng/ml

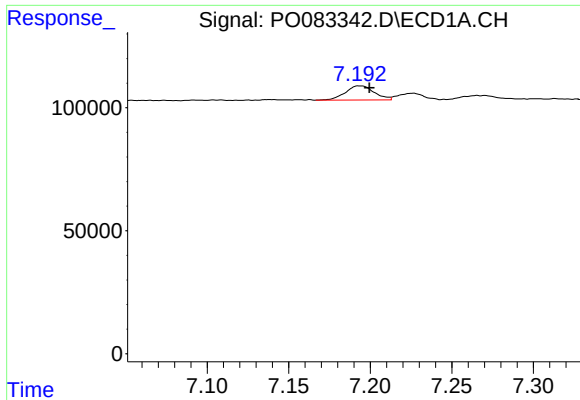

#26 AR-1254-1


R.T.: 7.193 min
Delta R.T.: -0.007 min
Response: 70231
Conc: 25.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2021

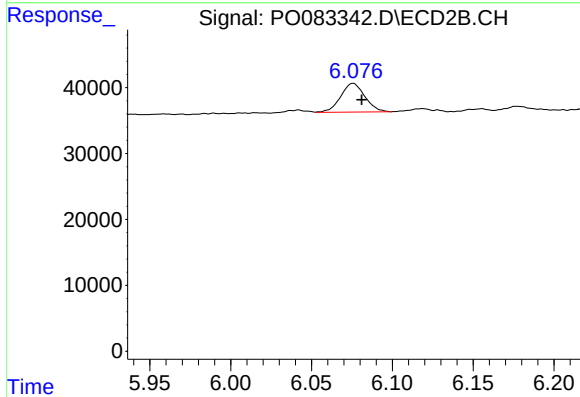


#26 AR-1254-1

R.T.: 6.076 min
Delta R.T.: -0.005 min
Response: 45767
Conc: 23.54 ng/ml

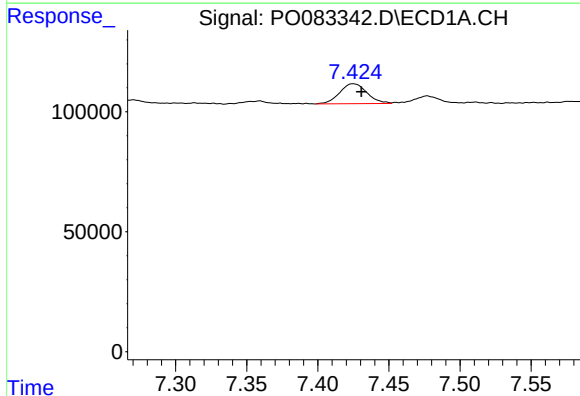


#27 AR-1254-2

R.T.: 7.425 min
Delta R.T.: -0.006 min
Response: 111002
Conc: 26.68 ng/ml

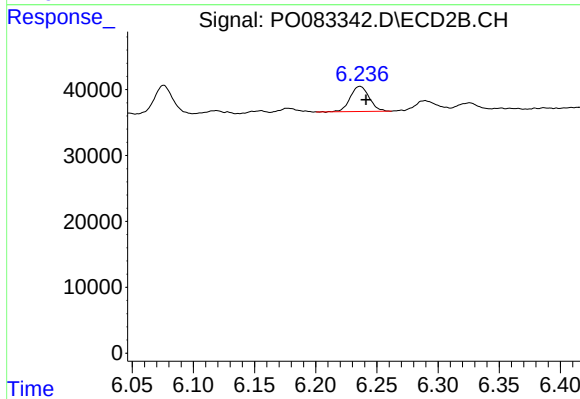

#27 AR-1254-2


R.T.: 6.236 min
Delta R.T.: -0.005 min
Response: 41317
Conc: 24.56 ng/ml

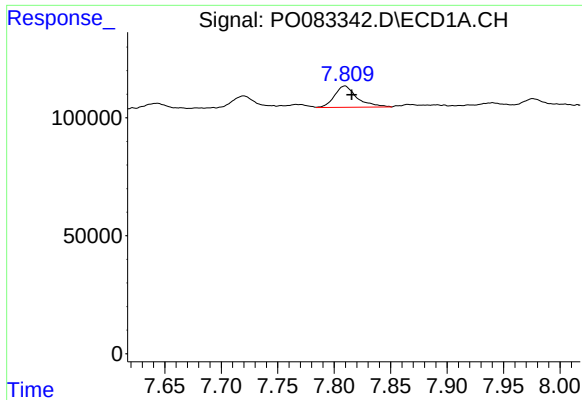

#28 AR-1254-3


R.T.: 7.810 min
Delta R.T.: -0.006 min
Response: 125223
Conc: 29.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2021

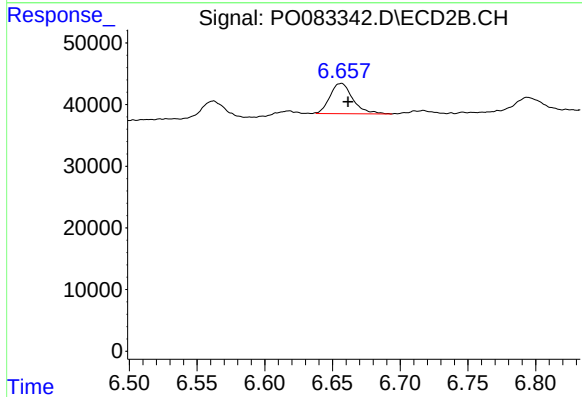


#28 AR-1254-3

R.T.: 6.656 min
Delta R.T.: -0.005 min
Response: 57680
Conc: 22.56 ng/ml

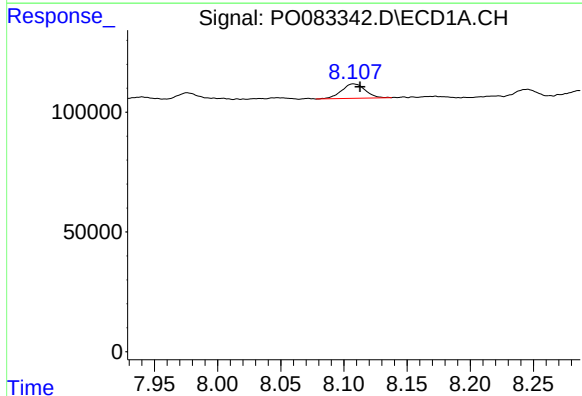


#29 AR-1254-4

R.T.: 8.107 min
Delta R.T.: -0.005 min
Response: 78771
Conc: 25.47 ng/ml

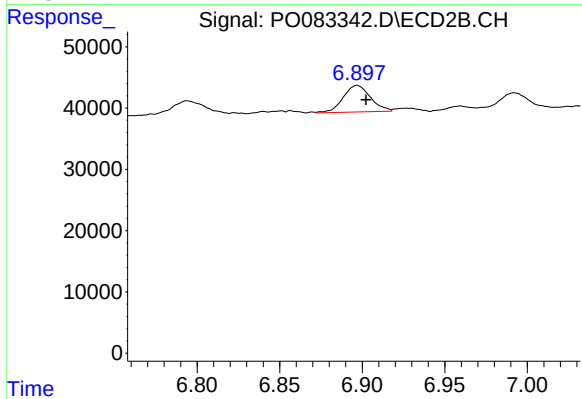

#29 AR-1254-4


R.T.: 6.897 min
Delta R.T.: -0.005 min
Response: 49836
Conc: 27.32 ng/ml

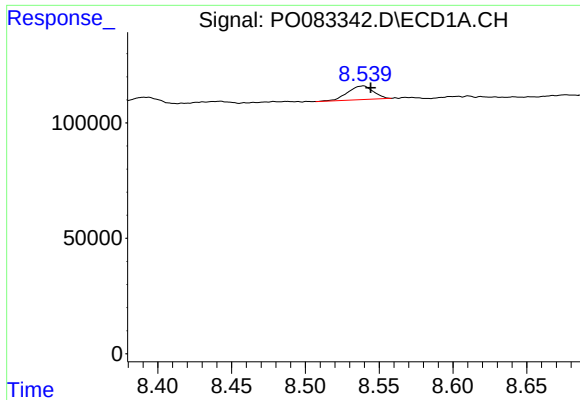

#30 AR-1254-5

R.T.: 8.539 min
Delta R.T.: -0.005 min
Response: 71998
Conc: 22.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2021

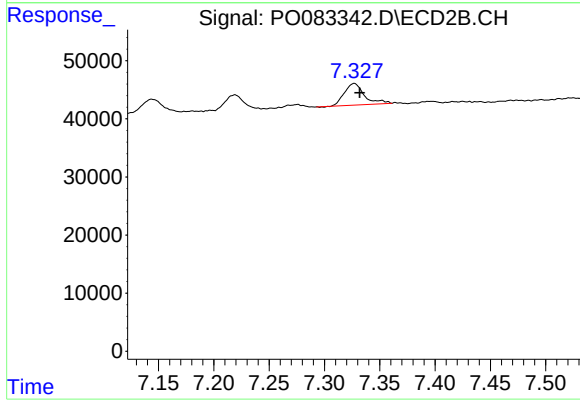

#30 AR-1254-5

R.T.: 7.327 min
Delta R.T.: -0.005 min
Response: 47359
Conc: 20.35 ng/ml