

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120121\
 Data File : P0083343.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Dec 2021 22:33
 Operator : AJ\MA
 Sample : M4068-09
 Misc : AR1262 MDL 25 PPB
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT4-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 00:00:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Nov 20 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.946	3.948	1874298	642908	21.357	21.091
2) SA Decachlor...	11.030	9.251	1532395	686815	23.304	22.847
Target Compounds						
36) L8 AR-1262-1	8.612	7.326	107779	33697	28.901	27.658
37) L8 AR-1262-2	9.176	7.881	172632	121587	26.828	26.913
38) L8 AR-1262-3	9.491	8.166	89048	49356	29.276	26.374m
39) L8 AR-1262-4	9.586	8.231	68310	79931	36.090	25.239 #
40) L8 AR-1262-5	10.269	8.732	66629	37547	26.702	25.325



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO120121\
Data File : PO083343.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Dec 2021 22:33
Operator : AJ\MA
Sample : M4068-09
Misc : AR1262 MDL 25 PPB
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_0
ClientSampleId :
MDL-WATER-03-QT4-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 00:00:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO111921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Nov 20 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

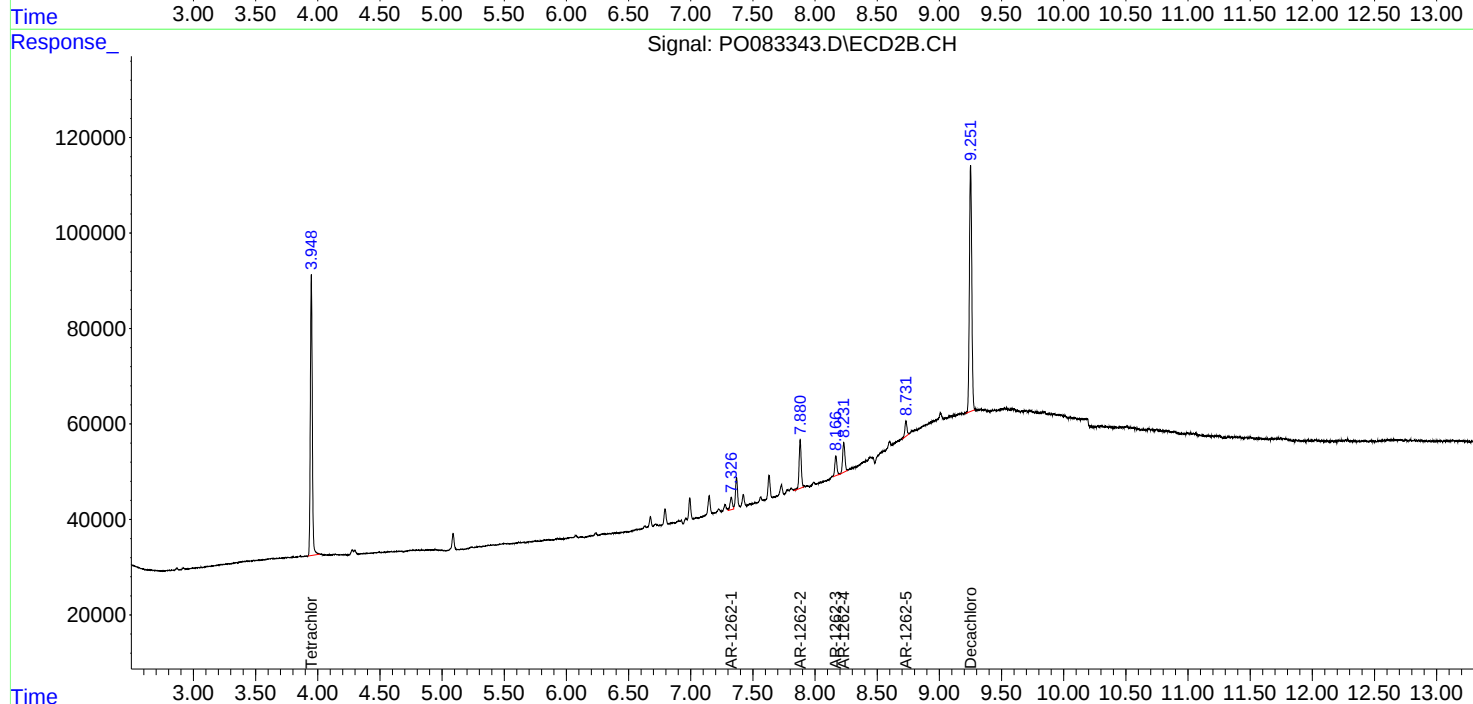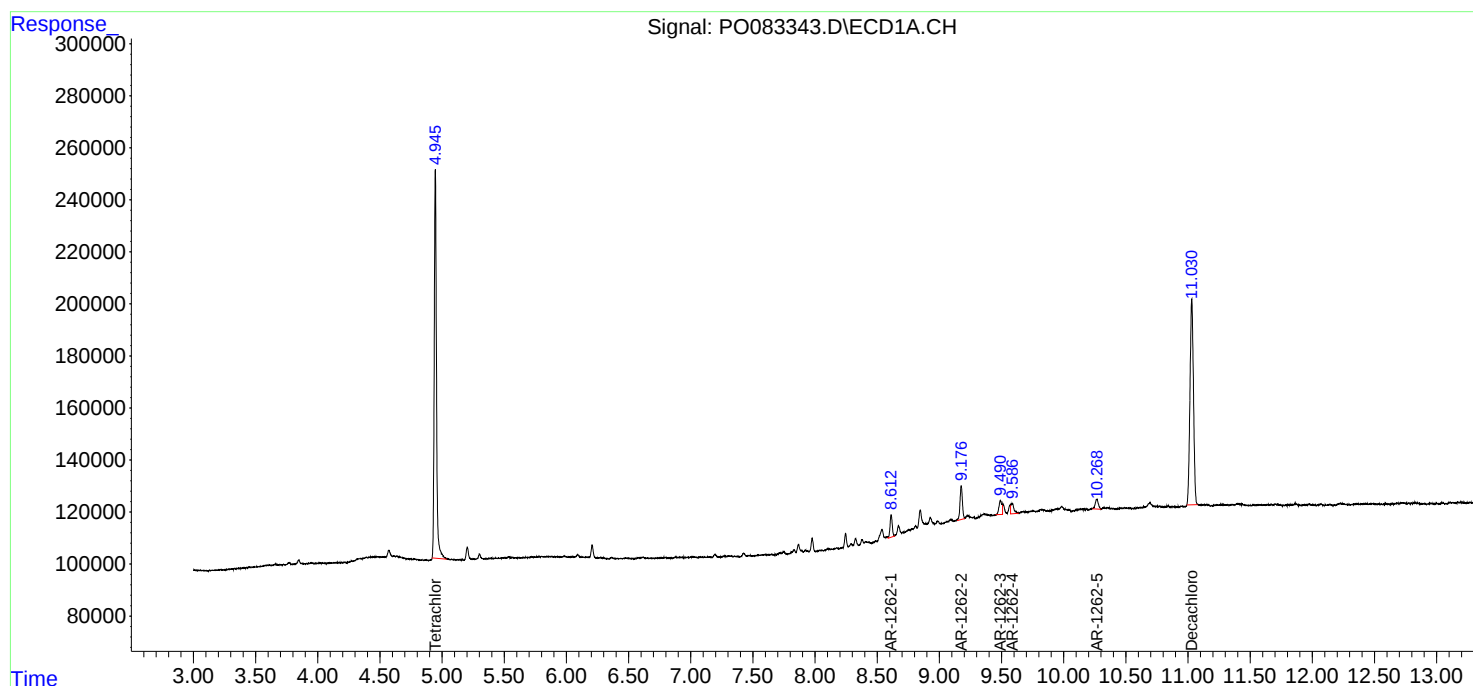


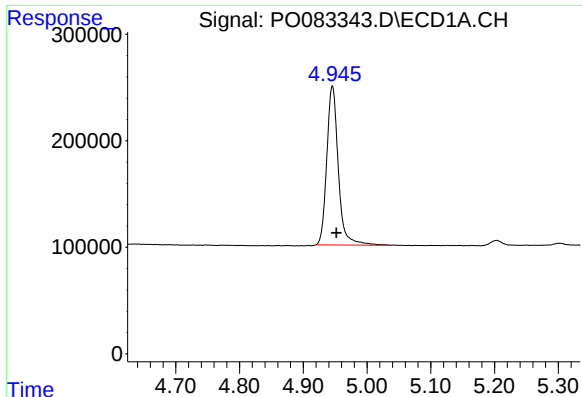

#1 Tetrachloro-m-xylene


R.T.: 4.946 min
Delta R.T.: -0.006 min
Response: 1874298
Conc: 21.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2021

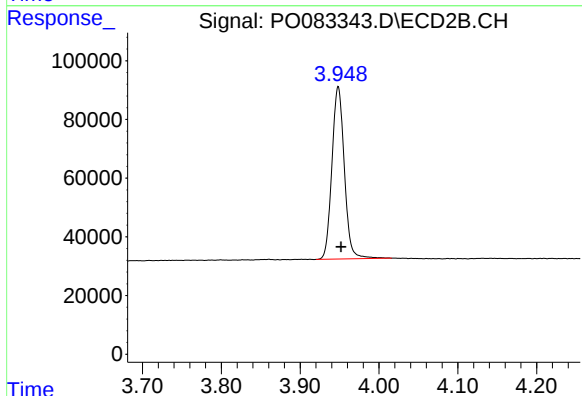


#1 Tetrachloro-m-xylene

R.T.: 3.948 min
Delta R.T.: -0.004 min
Response: 642908
Conc: 21.09 ng/ml

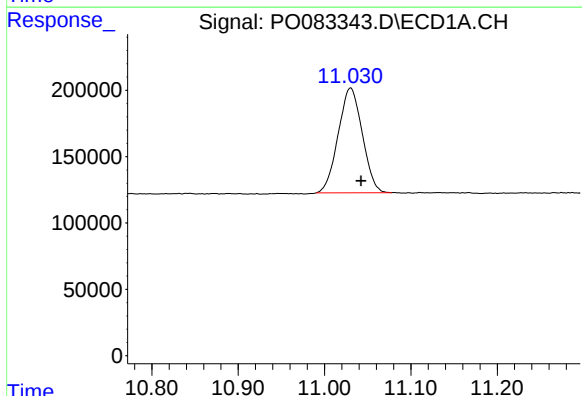


#2 Decachlorobiphenyl

R.T.: 11.030 min
Delta R.T.: -0.012 min
Response: 1532395
Conc: 23.30 ng/ml

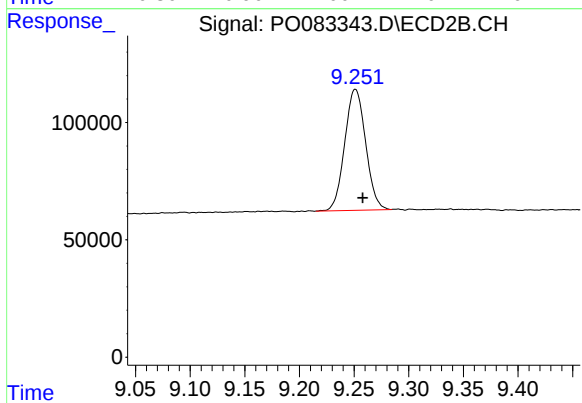

#2 Decachlorobiphenyl


R.T.: 9.251 min
Delta R.T.: -0.007 min
Response: 686815
Conc: 22.85 ng/ml

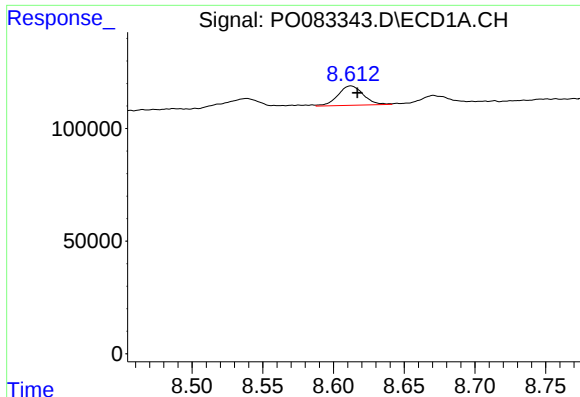

#36 AR-1262-1


R.T.: 8.612 min
Delta R.T.: -0.005 min
Response: 107779
Conc: 28.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2021

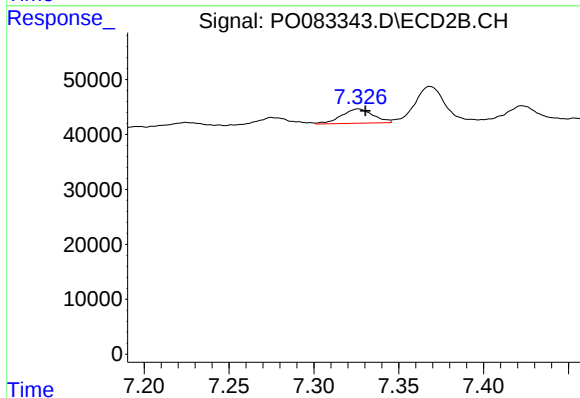


#36 AR-1262-1

R.T.: 7.326 min
Delta R.T.: -0.004 min
Response: 33697
Conc: 27.66 ng/ml

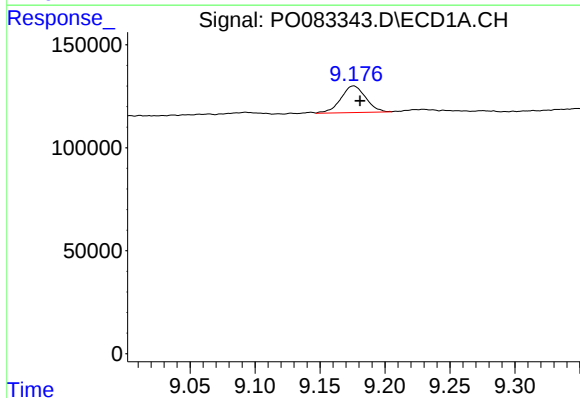


#37 AR-1262-2

R.T.: 9.176 min
Delta R.T.: -0.005 min
Response: 172632
Conc: 26.83 ng/ml

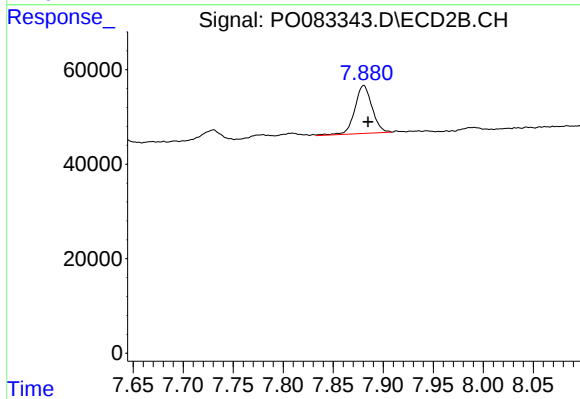

#37 AR-1262-2


R.T.: 7.881 min
Delta R.T.: -0.004 min
Response: 121587
Conc: 26.91 ng/ml

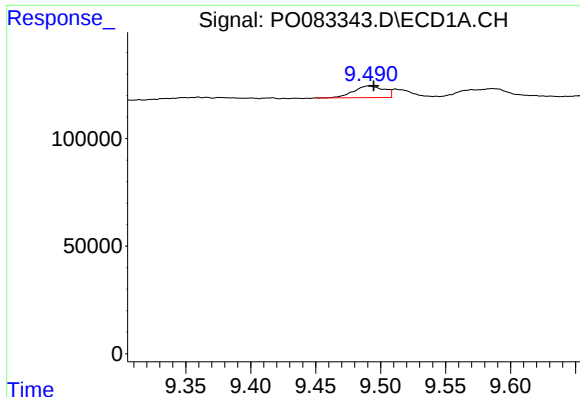

#38 AR-1262-3


R.T.: 9.491 min
Delta R.T.: -0.004 min
Response: 89048
Conc: 29.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2021

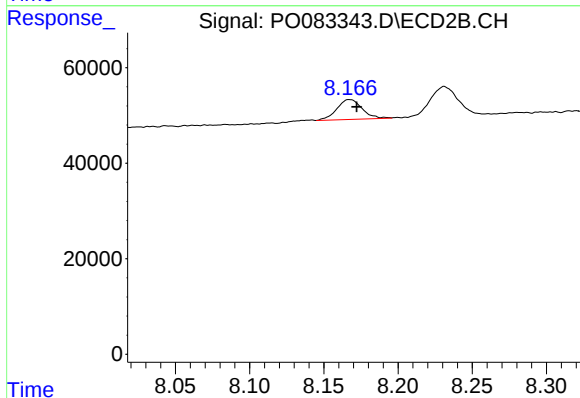


#38 AR-1262-3

R.T.: 8.166 min
Delta R.T.: -0.006 min
Response: 49356
Conc: 26.37 ng/ml m

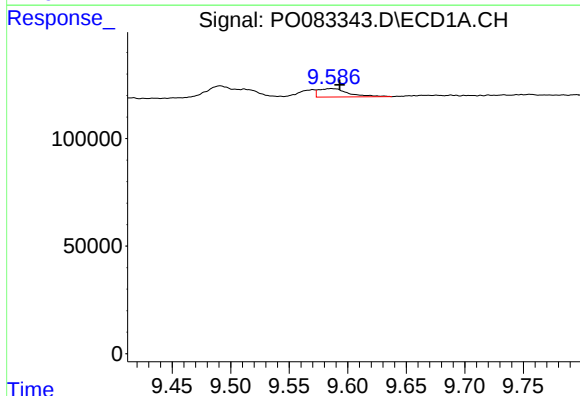


#39 AR-1262-4

R.T.: 9.586 min
Delta R.T.: -0.007 min
Response: 68310
Conc: 36.09 ng/ml

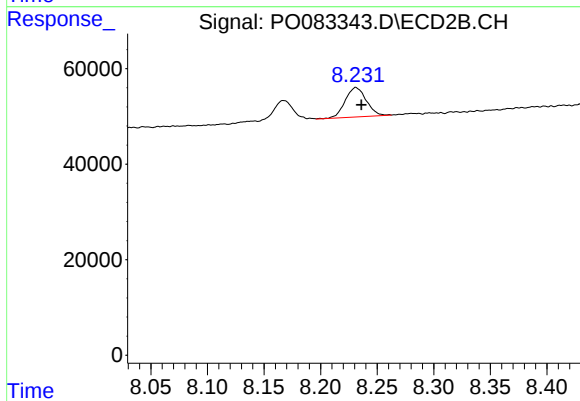

#39 AR-1262-4


R.T.: 8.231 min
Delta R.T.: -0.005 min
Response: 79931
Conc: 25.24 ng/ml

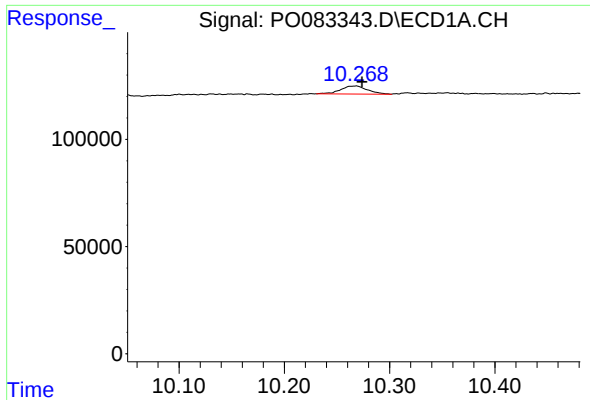

#40 AR-1262-5

R.T.: 10.269 min
Delta R.T.: -0.005 min
Response: 66629
Conc: 26.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2021

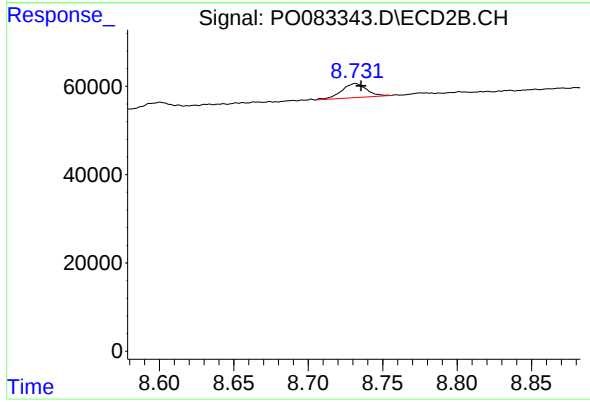

#40 AR-1262-5

R.T.: 8.732 min
Delta R.T.: -0.004 min
Response: 37547
Conc: 25.32 ng/ml