

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120121\
 Data File : PO083344.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Dec 2021 22:50
 Operator : AJ\MA
 Sample : M4068-09
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT4-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 00:01:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Nov 20 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.947	3.949	1908834	644285	21.751	21.137
2) SA Decachlor...	11.032	9.251	1674639	744528	25.467	24.767
Target Compounds						
41) L9 AR-1268-1	9.491	8.167	210185	145031	25.406	25.150m
42) L9 AR-1268-2	9.589	8.233	187508	122904	24.378	25.589
43) L9 AR-1268-3	9.818	8.440	173509	104575	26.458	25.369
44) L9 AR-1268-4	10.265	8.731	72177	41582	25.276	24.531
45) L9 AR-1268-5	10.688	9.010	603549	287369	26.917	24.446



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120121\
Data File : P0083344.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Dec 2021 22:50
Operator : AJ\MA
Sample : M4068-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 00:01:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Nov 20 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

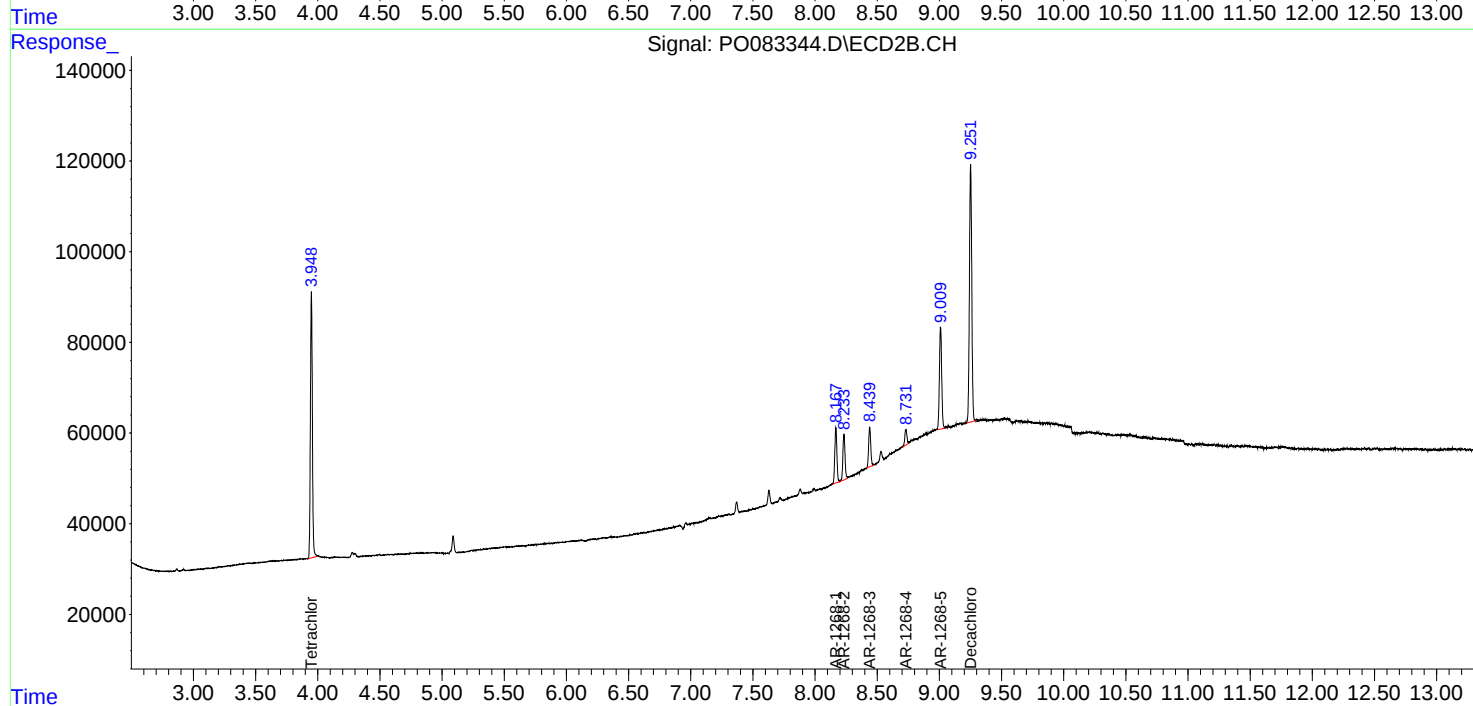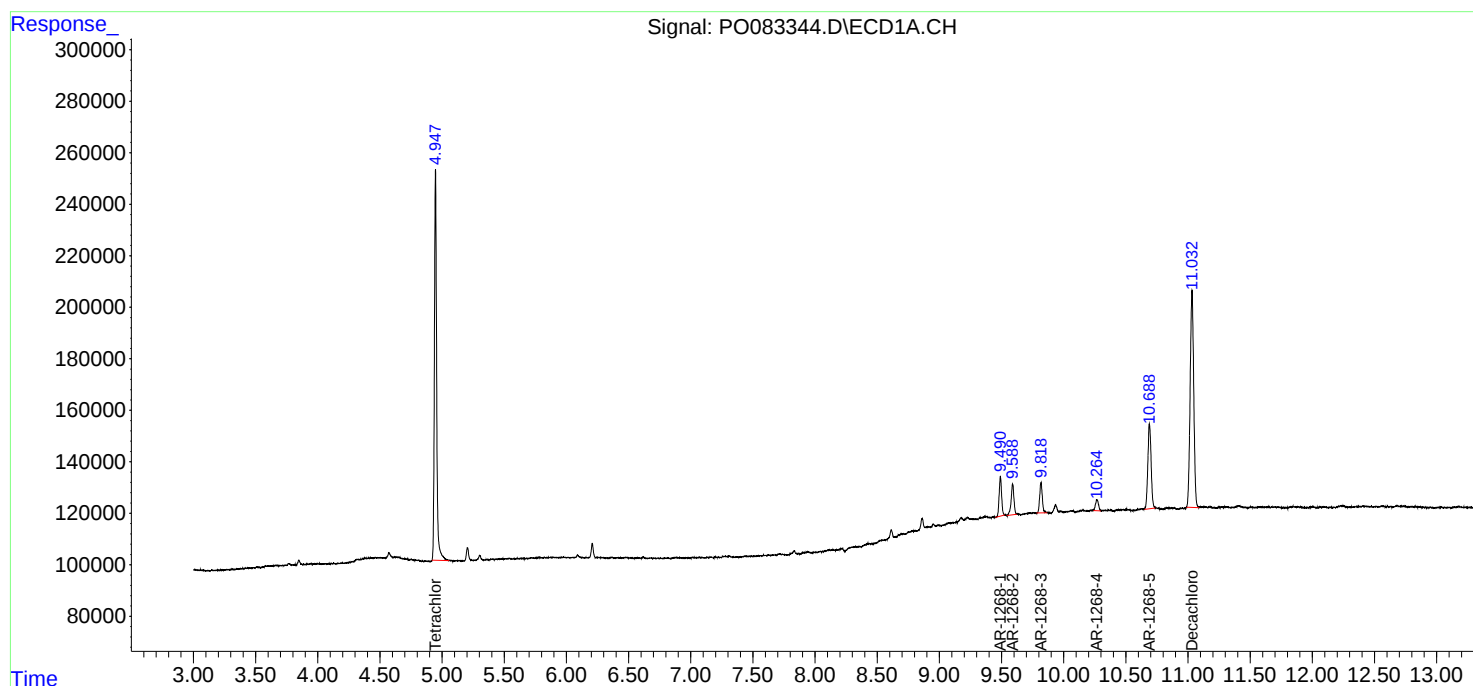


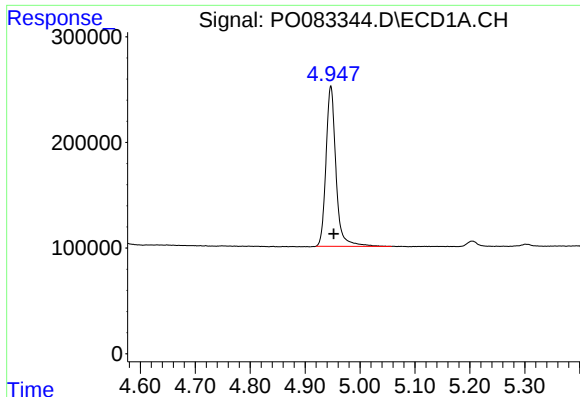

#1 Tetrachloro-m-xylene


R.T.: 4.947 min
Delta R.T.: -0.005 min
Response: 1908834
Conc: 21.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2021

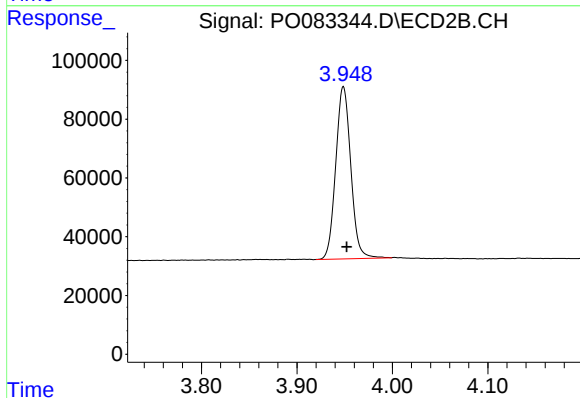


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: -0.003 min
Response: 644285
Conc: 21.14 ng/ml

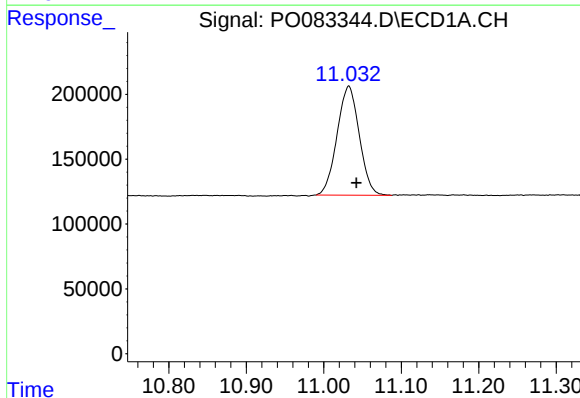


#2 Decachlorobiphenyl

R.T.: 11.032 min
Delta R.T.: -0.010 min
Response: 1674639
Conc: 25.47 ng/ml

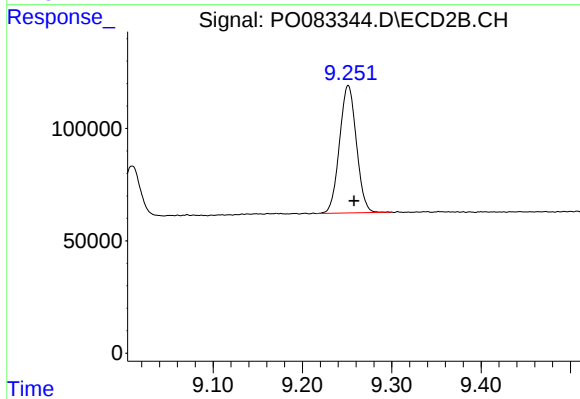

#2 Decachlorobiphenyl


R.T.: 9.251 min
Delta R.T.: -0.007 min
Response: 744528
Conc: 24.77 ng/ml

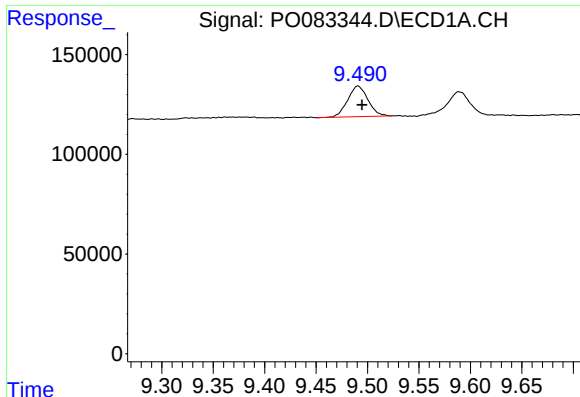

#41 AR-1268-1


R.T.: 9.491 min
Delta R.T.: -0.004 min
Response: 210185
Conc: 25.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2021

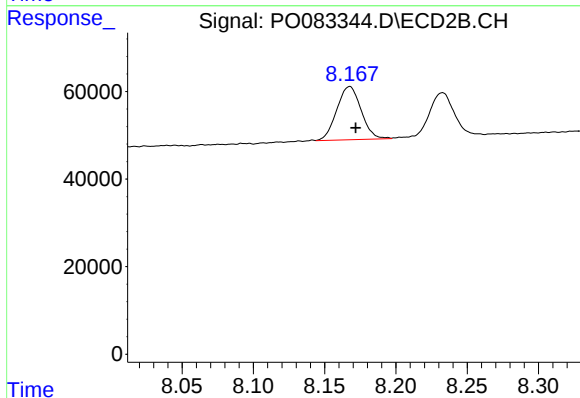


#41 AR-1268-1

R.T.: 8.167 min
Delta R.T.: -0.004 min
Response: 145031
Conc: 25.15 ng/ml m

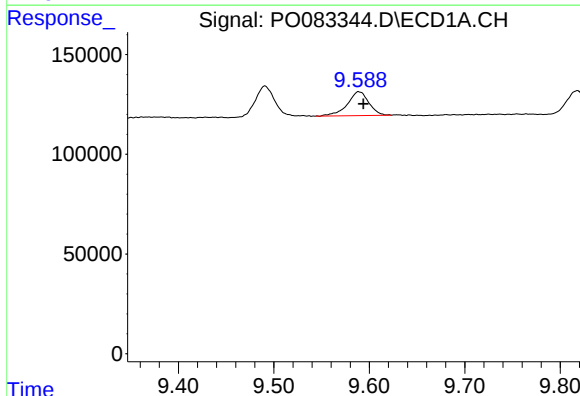


#42 AR-1268-2

R.T.: 9.589 min
Delta R.T.: -0.005 min
Response: 187508
Conc: 24.38 ng/ml

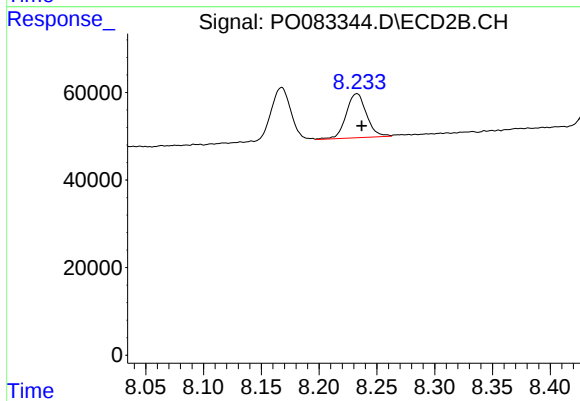

#42 AR-1268-2


R.T.: 8.233 min
Delta R.T.: -0.004 min
Response: 122904
Conc: 25.59 ng/ml

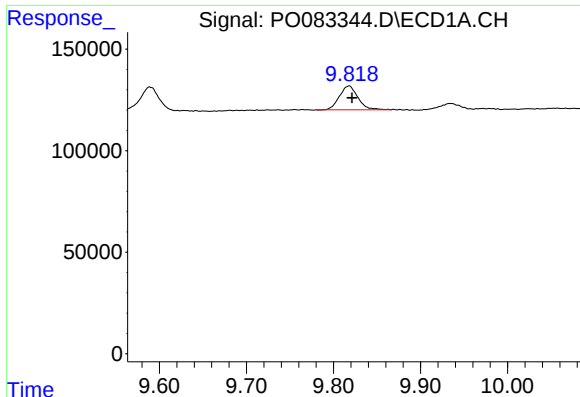

#43 AR-1268-3


R.T.: 9.818 min
Delta R.T.: -0.003 min
Response: 173509
Conc: 26.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2021

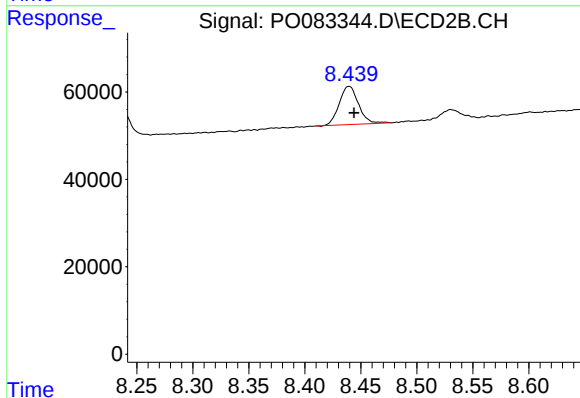


#43 AR-1268-3

R.T.: 8.440 min
Delta R.T.: -0.004 min
Response: 104575
Conc: 25.37 ng/ml

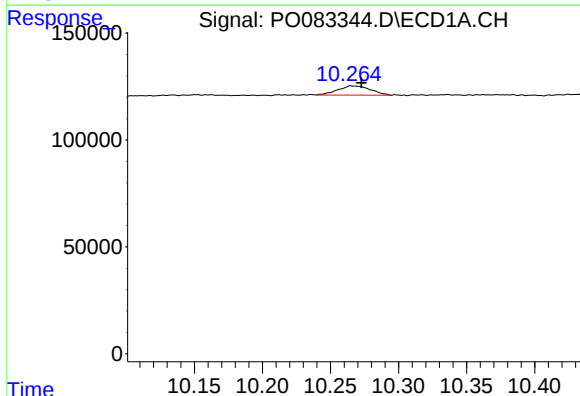


#44 AR-1268-4

R.T.: 10.265 min
Delta R.T.: -0.008 min
Response: 72177
Conc: 25.28 ng/ml

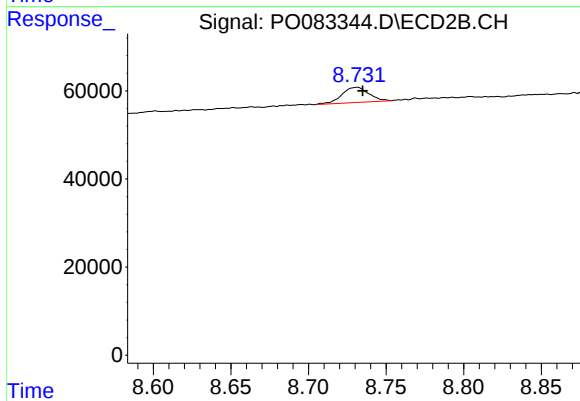

#44 AR-1268-4


R.T.: 8.731 min
Delta R.T.: -0.004 min
Response: 41582
Conc: 24.53 ng/ml

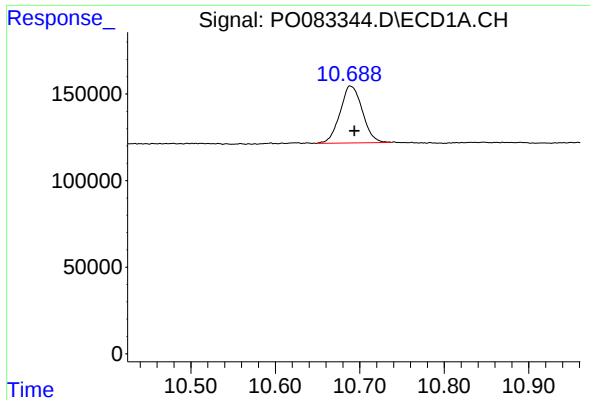

#45 AR-1268-5

R.T.: 10.688 min
Delta R.T.: -0.005 min
Response: 603549
Conc: 26.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2021

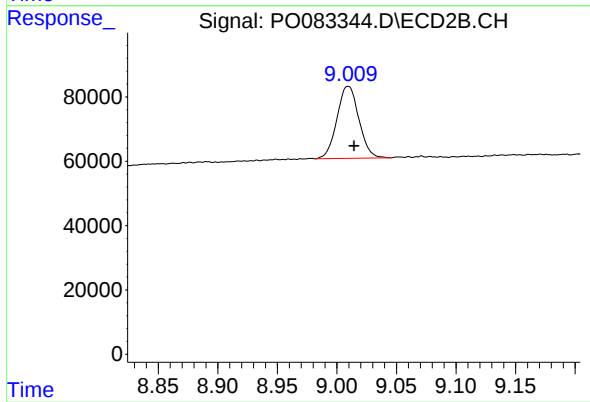

#45 AR-1268-5

R.T.: 9.010 min
Delta R.T.: -0.005 min
Response: 287369
Conc: 24.45 ng/ml