

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120123\
 Data File : PO100222.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2023 17:21
 Operator : YP/AJ
 Sample : 05592-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MW04S

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/04/2023
 Supervised By :Ankita Jodhani 12/04/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 21:26:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 21 15:58:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.478	3.704	24245062	27202640	14.205m	18.136 #
2) SA Decachlor...	10.354	8.794	12228663	17868542	16.836	15.968

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120123\
Data File : PO100222.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2023 17:21
Operator : YP/AJ
Sample : 05592-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MW04S


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/04/2023
Supervised By :Ankita Jodhani 12/04/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 21:26:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 21 15:58:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

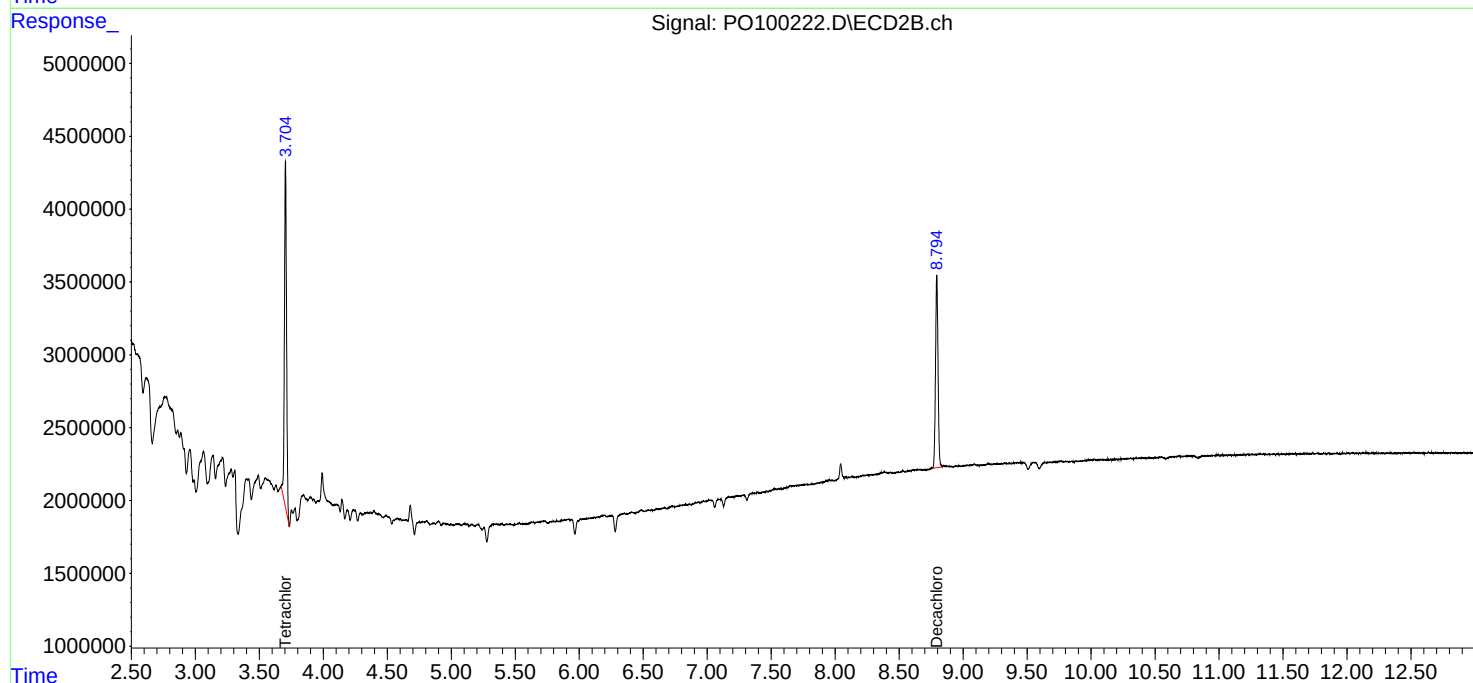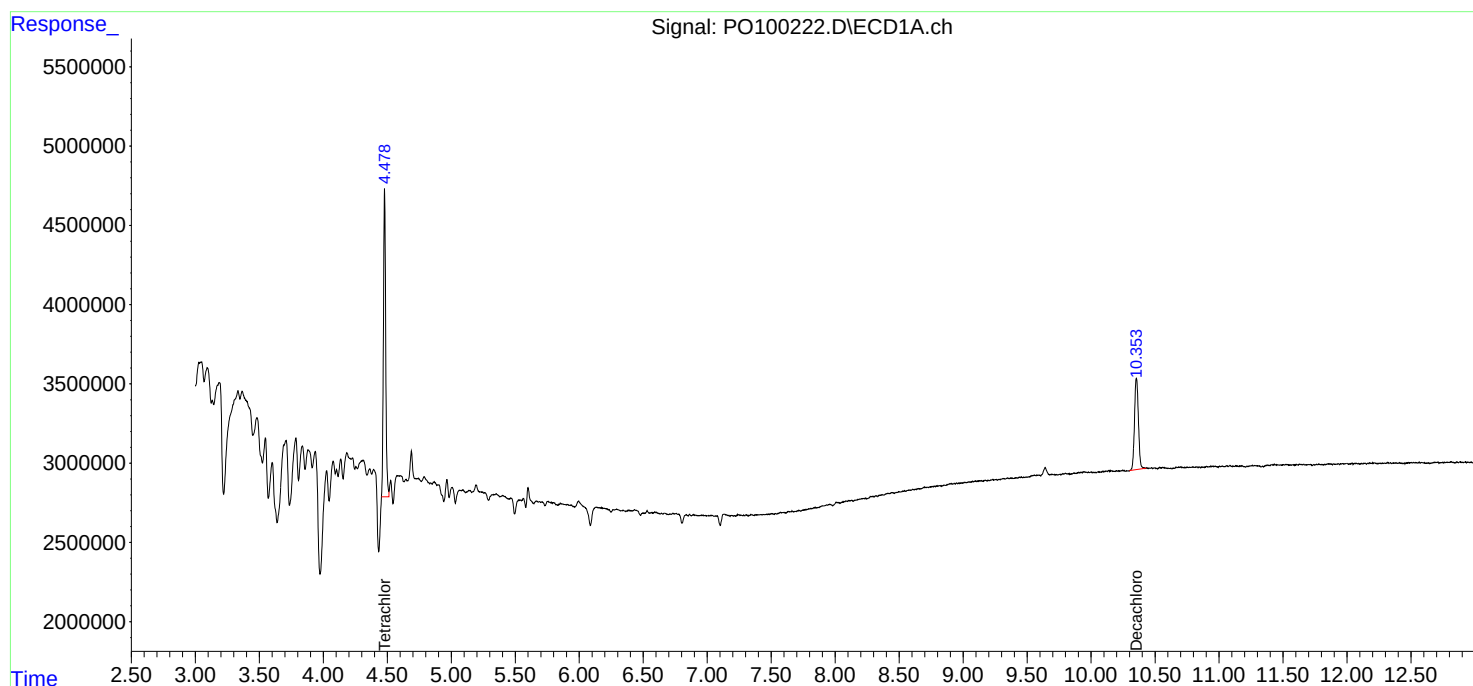

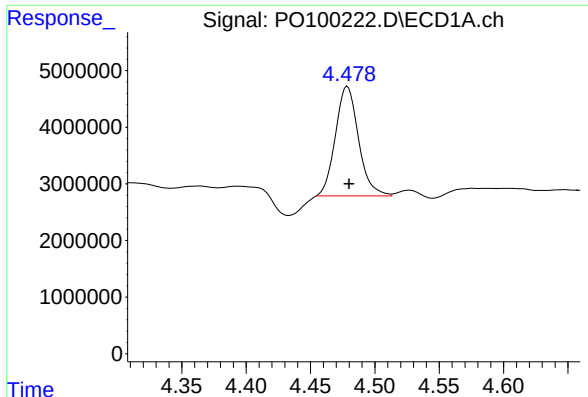


#1 Tetrachloro-m-xylene

R.T.: 4.478 min
Delta R.T.: -0.002 min
Response: 24245062
Conc: 14.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
MW04S


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/04/2023
Supervised By :Ankita Jodhani 12/04/2023

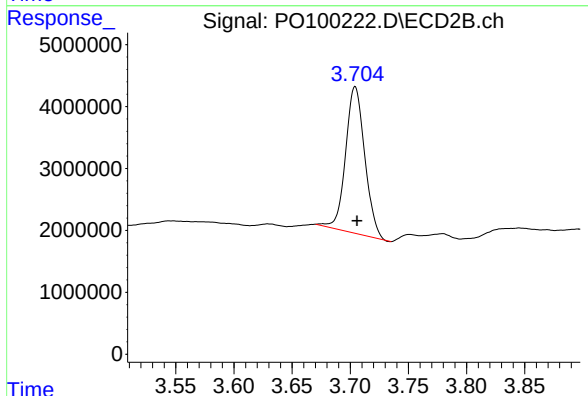


#1 Tetrachloro-m-xylene

R.T.: 3.704 min
Delta R.T.: -0.002 min
Response: 27202640
Conc: 18.14 ng/ml

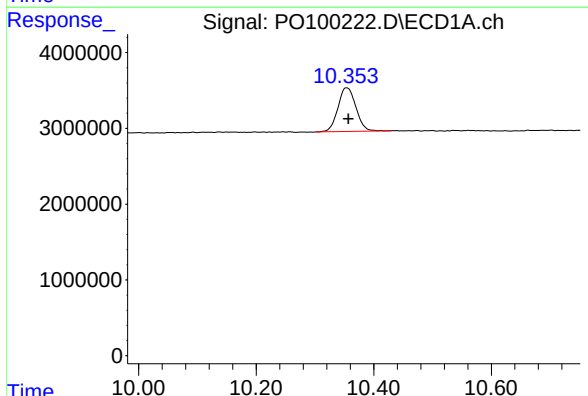

#2 Decachlorobiphenyl

R.T.: 10.354 min
Delta R.T.: -0.003 min
Response: 12228663
Conc: 16.84 ng/ml

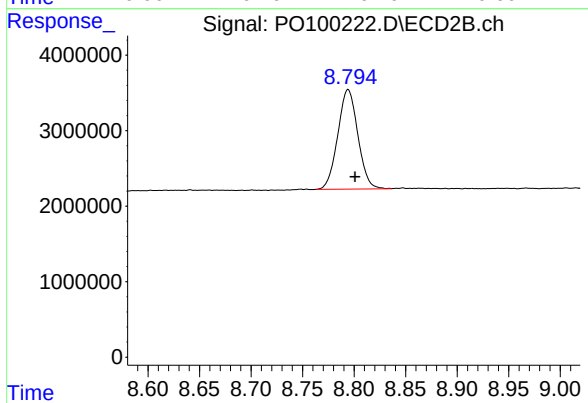

#2 Decachlorobiphenyl

R.T.: 8.794 min
Delta R.T.: -0.007 min
Response: 17868542
Conc: 15.97 ng/ml