

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0120219\
 Data File : P0064271.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Dec 2019 19:21
 Operator : SM/AJ
 Sample : K6090-03MS
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-20-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 01:37:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 28 01:28:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.312	3.559	644656	534678	21.768	22.480
2)	SA Decachlor...	9.941	8.524	699932	690599	17.078	16.905
Target Compounds							
3)	L1 AR-1016-1	5.406	0.000	14387	0	11.083	N.D. #
9)	L2 AR-1221-2	4.616	3.857	12314	11639	44.537	58.239 #
10)	L2 AR-1221-3	4.616	0.000	12314	0	14.665	N.D. #
11)	L3 AR-1232-1	4.616	0.000	12314	0	9.605	N.D. #
21)	L5 AR-1248-1	5.406	0.000	14387	0	25.650	N.D. #
31)	L7 AR-1260-1	0.000	6.108	0	6459	N.D.	3.680 #
33)	L7 AR-1260-3	0.000	6.507	0	7996	N.D.	3.933 #
35)	L7 AR-1260-5	8.218	7.159	7538	9654	1.707	1.994
37)	L8 AR-1262-2	8.218	7.159	7538	9654	1.367	1.618
38)	L8 AR-1262-3	0.000	7.443	0	3304	N.D.	1.417 #
39)	L8 AR-1262-4	0.000	7.510	0	8670	N.D.	1.947 #
41)	L9 AR-1268-1	0.000	7.443	0	3304	N.D.	0.473 #
42)	L9 AR-1268-2	0.000	7.510	0	8670	N.D.	1.354 #
43)	L9 AR-1268-3	0.000	7.775	0	10069	N.D.	1.923 #
45)	L9 AR-1268-5	0.000	8.278	0	9432	N.D.	0.571 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120219\
Data File : PO064271.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Dec 2019 19:21
Operator : SM/AJ
Sample : K6090-03MS
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-20-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 01:37:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112719.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 28 01:28:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

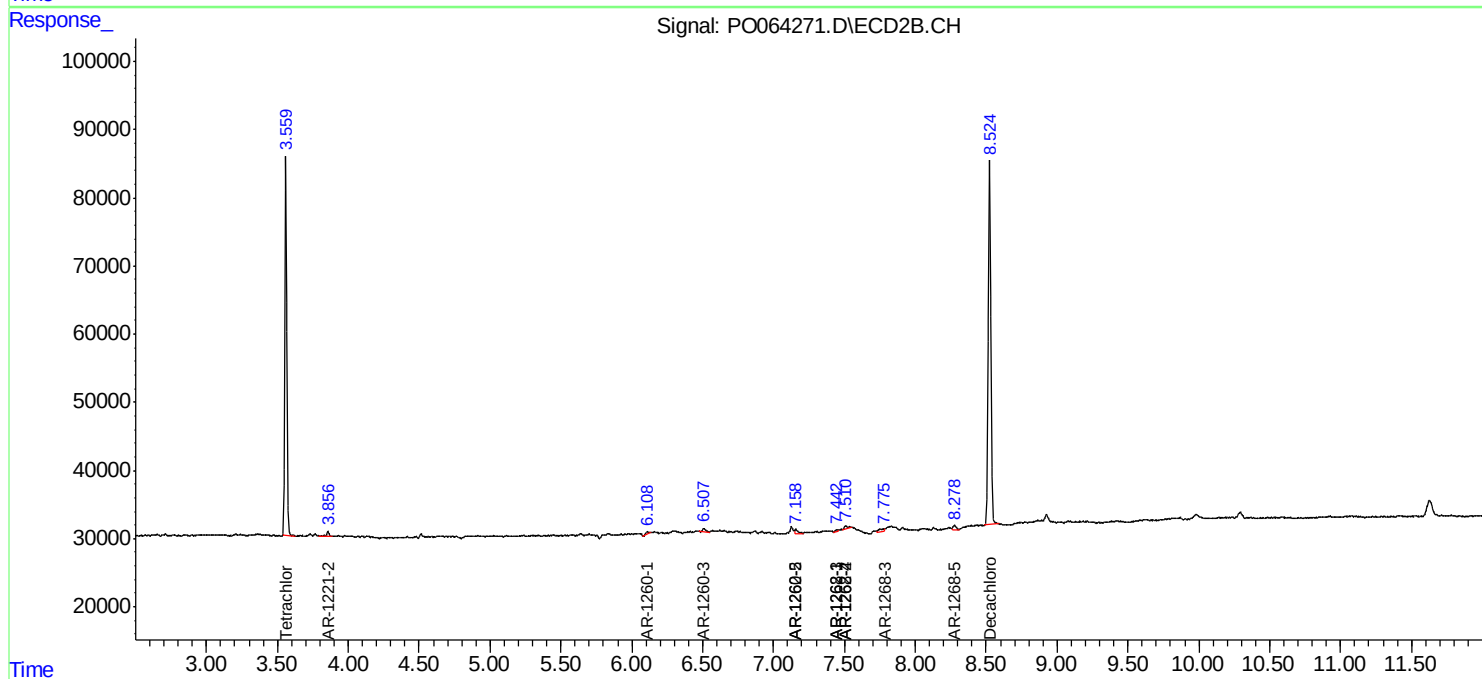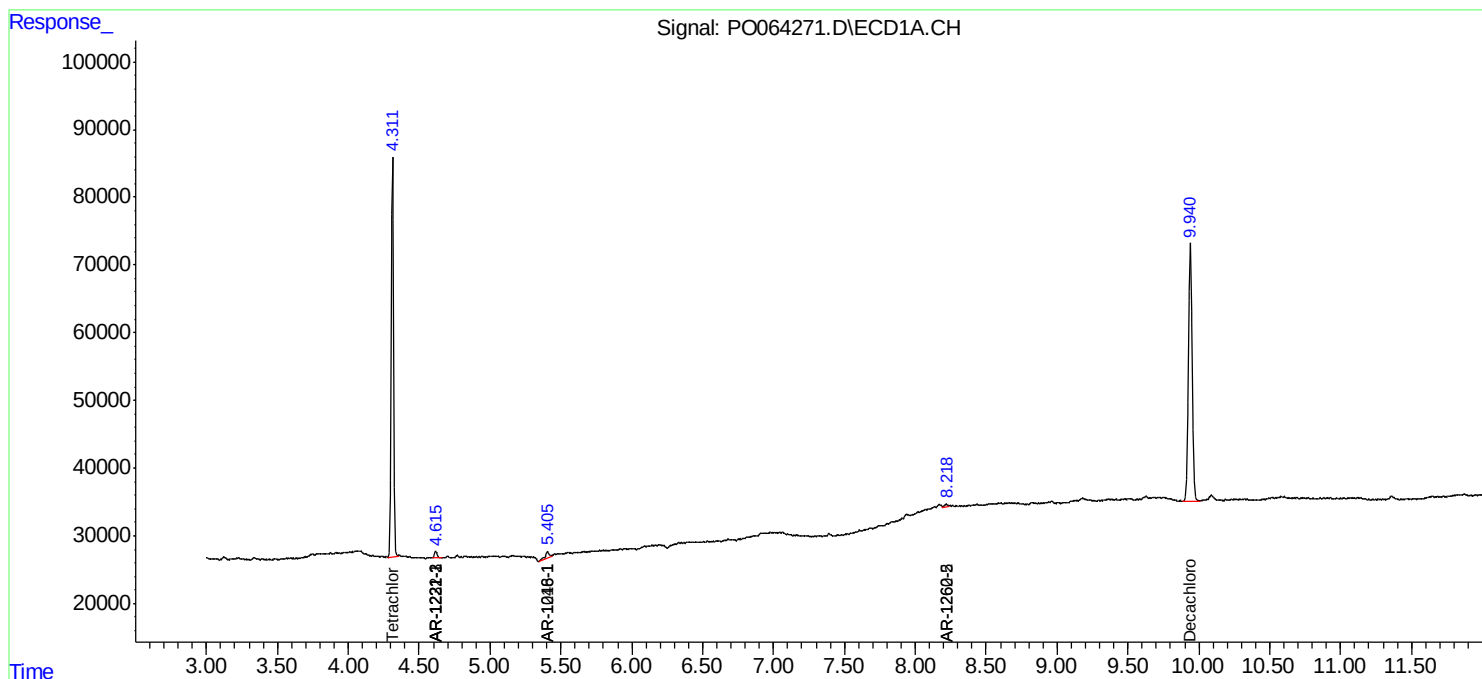


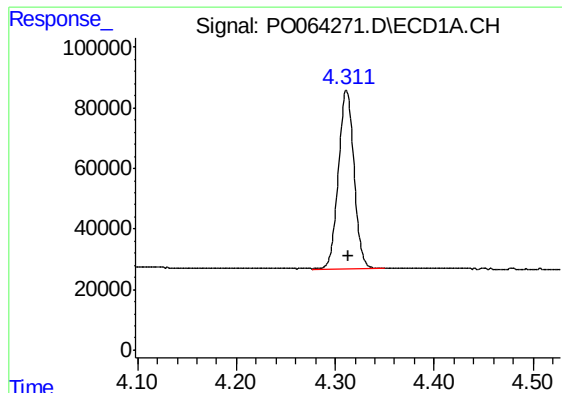

#1 Tetrachloro-m-xylene


R.T.: 4.312 min
Delta R.T.: -0.001 min
Response: 644656
Conc: 21.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-20-S

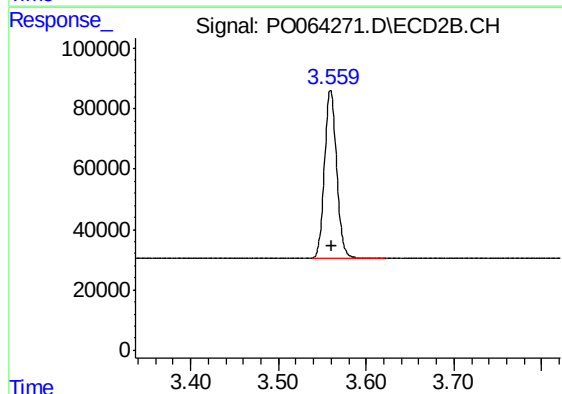


#1 Tetrachloro-m-xylene

R.T.: 3.559 min
Delta R.T.: -0.002 min
Response: 534678
Conc: 22.48 ng/ml

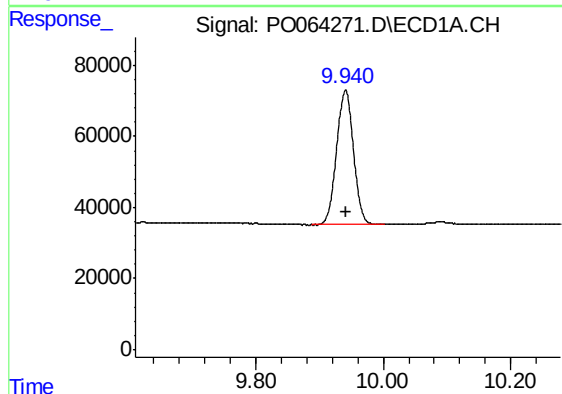


#2 Decachlorobiphenyl

R.T.: 9.941 min
Delta R.T.: 0.000 min
Response: 699932
Conc: 17.08 ng/ml

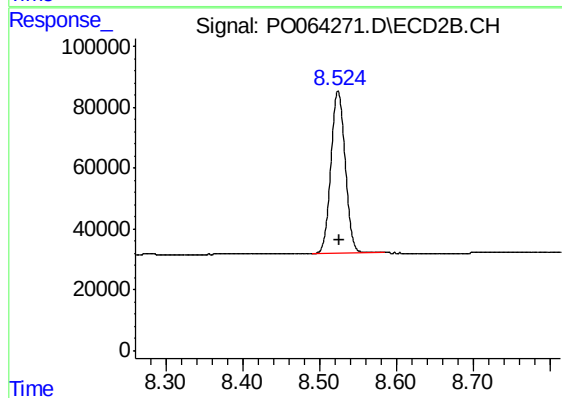

#2 Decachlorobiphenyl


R.T.: 8.524 min
Delta R.T.: -0.003 min
Response: 690599
Conc: 16.91 ng/ml

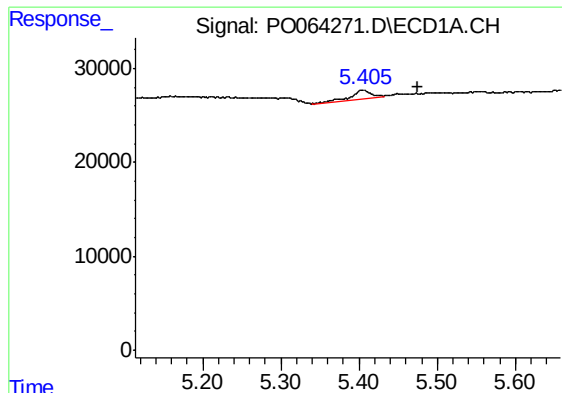

#3 AR-1016-1


R.T.: 5.406 min
Delta R.T.: -0.069 min
Response: 14387
Conc: 11.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-20-S

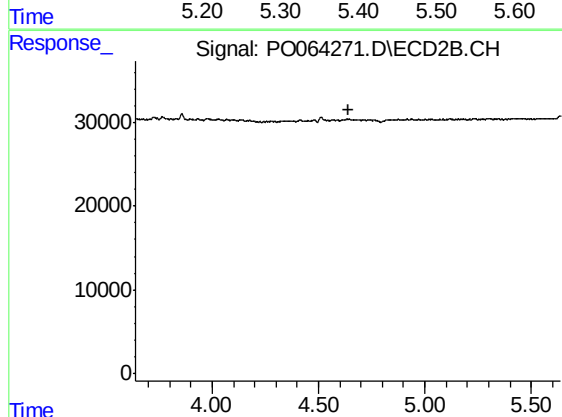


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.638 min
Response: 0
Conc: N.D.

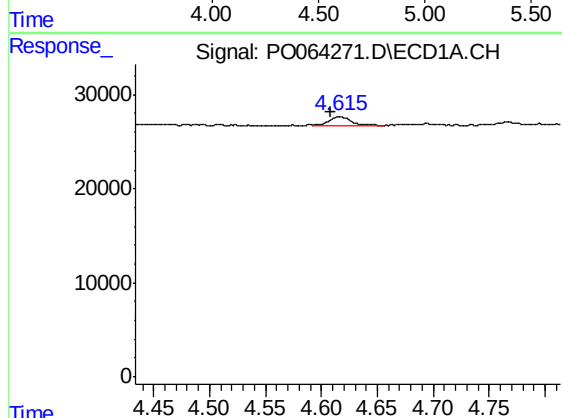


#9 AR-1221-2

R.T.: 4.616 min
Delta R.T.: 0.008 min
Response: 12314
Conc: 44.54 ng/ml

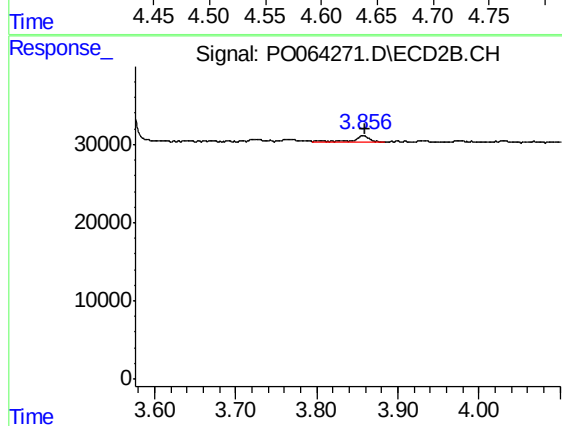

#9 AR-1221-2


R.T.: 3.857 min
Delta R.T.: -0.003 min
Response: 11639
Conc: 58.24 ng/ml

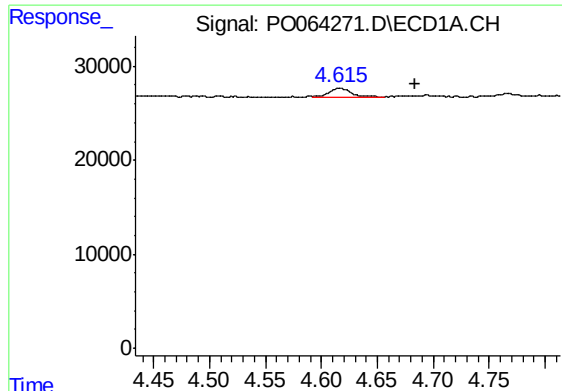

#10 AR-1221-3


R.T.: 4.616 min
Delta R.T.: -0.068 min
Response: 12314
Conc: 14.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-20-S

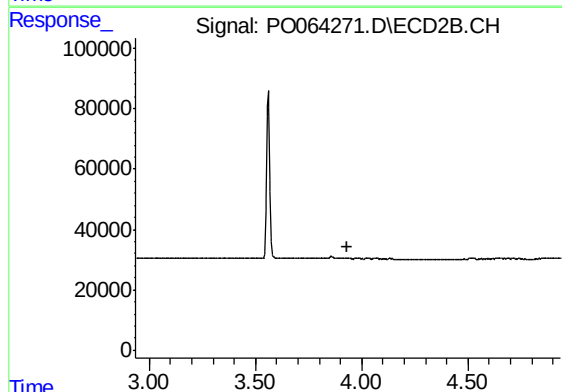


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 3.935 min
Response: 0
Conc: N.D.

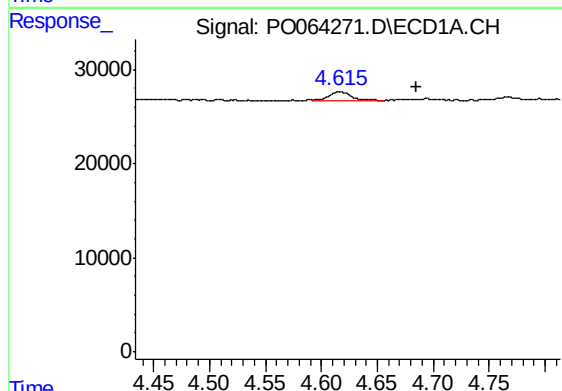


#11 AR-1232-1

R.T.: 4.616 min
Delta R.T.: -0.069 min
Response: 12314
Conc: 9.60 ng/ml

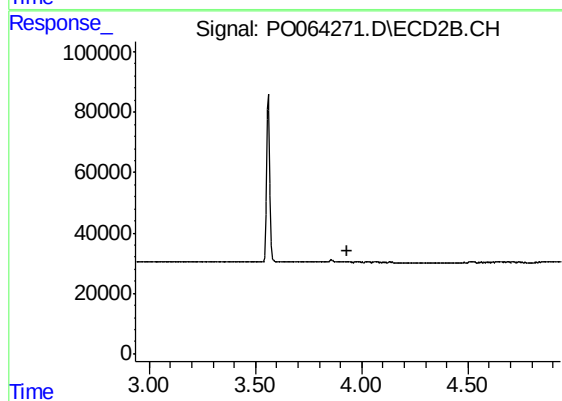

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 3.935 min
Response: 0
Conc: N.D.

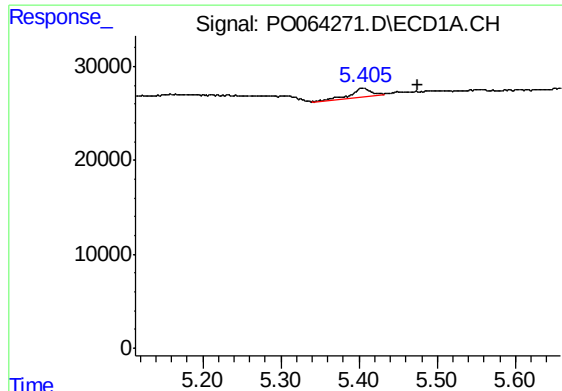

#21 AR-1248-1


R.T.: 5.406 min
Delta R.T.: -0.070 min
Response: 14387
Conc: 25.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-20-S

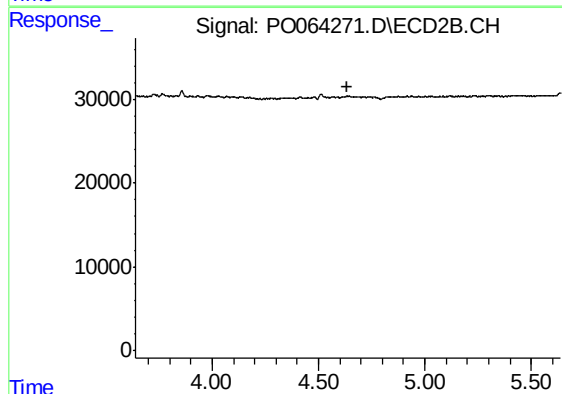


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.638 min
Response: 0
Conc: N.D.

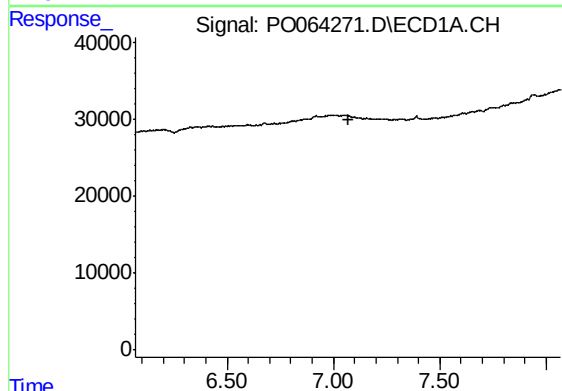


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 7.069 min
Response: 0
Conc: N.D.

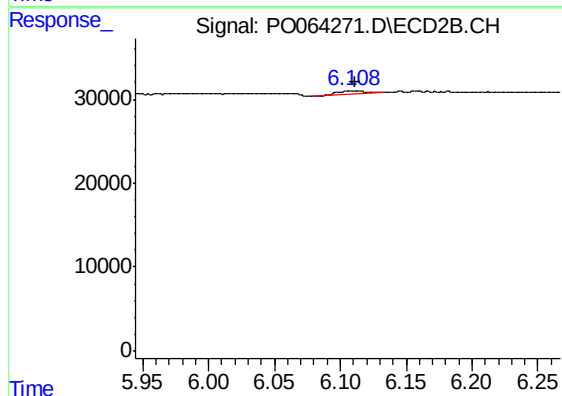

#31 AR-1260-1


R.T.: 6.108 min
Delta R.T.: -0.004 min
Response: 6459
Conc: 3.68 ng/ml

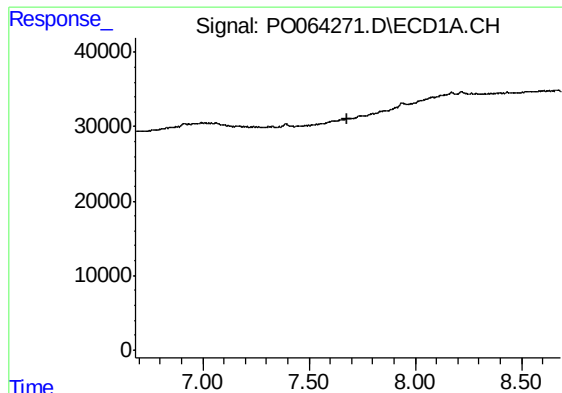

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.683 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-20-S

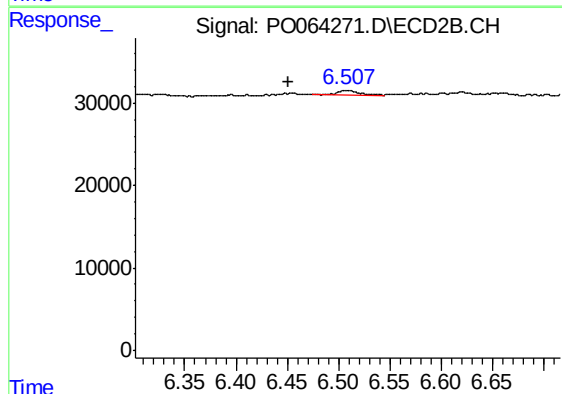


#33 AR-1260-3

R.T.: 6.507 min
Delta R.T.: 0.056 min
Response: 7996
Conc: 3.93 ng/ml

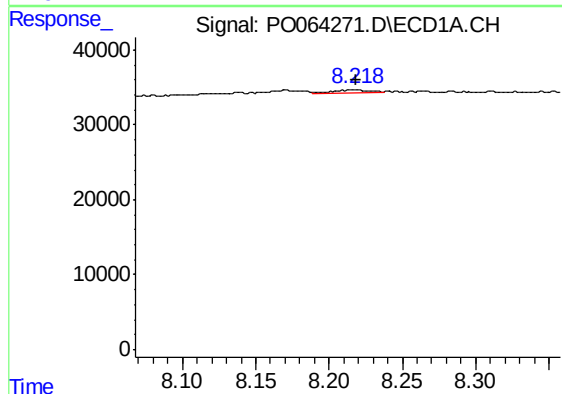


#35 AR-1260-5

R.T.: 8.218 min
Delta R.T.: 0.000 min
Response: 7538
Conc: 1.71 ng/ml

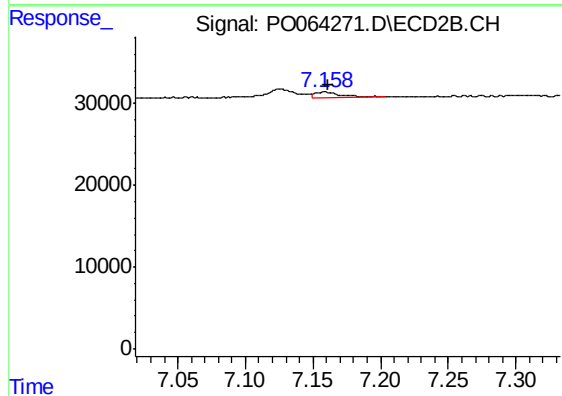

#35 AR-1260-5


R.T.: 7.159 min
Delta R.T.: -0.003 min
Response: 9654
Conc: 1.99 ng/ml

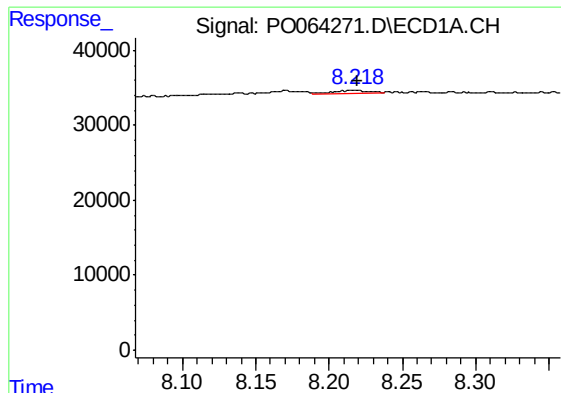

#37 AR-1262-2


R.T.: 8.218 min
Delta R.T.: -0.001 min
Response: 7538
Conc: 1.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-20-S

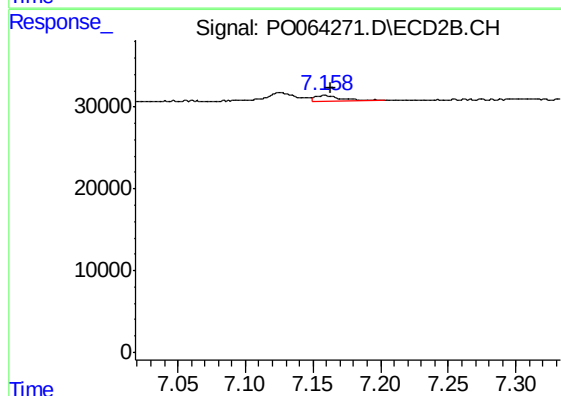


#37 AR-1262-2

R.T.: 7.159 min
Delta R.T.: -0.004 min
Response: 9654
Conc: 1.62 ng/ml

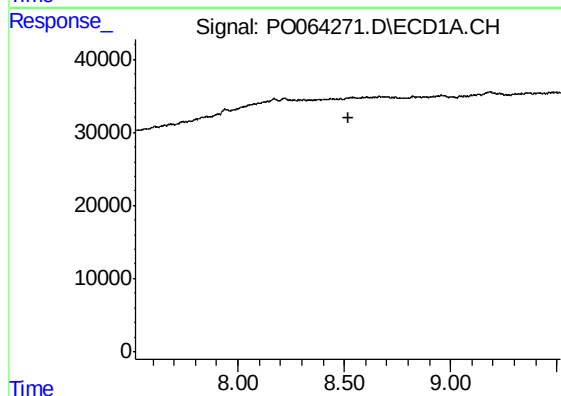


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.518 min
Response: 0
Conc: N.D.

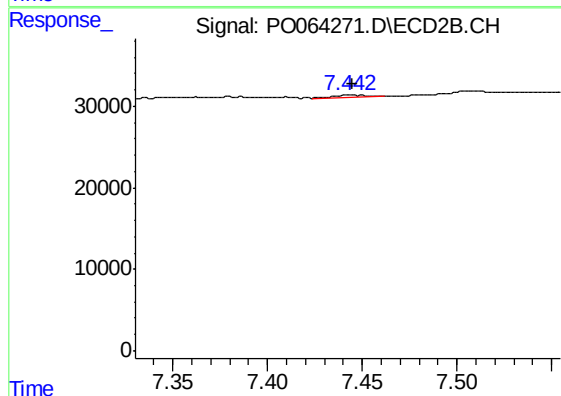

#38 AR-1262-3


R.T.: 7.443 min
Delta R.T.: -0.002 min
Response: 3304
Conc: 1.42 ng/ml

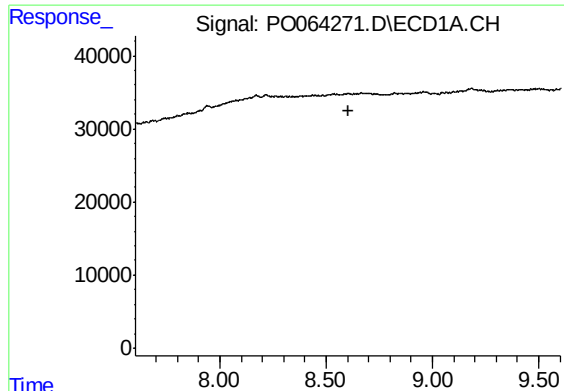

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.603 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-20-S

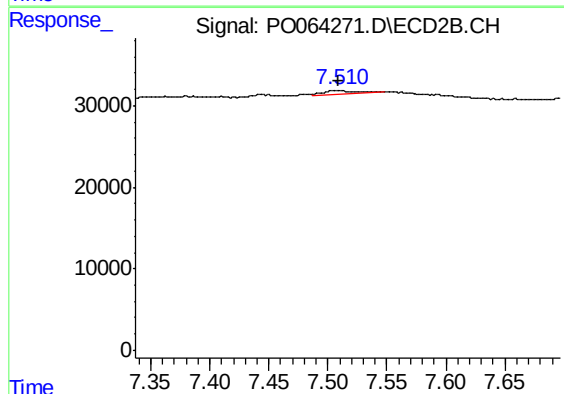


#39 AR-1262-4

R.T.: 7.510 min
Delta R.T.: 0.001 min
Response: 8670
Conc: 1.95 ng/ml

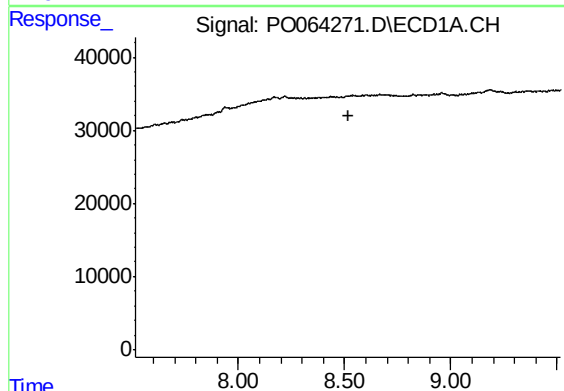


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.516 min
Response: 0
Conc: N.D.

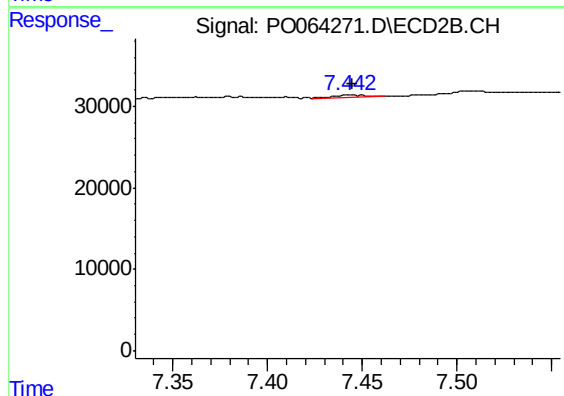

#41 AR-1268-1


R.T.: 7.443 min
Delta R.T.: -0.001 min
Response: 3304
Conc: 0.47 ng/ml

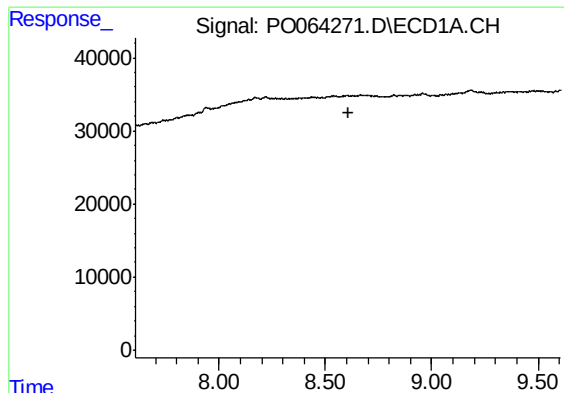

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.606 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-20-S

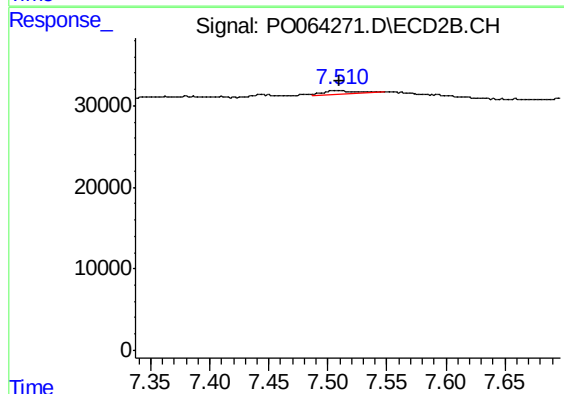


#42 AR-1268-2

R.T.: 7.510 min
Delta R.T.: 0.000 min
Response: 8670
Conc: 1.35 ng/ml

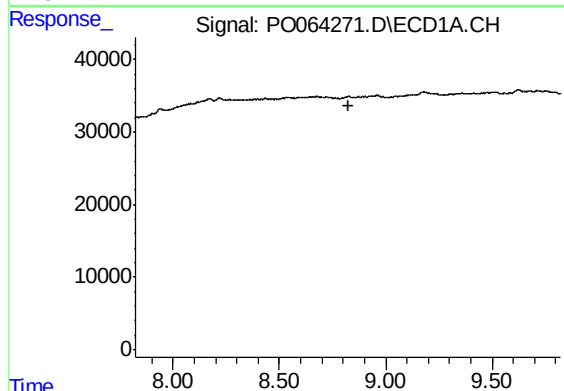


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.823 min
Response: 0
Conc: N.D.

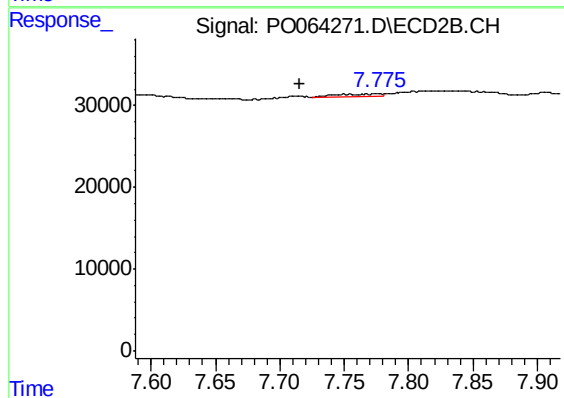

#43 AR-1268-3


R.T.: 7.775 min
Delta R.T.: 0.060 min
Response: 10069
Conc: 1.92 ng/ml

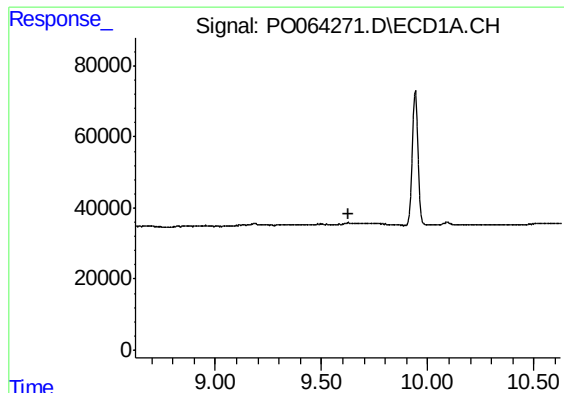

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.624 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-20-S

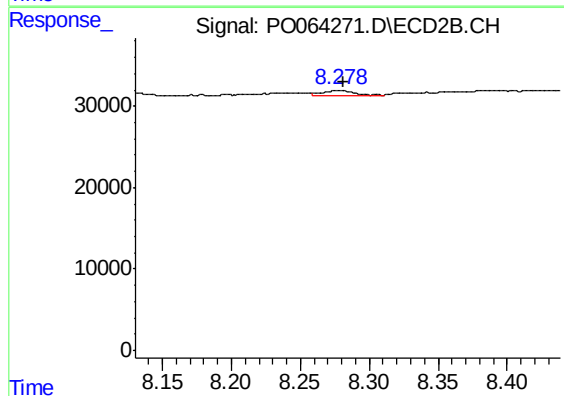

#45 AR-1268-5

R.T.: 8.278 min
Delta R.T.: -0.003 min
Response: 9432
Conc: 0.57 ng/ml