

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0120219\
 Data File : P0064264.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Dec 2019 17:24
 Operator : SM/AJ
 Sample : K6084-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 30735

Manual Integrations
 APPROVED

mohammad
 12/3/2019 1:33:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 01:34:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 28 01:28:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.335	3.560	4735240	3053528	159.891m	128.380
2)	SA Decachlor...	9.943	8.526	744099	705482	18.156	17.270

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120219\
Data File : PO064264.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Dec 2019 17:24
Operator : SM/AJ
Sample : K6084-03
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
30735


Manual Integrations
APPROVED

mohammad
12/3/2019 1:33:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 01:34:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112719.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 28 01:28:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

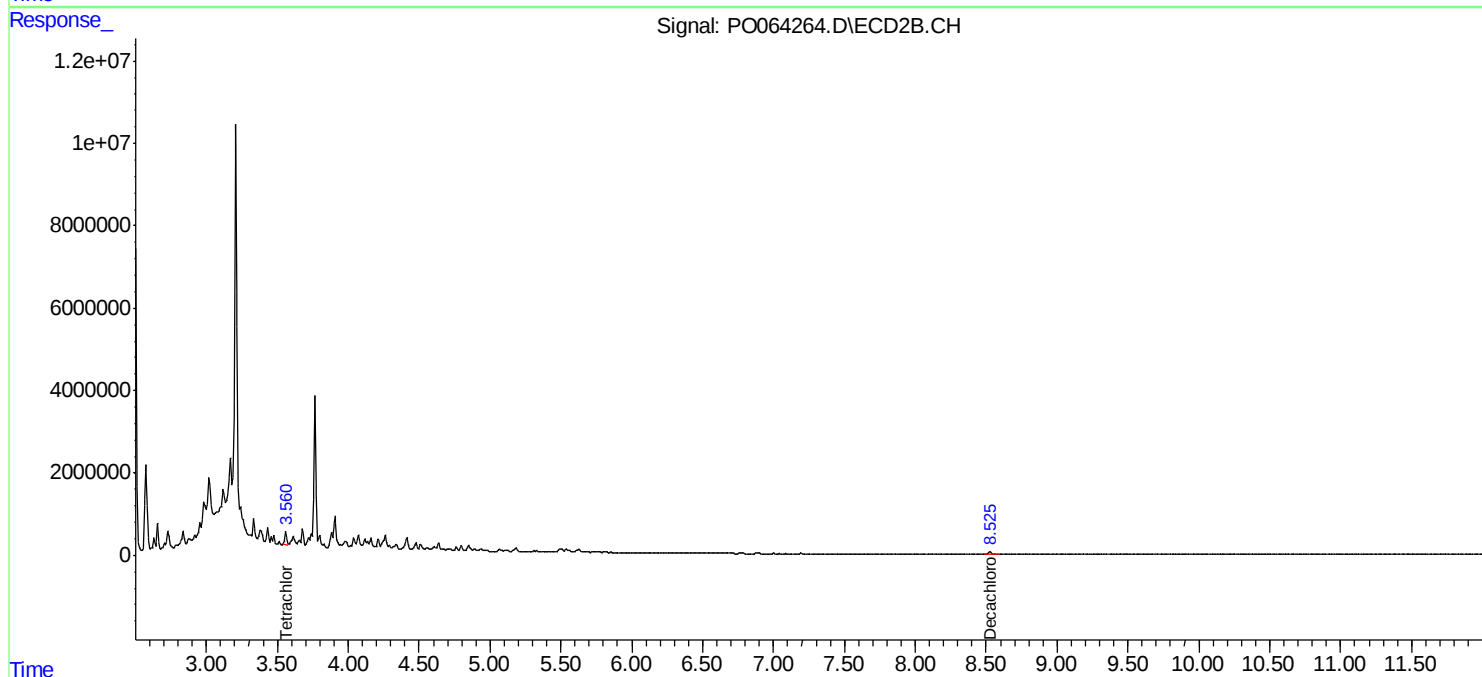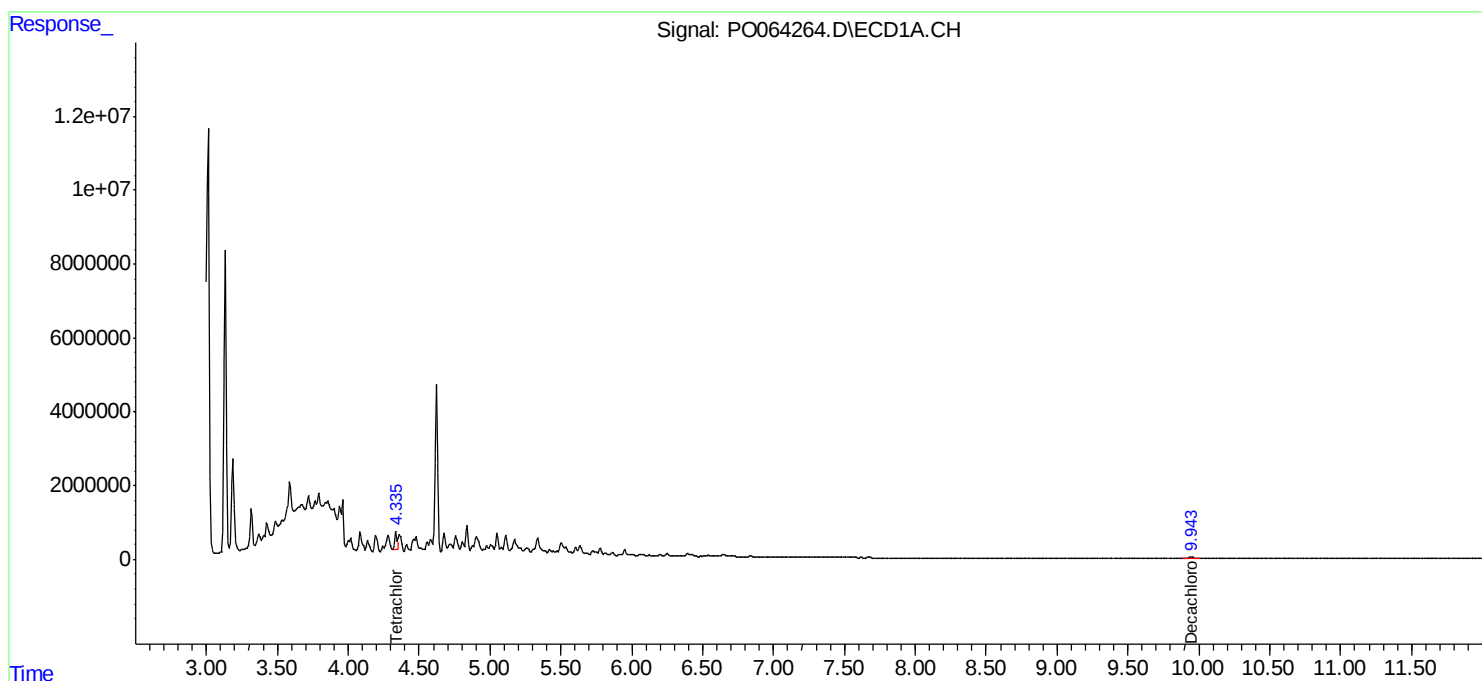

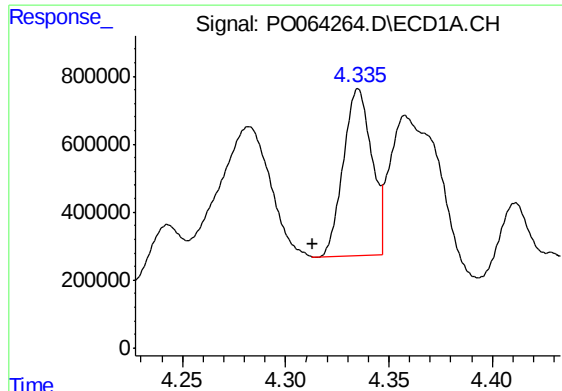


#1 Tetrachloro-m-xylene

R.T.: 4.335 min
Delta R.T.: 0.022 min
Response: 4735240
Conc: 159.89 ng/ml m

Instrument :
ECD_O
ClientSampleId :
30735


Manual Integrations
APPROVED

mohammad
12/3/2019 1:33:26 PM

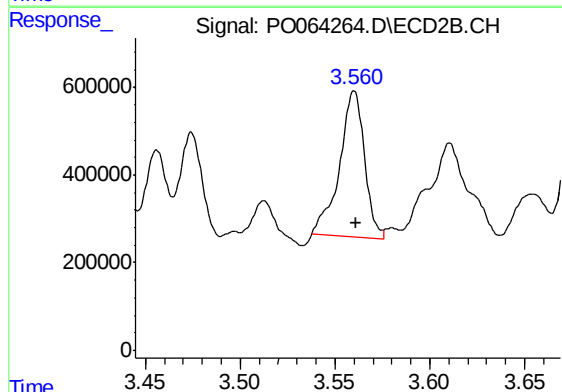


#1 Tetrachloro-m-xylene

R.T.: 3.560 min
Delta R.T.: -0.001 min
Response: 3053528
Conc: 128.38 ng/ml

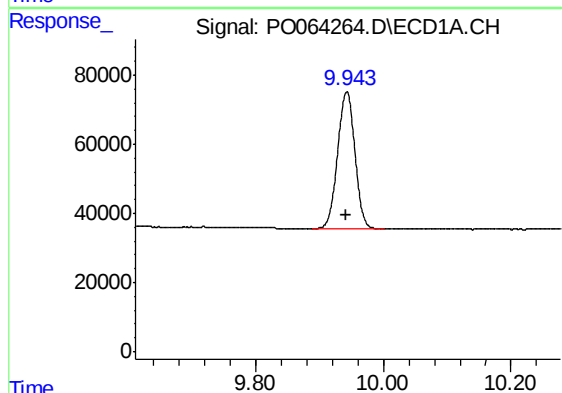

#2 Decachlorobiphenyl

R.T.: 9.943 min
Delta R.T.: 0.002 min
Response: 744099
Conc: 18.16 ng/ml

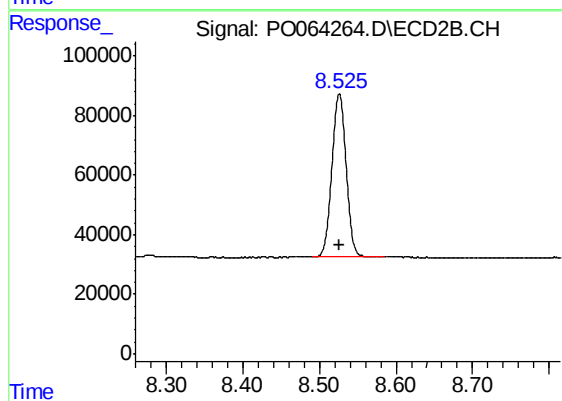

#2 Decachlorobiphenyl

R.T.: 8.526 min
Delta R.T.: 0.000 min
Response: 705482
Conc: 17.27 ng/ml