

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120221\
 Data File : PO083396.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Dec 2021 18:40
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 02:25:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Nov 20 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.947	3.949	2164208	709052	24.661	23.261
2)	SA Decachlor...	11.039	9.255	1598703	701891	24.313	23.348
Target Compounds							
5)	L1 AR-1016-3	6.364	0.000	18743	0	7.470	N.D. #
8)	L2 AR-1221-1	5.190f	0.000	59426	0	62.711	N.D. #
9)	L2 AR-1221-2	5.303	0.000	25795	0	38.366	N.D. #
10)	L2 AR-1221-3	0.000	4.393	0	24275	N.D.	26.841 #
11)	L3 AR-1232-1	0.000	4.393	0	24275	N.D.	31.667 #
18)	L4 AR-1242-3	6.364	0.000	18743	0	10.037	N.D. #
28)	L6 AR-1254-3	7.835f	0.000	26211	0	6.103	N.D. #
32)	L7 AR-1260-2	8.273f	0.000	10934	0	2.913	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120221\
Data File : PO083396.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Dec 2021 18:40
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 02:25:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Nov 20 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

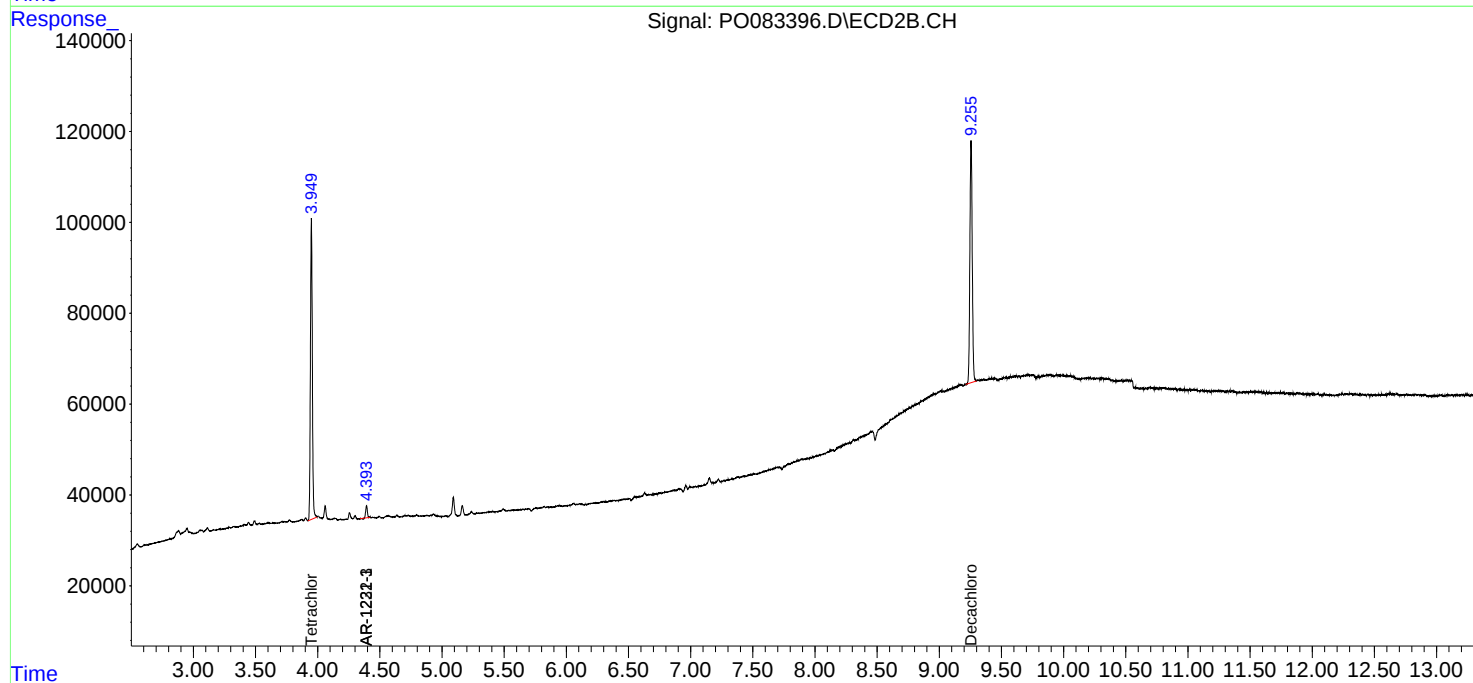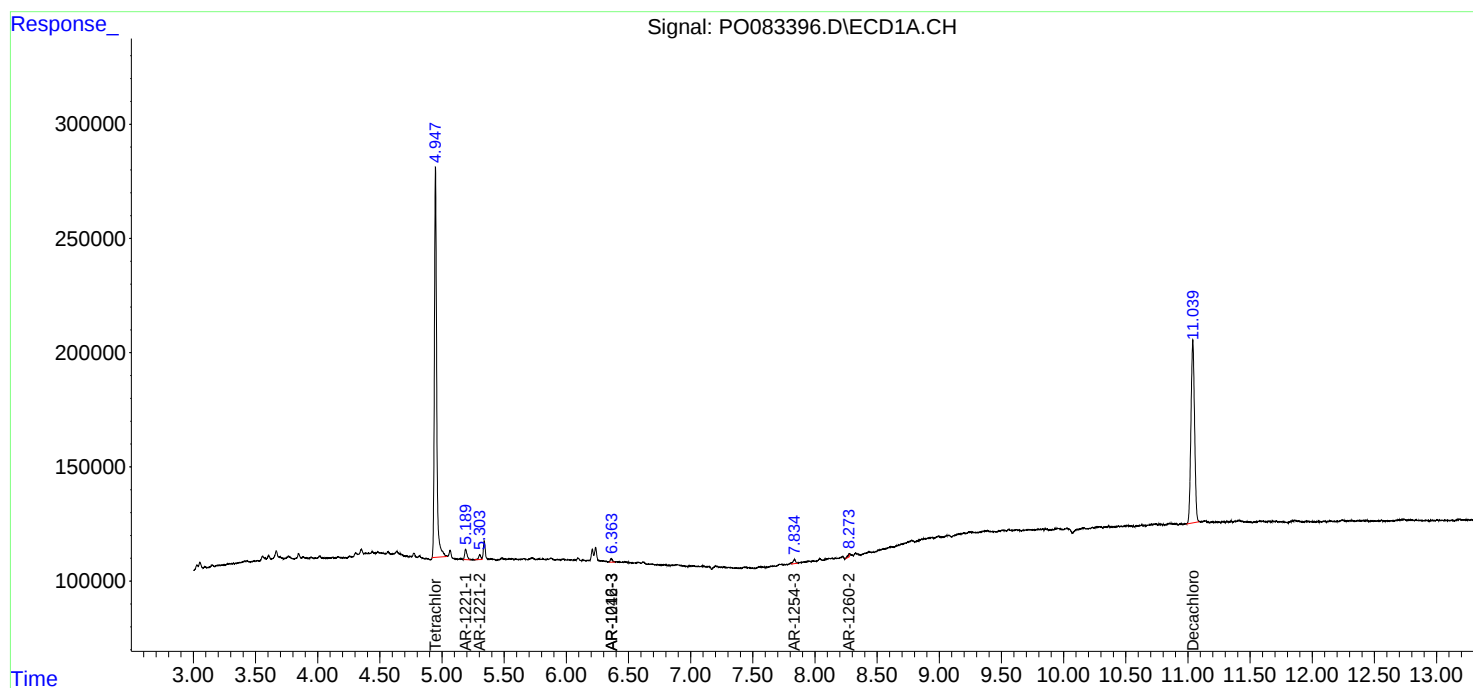


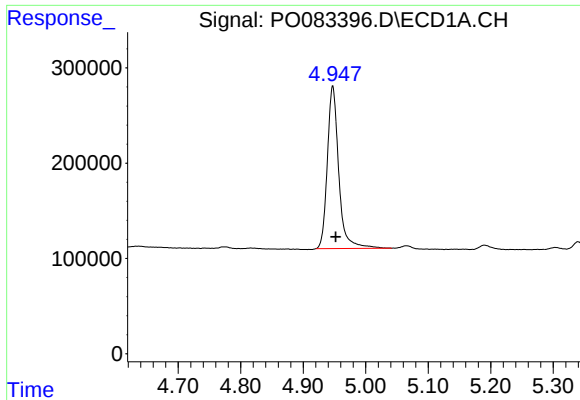

#1 Tetrachloro-m-xylene


R.T.: 4.947 min
Delta R.T.: -0.005 min
Response: 2164208
Conc: 24.66 ng/ml

Instrument :
ECD_O
ClientSampleId :

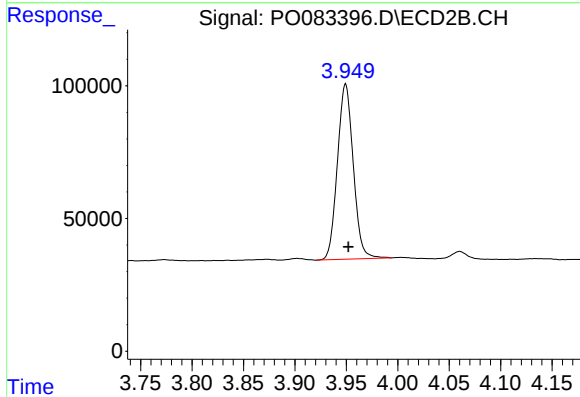


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: -0.003 min
Response: 709052
Conc: 23.26 ng/ml

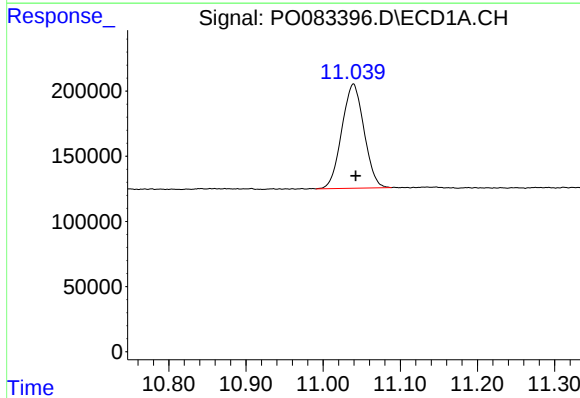


#2 Decachlorobiphenyl

R.T.: 11.039 min
Delta R.T.: -0.003 min
Response: 1598703
Conc: 24.31 ng/ml

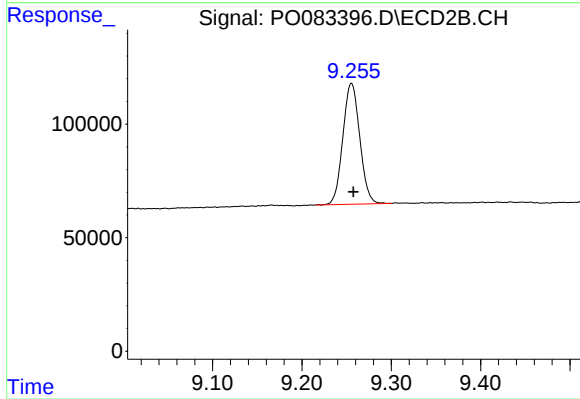

#2 Decachlorobiphenyl


R.T.: 9.255 min
Delta R.T.: -0.002 min
Response: 701891
Conc: 23.35 ng/ml

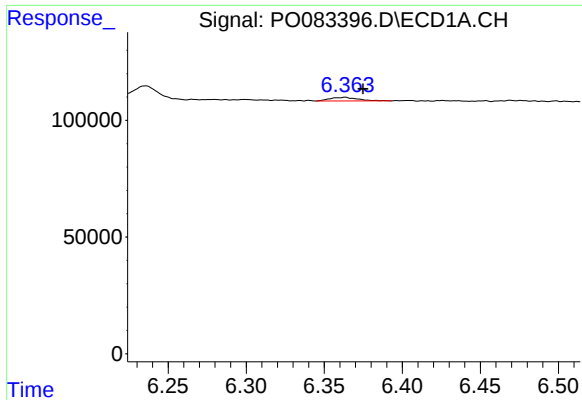

#5 AR-1016-3


R.T.: 6.364 min
Delta R.T.: -0.011 min
Response: 18743
Conc: 7.47 ng/ml

Instrument :
ECD_O
ClientSampleId :

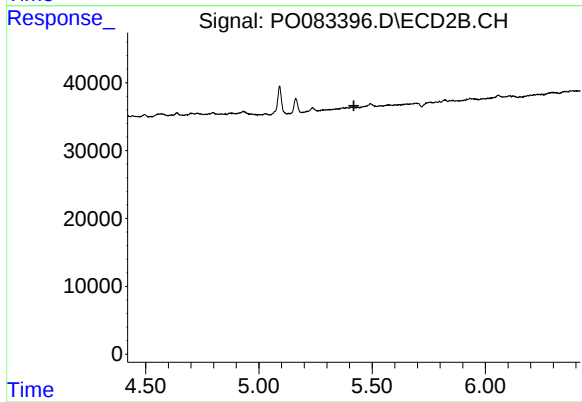


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 5.419 min
Response: 0
Conc: N.D.

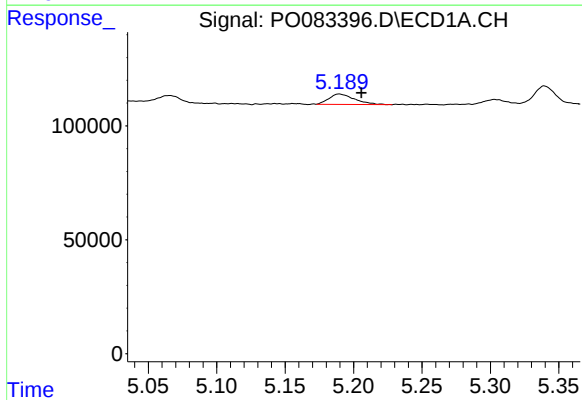


#8 AR-1221-1

R.T.: 5.190 min
Delta R.T.: -0.016 min
Response: 59426
Conc: 62.71 ng/ml

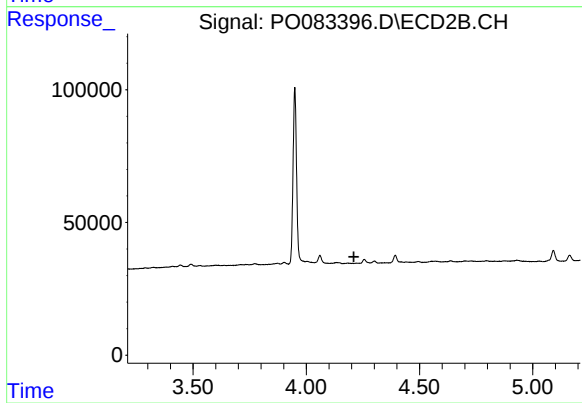

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 4.210 min
Response: 0
Conc: N.D.

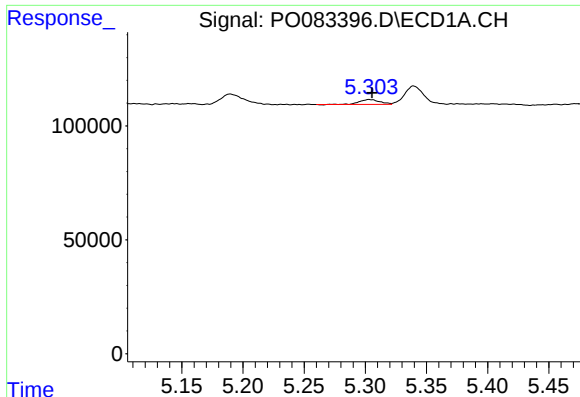

#9 AR-1221-2


R.T.: 5.303 min
Delta R.T.: -0.003 min
Response: 25795
Conc: 38.37 ng/ml

Instrument :
ECD_O
ClientSampleId :

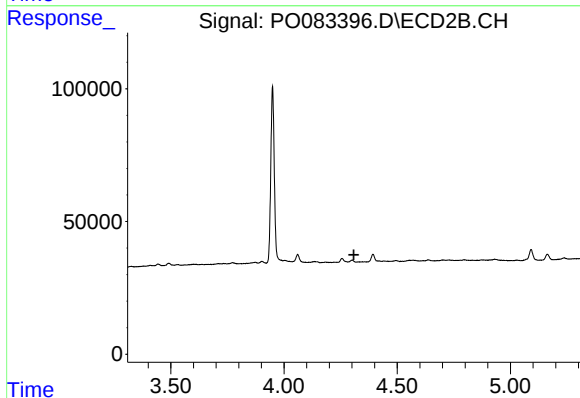


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.309 min
Response: 0
Conc: N.D.

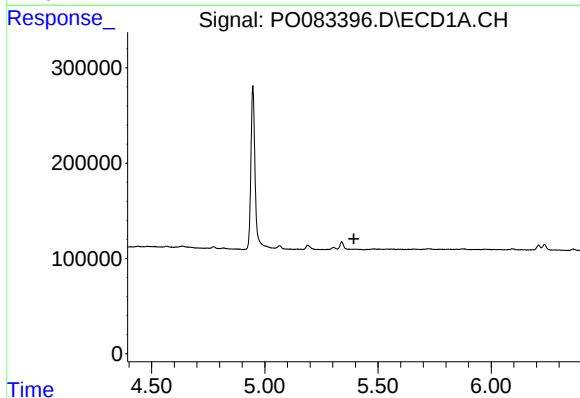


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 5.394 min
Response: 0
Conc: N.D.

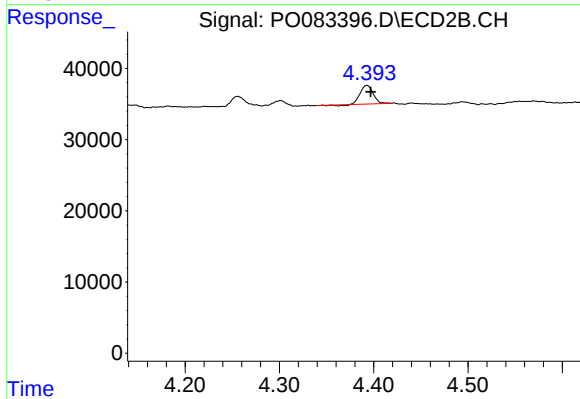

#10 AR-1221-3


R.T.: 4.393 min
Delta R.T.: -0.004 min
Response: 24275
Conc: 26.84 ng/ml

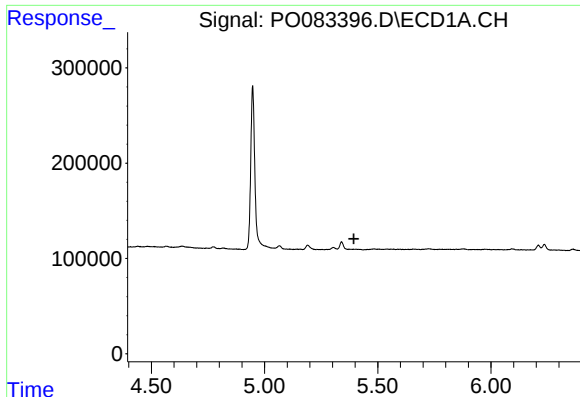

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 5.394 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

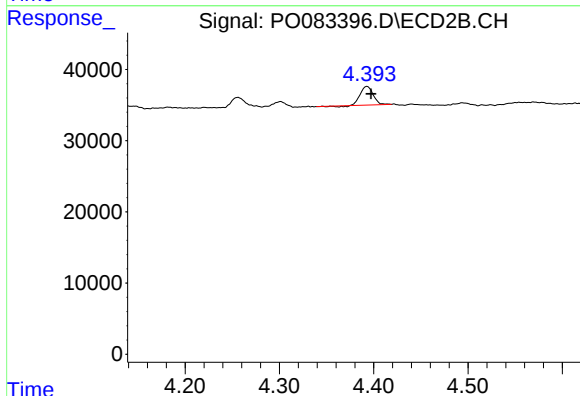


#11 AR-1232-1

R.T.: 4.393 min
Delta R.T.: -0.004 min
Response: 24275
Conc: 31.67 ng/ml

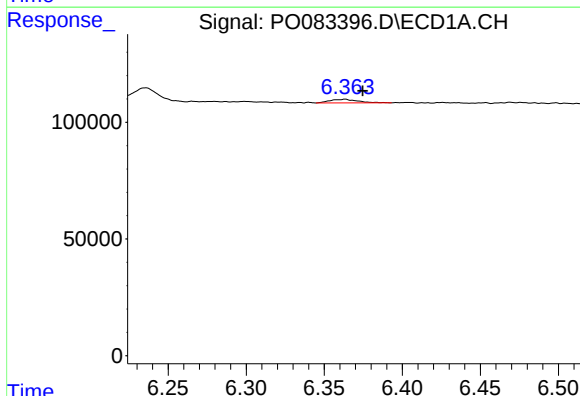


#18 AR-1242-3

R.T.: 6.364 min
Delta R.T.: -0.011 min
Response: 18743
Conc: 10.04 ng/ml

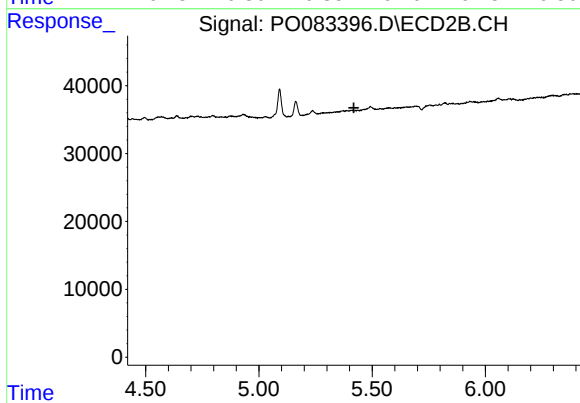

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T.: 5.420 min
Response: 0
Conc: N.D.

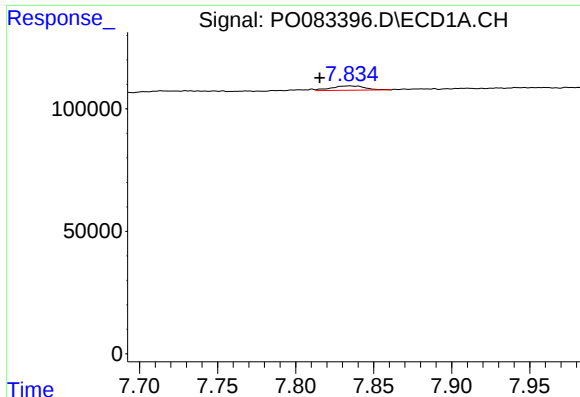

#28 AR-1254-3


R.T.: 7.835 min
Delta R.T.: 0.019 min
Response: 26211
Conc: 6.10 ng/ml

Instrument :
ECD_O
ClientSampleId :

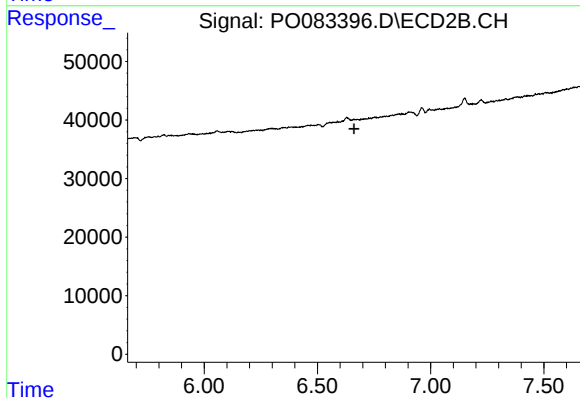


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.661 min
Response: 0
Conc: N.D.

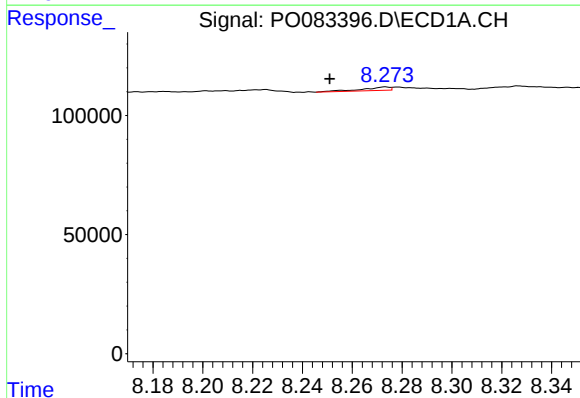

#32 AR-1260-2

R.T.: 8.273 min
Delta R.T.: 0.022 min
Response: 10934
Conc: 2.91 ng/ml

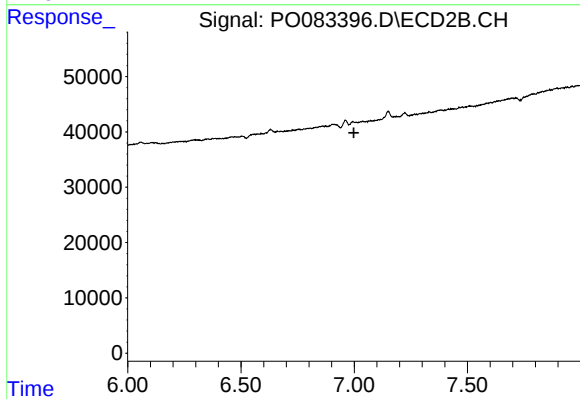

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.999 min
Response: 0
Conc: N.D.