

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120221\
 Data File : PO083383.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Dec 2021 14:21
 Operator : AJ\MA
 Sample : PB141115BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB141115BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 02:19:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Nov 20 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.947	3.950	1958500	655737	22.317	21.512
2)	SA Decachlor...	11.037	9.256	1492494	686810	22.697	22.847

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120221\
Data File : P0083383.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Dec 2021 14:21
Operator : AJ\MA
Sample : PB141115BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB141115BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 02:19:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Nov 20 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

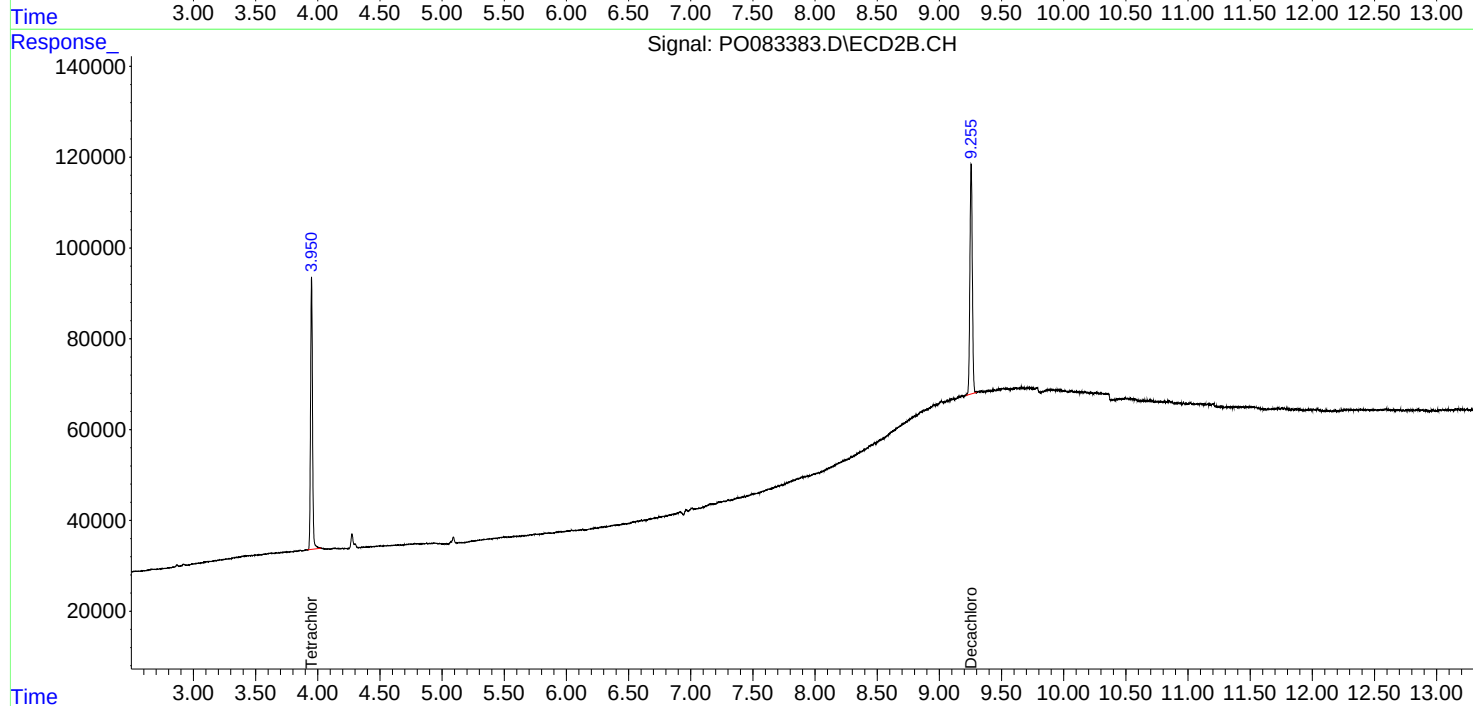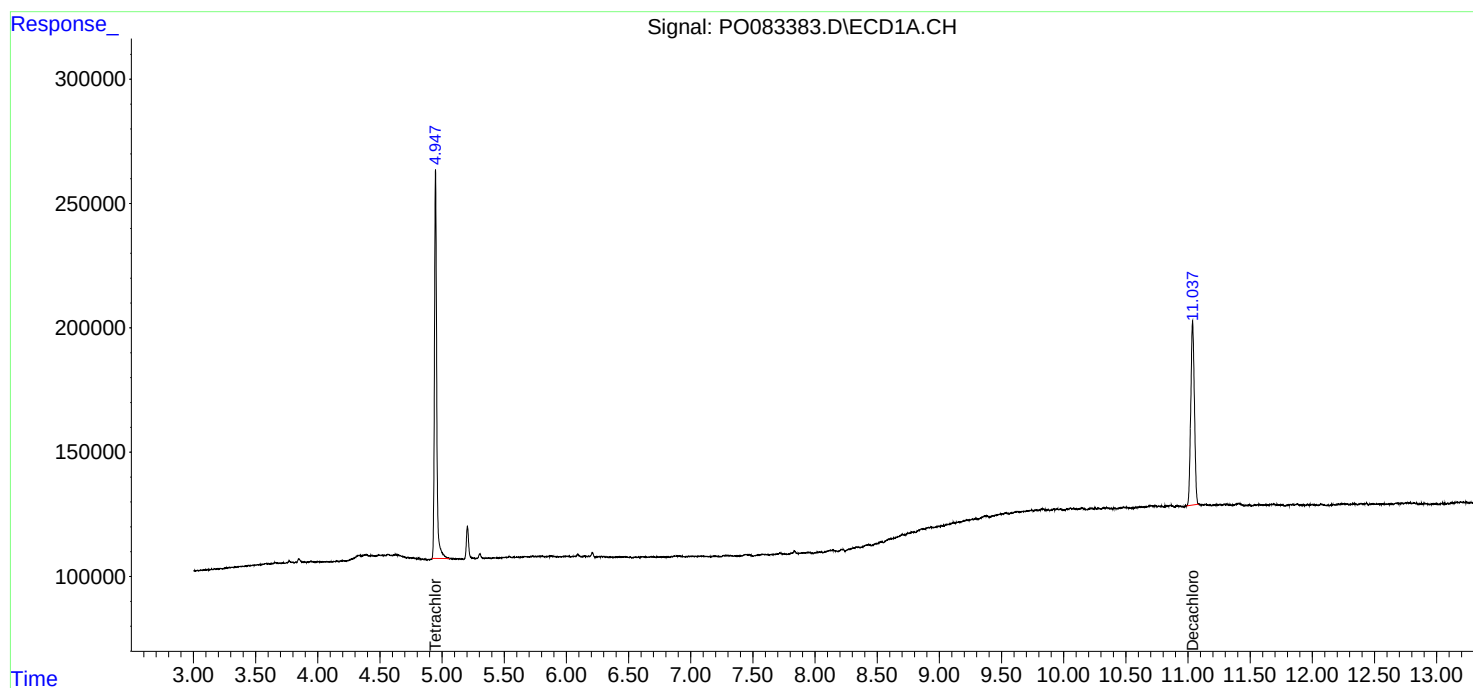


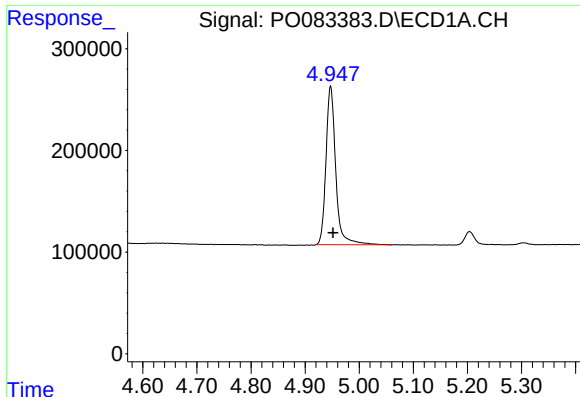

#1 Tetrachloro-m-xylene


R.T.: 4.947 min
Delta R.T.: -0.005 min
Response: 1958500
Conc: 22.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB141115BL

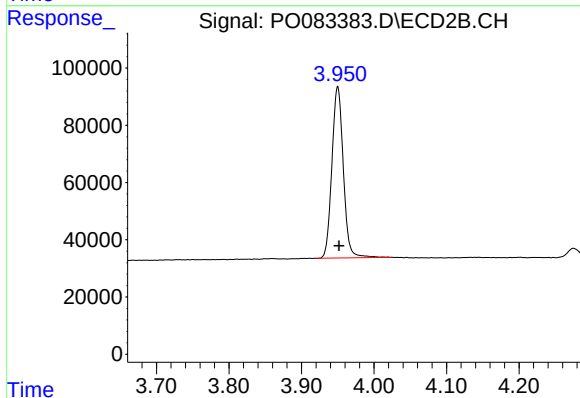


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: -0.002 min
Response: 655737
Conc: 21.51 ng/ml

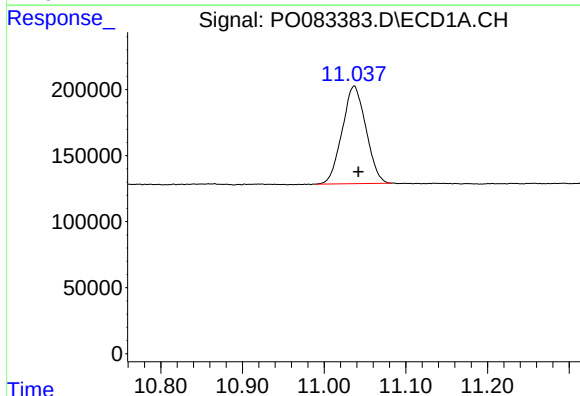

#2 Decachlorobiphenyl

R.T.: 11.037 min
Delta R.T.: -0.005 min
Response: 1492494
Conc: 22.70 ng/ml

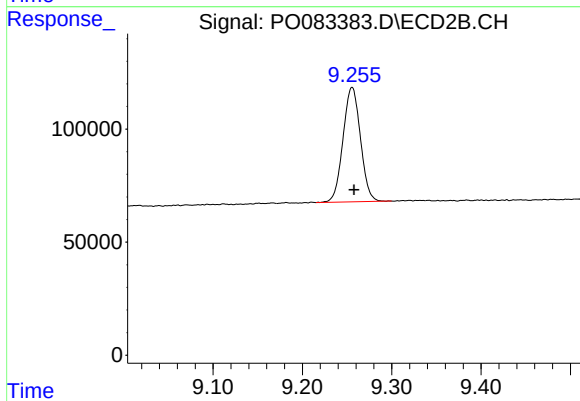

#2 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: -0.002 min
Response: 686810
Conc: 22.85 ng/ml