

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120221\
 Data File : PO083401.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Dec 2021 20:07
 Operator : AJ\MA
 Sample : M4899-01 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 01-A-01-B-01-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 02:27:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Nov 20 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.947	3.948	227142	80746	2.588	2.649m
2) SA Decachlor...	11.038	9.256	167593	76465	2.549m	2.544m

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120221\
Data File : P0083401.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Dec 2021 20:07
Operator : AJ\MA
Sample : M4899-01 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
01-A-01-B-01-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 02:27:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Nov 20 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

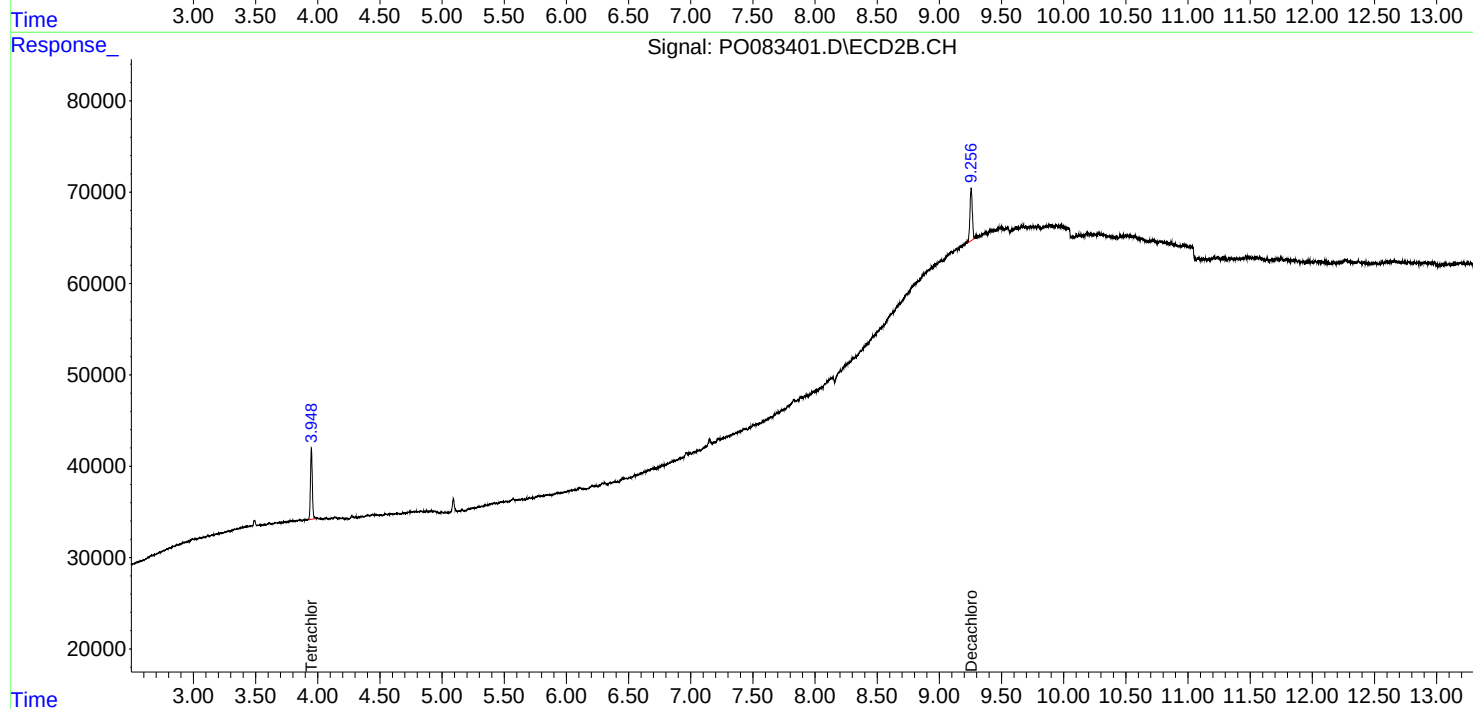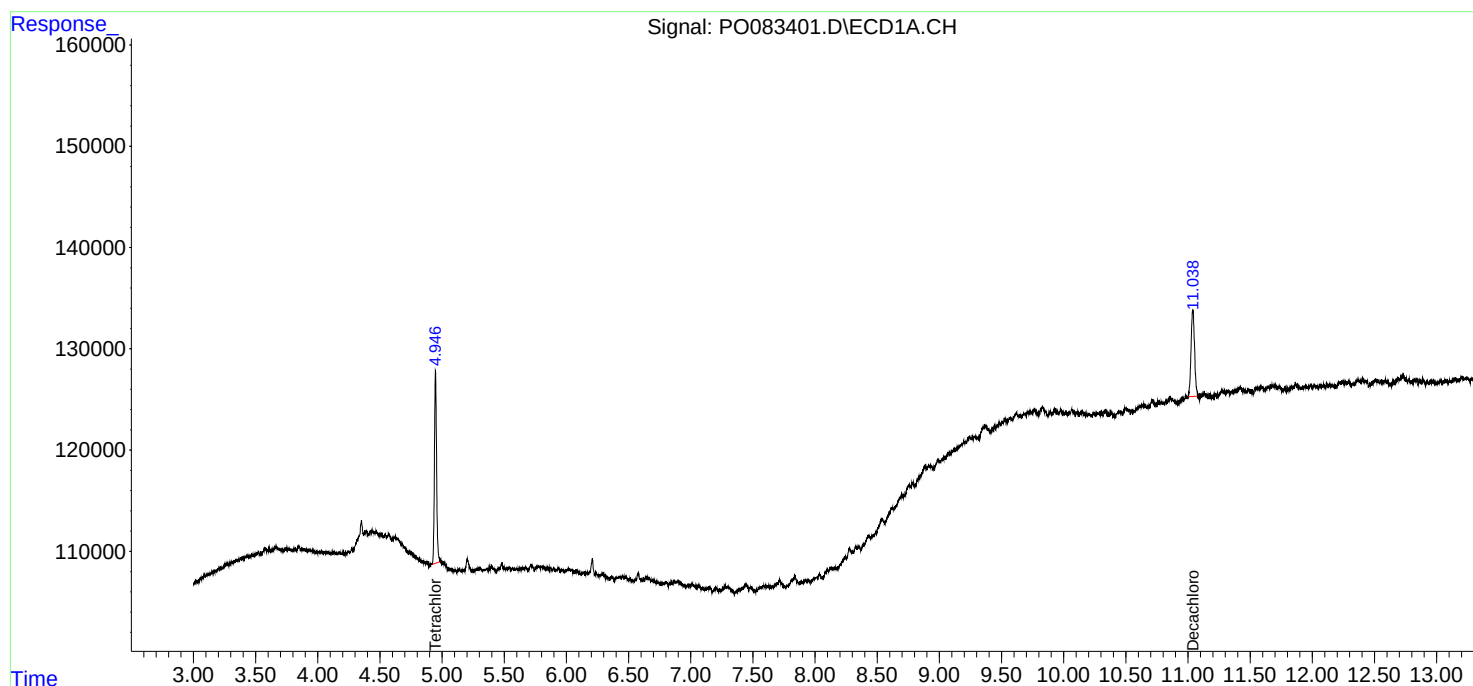


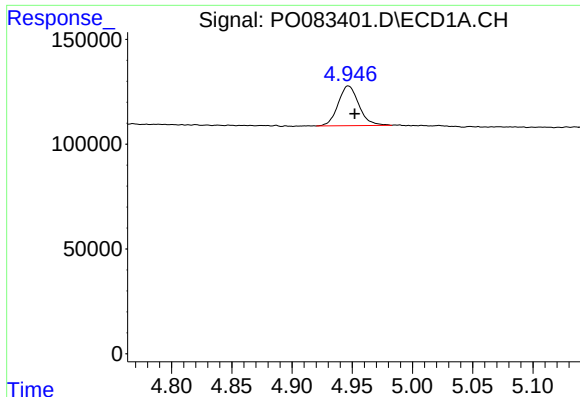

#1 Tetrachloro-m-xylene


R.T.: 4.947 min
Delta R.T.: -0.005 min
Response: 227142
Conc: 2.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
01-A-01-B-01-C

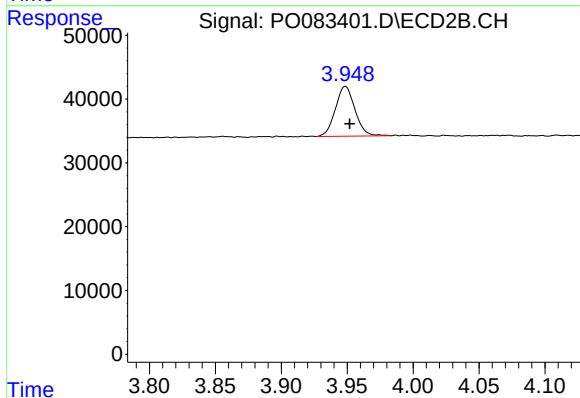


#1 Tetrachloro-m-xylene

R.T.: 3.948 min
Delta R.T.: -0.004 min
Response: 80746
Conc: 2.65 ng/ml m

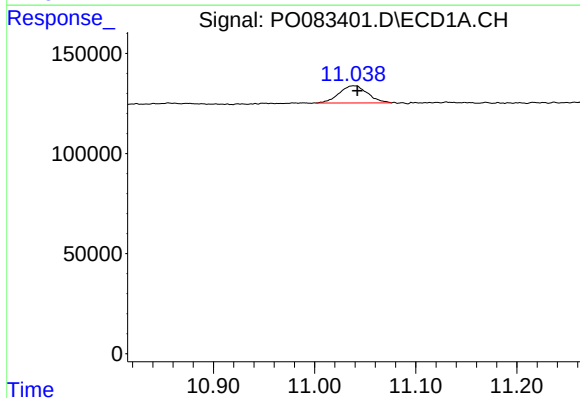

#2 Decachlorobiphenyl

R.T.: 11.038 min
Delta R.T.: -0.004 min
Response: 167593
Conc: 2.55 ng/ml m

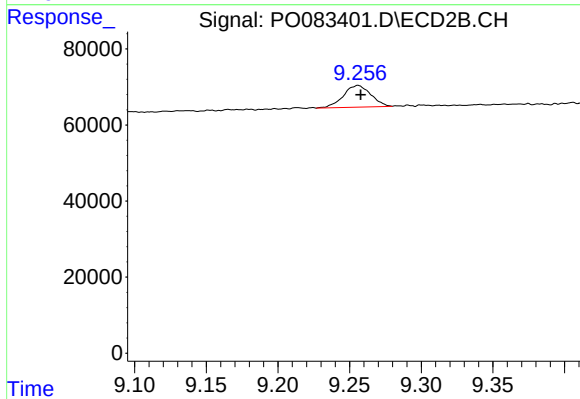

#2 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: -0.002 min
Response: 76465
Conc: 2.54 ng/ml m