

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120225\
 Data File : PO115532.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2025 21:33
 Operator : YP/AJ
 Sample : Q3748-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AU-05-12-1-2025

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 12/03/2025
 Supervised By :Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 01:23:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 05 06:00:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.336	3.640	180.7E6	109.2E6	25.669	24.455
2) SA Decachlor...	9.916	8.625	114.2E6	87990858	25.826m	22.540

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120225\
Data File : PO115532.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2025 21:33
Operator : YP/AJ
Sample : Q3748-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AU-05-12-1-2025


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 01:23:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 05 06:00:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

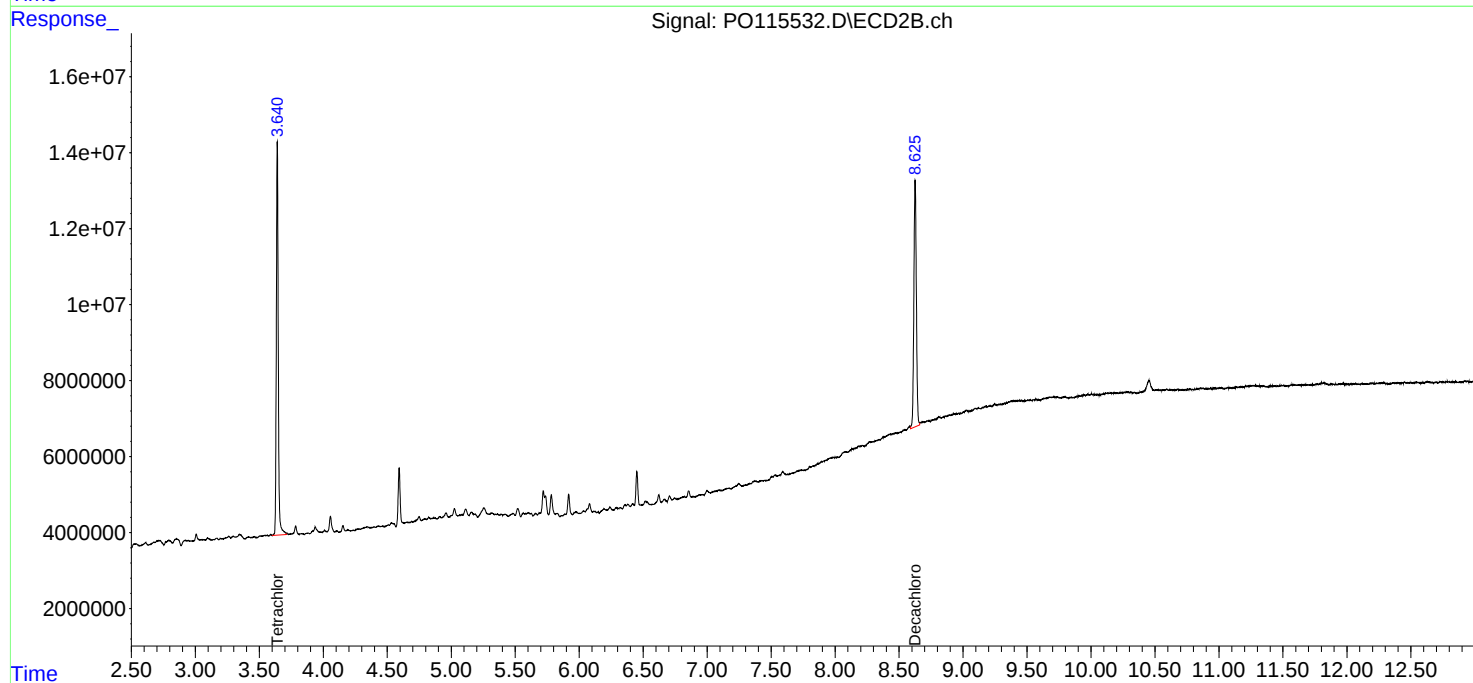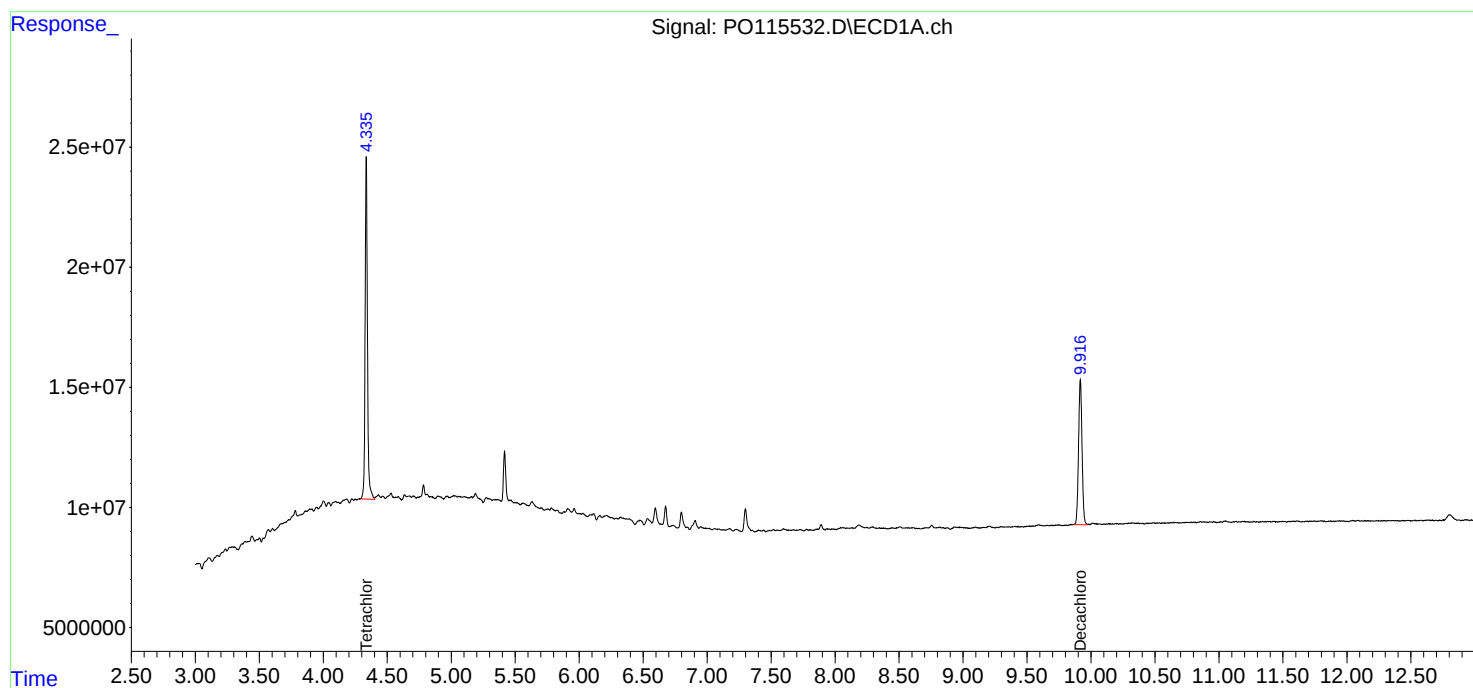

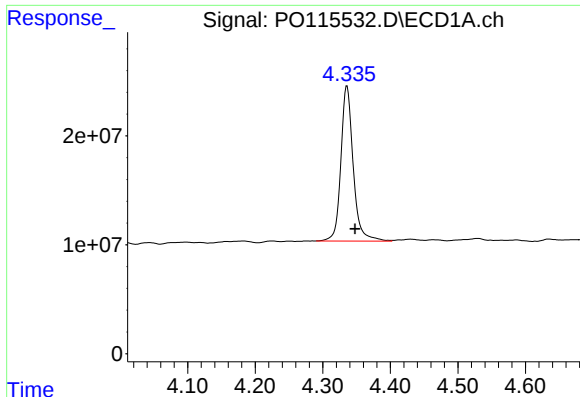


#1 Tetrachloro-m-xylene

R.T.: 4.336 min
Delta R.T.: -0.012 min
Response: 180664223
Conc: 25.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
AU-05-12-1-2025


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/03/2025
Supervised By :Sohil Jodhani 12/03/2025

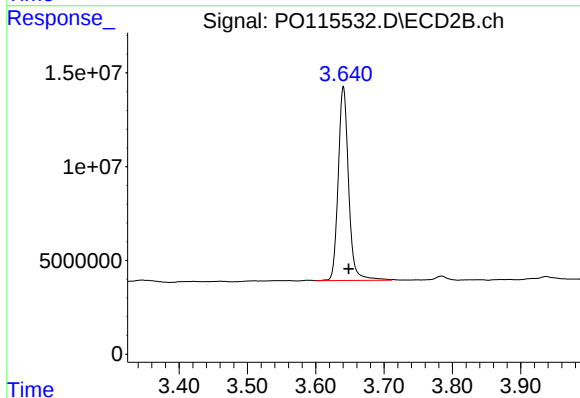


#1 Tetrachloro-m-xylene

R.T.: 3.640 min
Delta R.T.: -0.008 min
Response: 109234460
Conc: 24.45 ng/ml

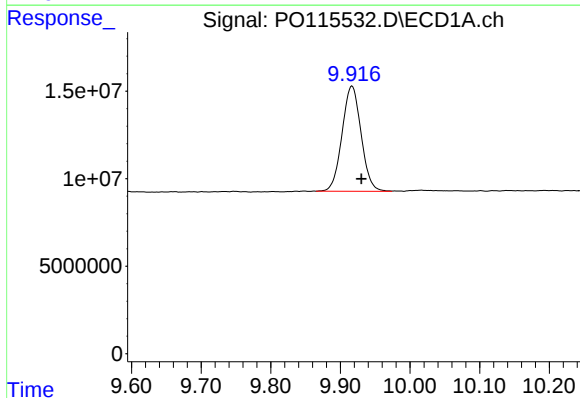

#2 Decachlorobiphenyl

R.T.: 9.916 min
Delta R.T.: -0.014 min
Response: 114157002
Conc: 25.83 ng/ml m

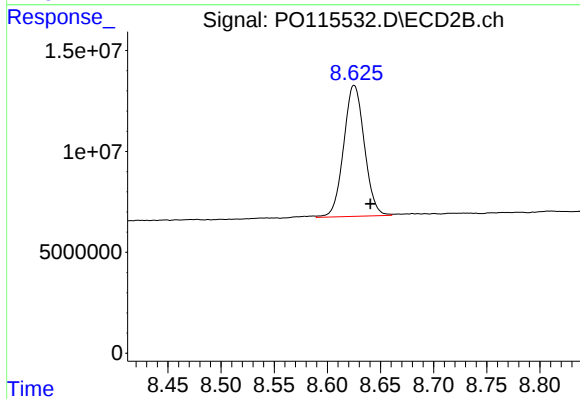

#2 Decachlorobiphenyl

R.T.: 8.625 min
Delta R.T.: -0.015 min
Response: 87990858
Conc: 22.54 ng/ml