

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO120321\
 Data File : PO083444.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Dec 2021 21:09
 Operator : AJ\MA
 Sample : M4927-13
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 23:10:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO111921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Nov 20 02:49:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.944	3.946	2599966	882379	29.626	28.948
2) SA Decachlor...	11.027f	9.250	1968090	888920	29.930	29.570
Target Compounds						
8) L2 AR-1221-1	5.199	0.000	391366	0	412.998	N.D. #
9) L2 AR-1221-2	5.299	0.000	33784	0	50.247	N.D. #
27) L6 AR-1254-2	7.428	0.000	39718	0	9.547	N.D. #
28) L6 AR-1254-3	7.809	0.000	40155	0	9.349	N.D. #
30) L6 AR-1254-5	8.536	0.000	27153	0	8.470	N.D. #
32) L7 AR-1260-2	8.242	0.000	20731	0	5.523	N.D. #
33) L7 AR-1260-3	8.608	0.000	12618	0	4.410	N.D. #
36) L8 AR-1262-1	8.608	0.000	12618	0	3.383	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120321\
Data File : PO083444.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Dec 2021 21:09
Operator : AJ\MA
Sample : M4927-13
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 23:10:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Nov 20 02:49:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

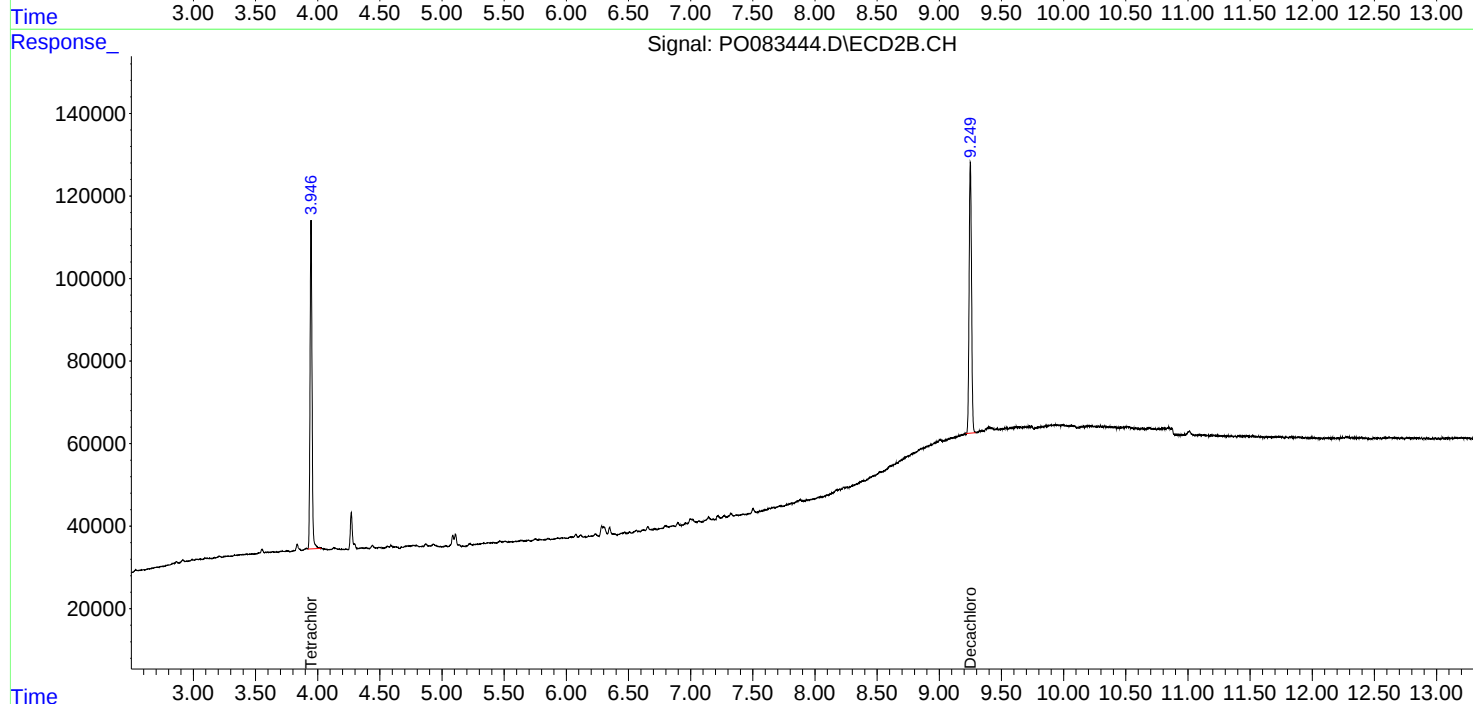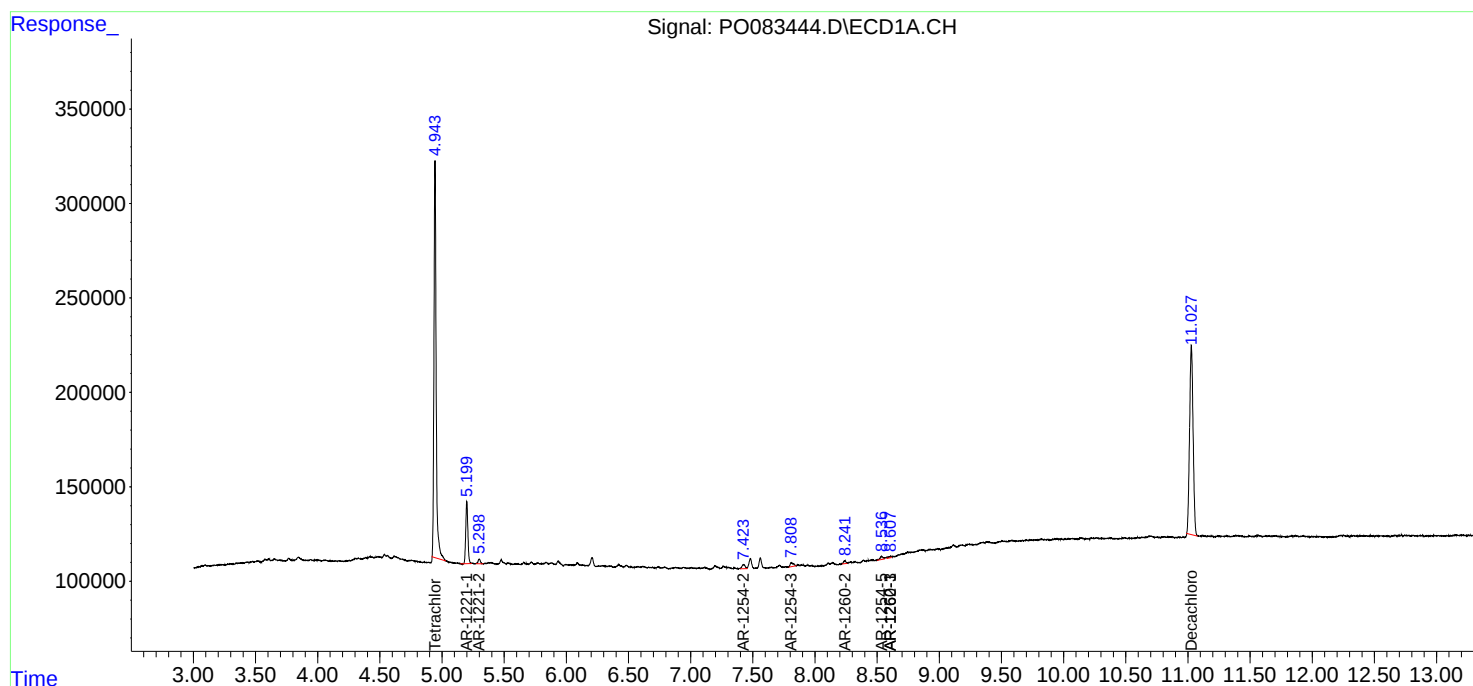


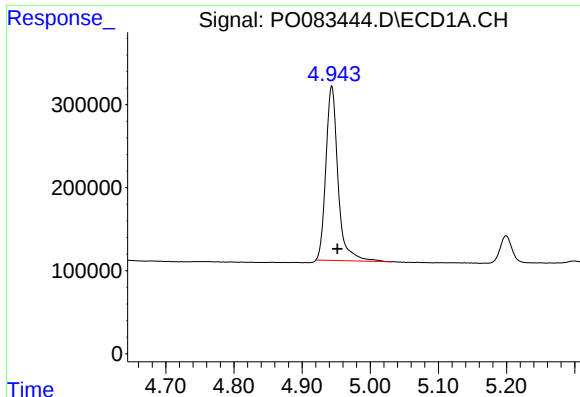

#1 Tetrachloro-m-xylene


R.T.: 4.944 min
Delta R.T.: -0.008 min
Response: 2599966
Conc: 29.63 ng/ml

Instrument :
ECD_O
ClientSampleId :

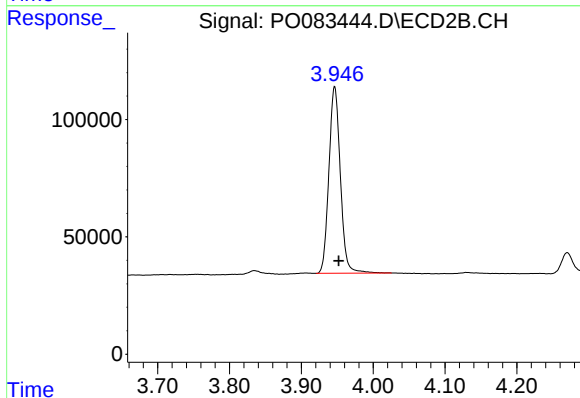


#1 Tetrachloro-m-xylene

R.T.: 3.946 min
Delta R.T.: -0.006 min
Response: 882379
Conc: 28.95 ng/ml

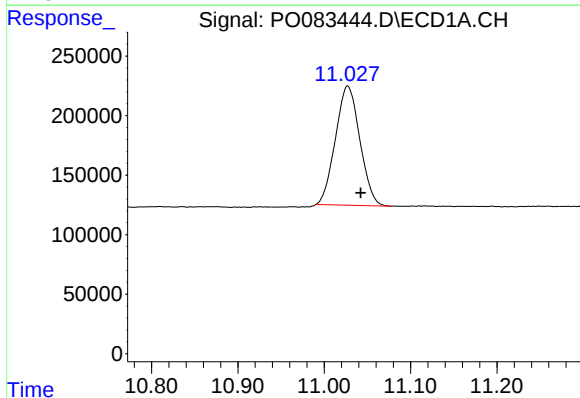


#2 Decachlorobiphenyl

R.T.: 11.027 min
Delta R.T.: -0.015 min
Response: 1968090
Conc: 29.93 ng/ml

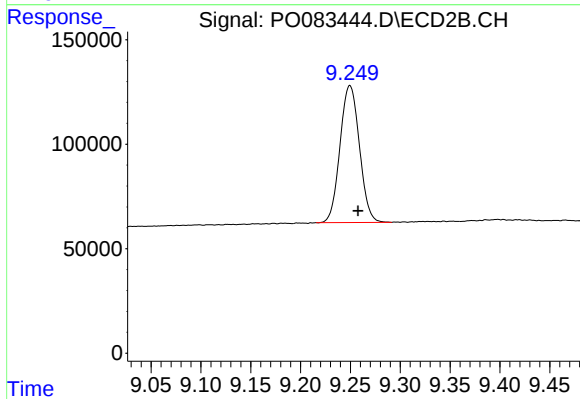

#2 Decachlorobiphenyl


R.T.: 9.250 min
Delta R.T.: -0.008 min
Response: 888920
Conc: 29.57 ng/ml

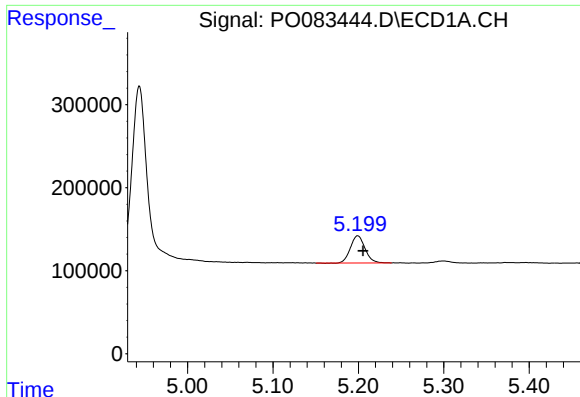

#8 AR-1221-1


R.T.: 5.199 min
Delta R.T.: -0.006 min
Response: 391366
Conc: 413.00 ng/ml

Instrument :
ECD_O
ClientSampleId :

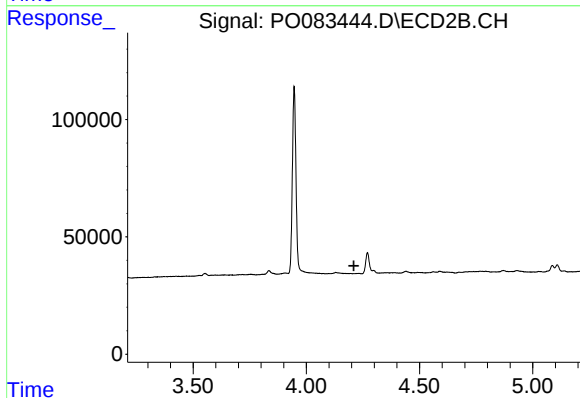


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.210 min
Response: 0
Conc: N.D.

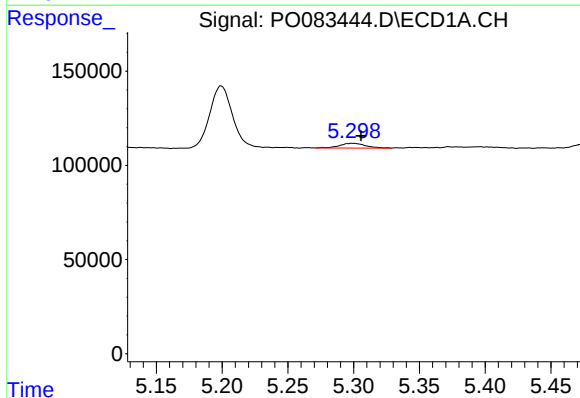


#9 AR-1221-2

R.T.: 5.299 min
Delta R.T.: -0.007 min
Response: 33784
Conc: 50.25 ng/ml

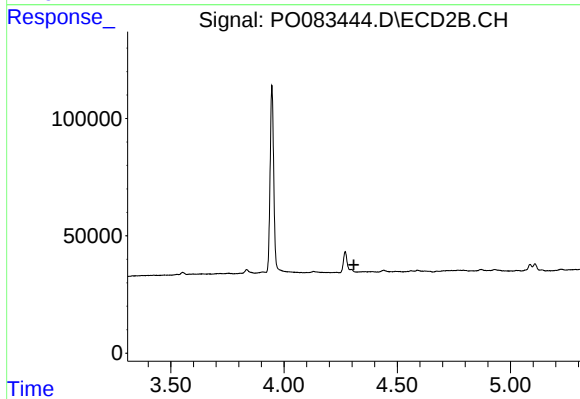

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.309 min
Response: 0
Conc: N.D.

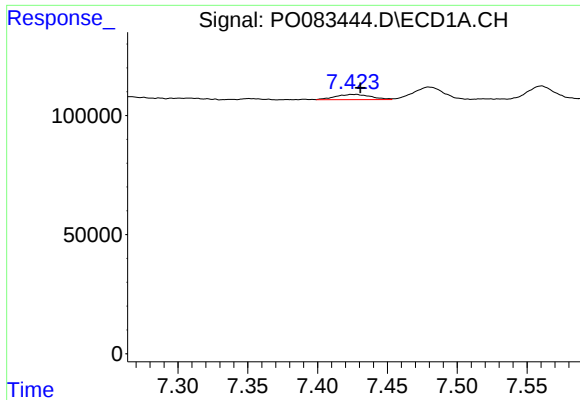

#27 AR-1254-2


R.T.: 7.428 min
Delta R.T.: -0.003 min
Response: 39718
Conc: 9.55 ng/ml

Instrument :
ECD_O
ClientSampleId :

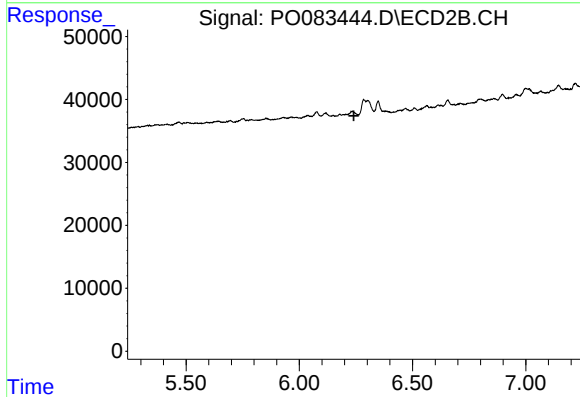


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

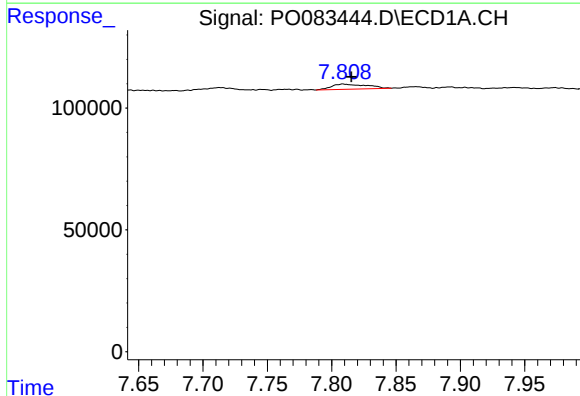


#28 AR-1254-3

R.T.: 7.809 min
Delta R.T.: -0.007 min
Response: 40155
Conc: 9.35 ng/ml

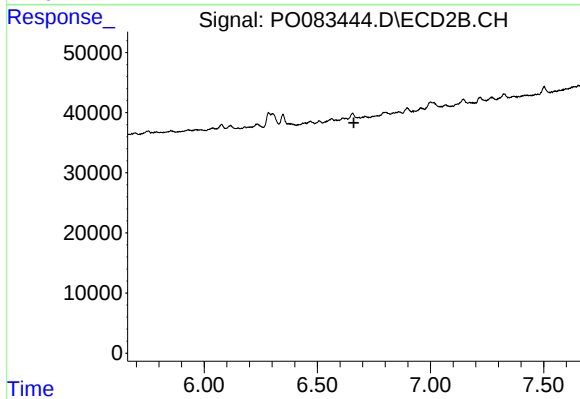

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.661 min
Response: 0
Conc: N.D.

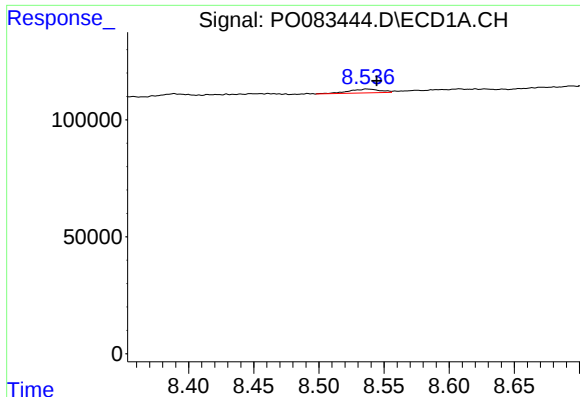

#30 AR-1254-5


R.T.: 8.536 min
Delta R.T.: -0.008 min
Response: 27153
Conc: 8.47 ng/ml

Instrument :
ECD_O
ClientSampleId :

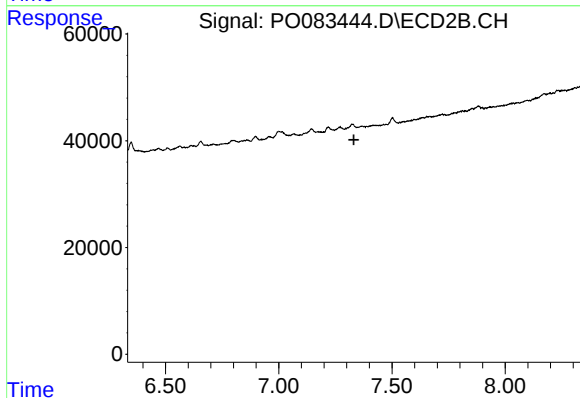


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.332 min
Response: 0
Conc: N.D.

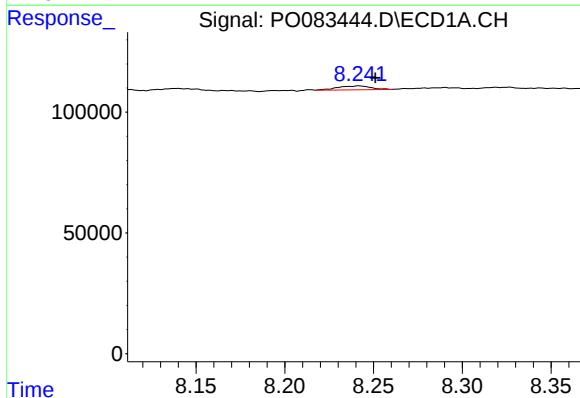


#32 AR-1260-2

R.T.: 8.242 min
Delta R.T.: -0.009 min
Response: 20731
Conc: 5.52 ng/ml

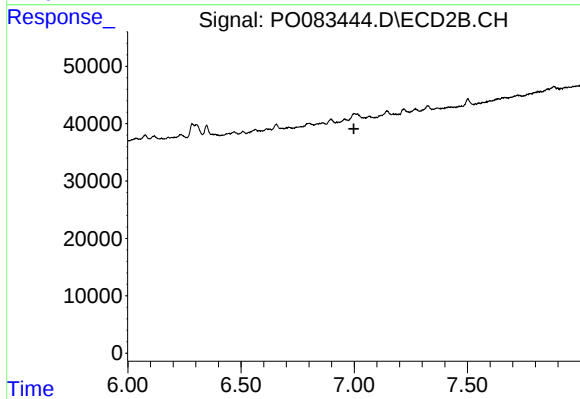

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.999 min
Response: 0
Conc: N.D.

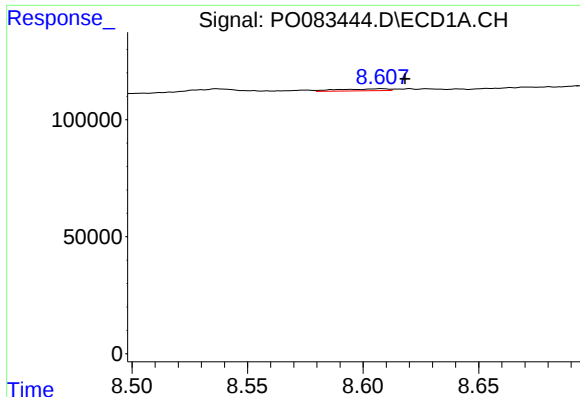

#33 AR-1260-3


R.T.: 8.608 min
Delta R.T.: -0.010 min
Response: 12618
Conc: 4.41 ng/ml

Instrument :
ECD_O
ClientSampleId :

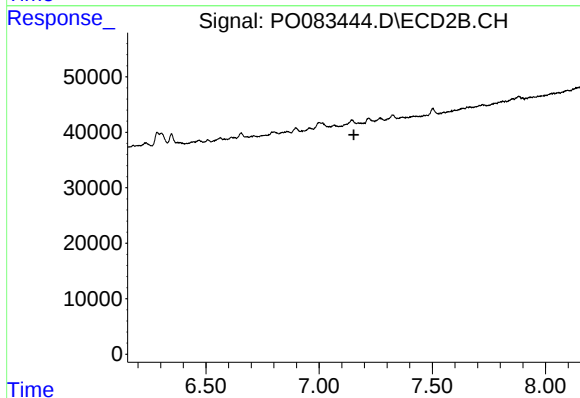


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.153 min
Response: 0
Conc: N.D.

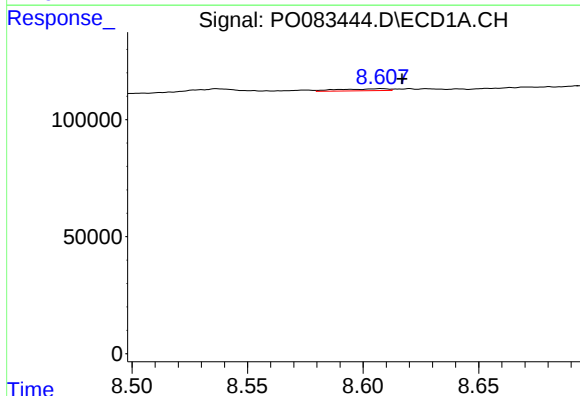

#36 AR-1262-1

R.T.: 8.608 min
Delta R.T.: -0.009 min
Response: 12618
Conc: 3.38 ng/ml

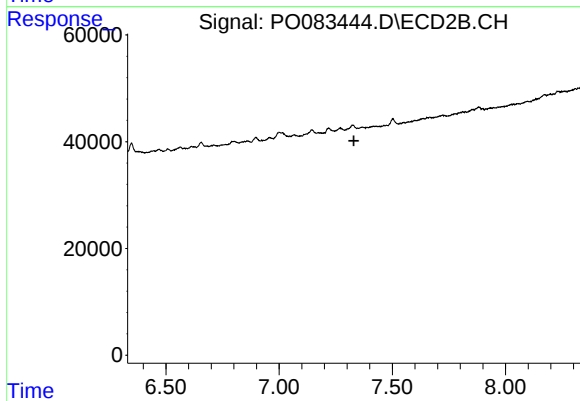

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.330 min
Response: 0
Conc: N.D.