

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120325\
 Data File : PO115572.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2025 19:25
 Operator : YP/AJ
 Sample : Q3769-02 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 Y2310-0306-B

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 12/04/2025
 Supervised By :mohammad ahmed 12/05/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 01:11:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 05 06:00:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.335	3.638	11368256	6843482	1.615m	1.532m
2) SA Decachlor...	9.913	8.624	9557353	4248536	2.162m	1.088m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120325\
Data File : PO115572.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2025 19:25
Operator : YP/AJ
Sample : Q3769-02 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
Y2310-0306-B


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/04/2025
Supervised By :mohammad ahmed 12/05/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 01:11:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 05 06:00:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

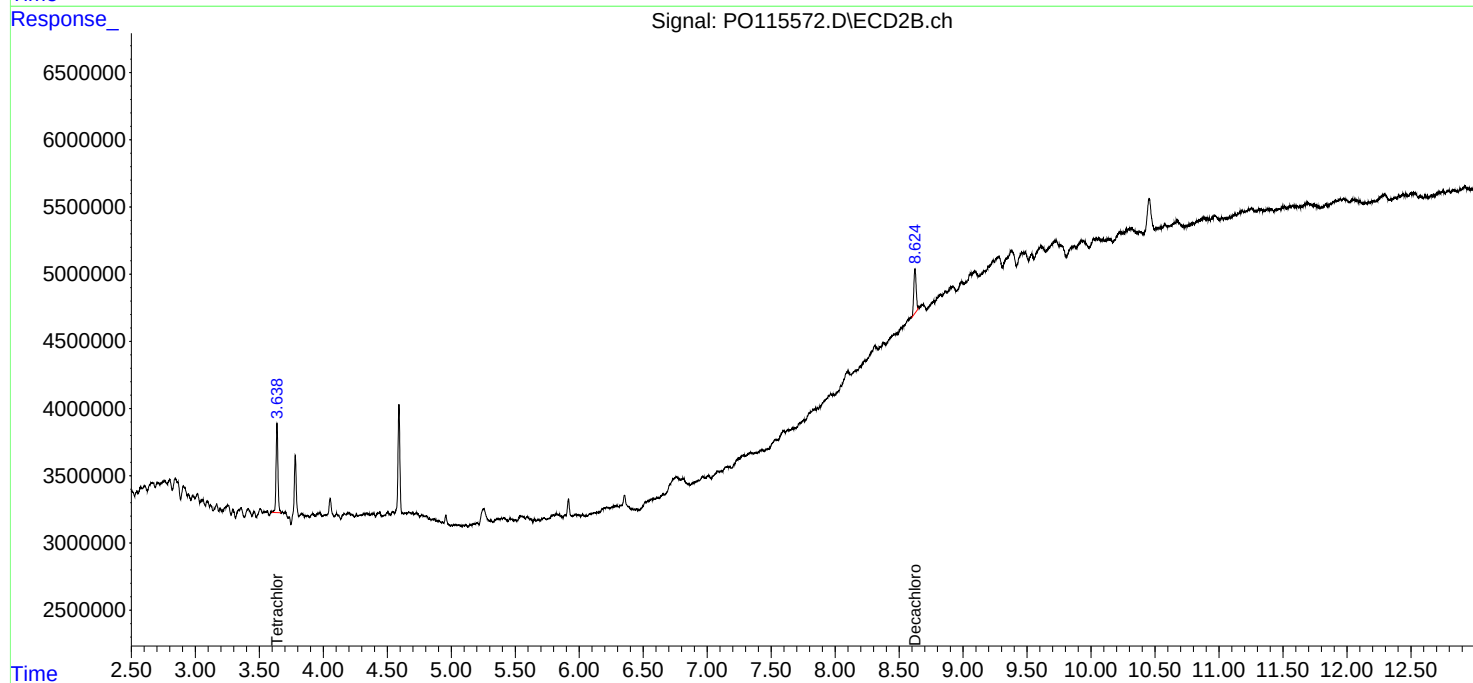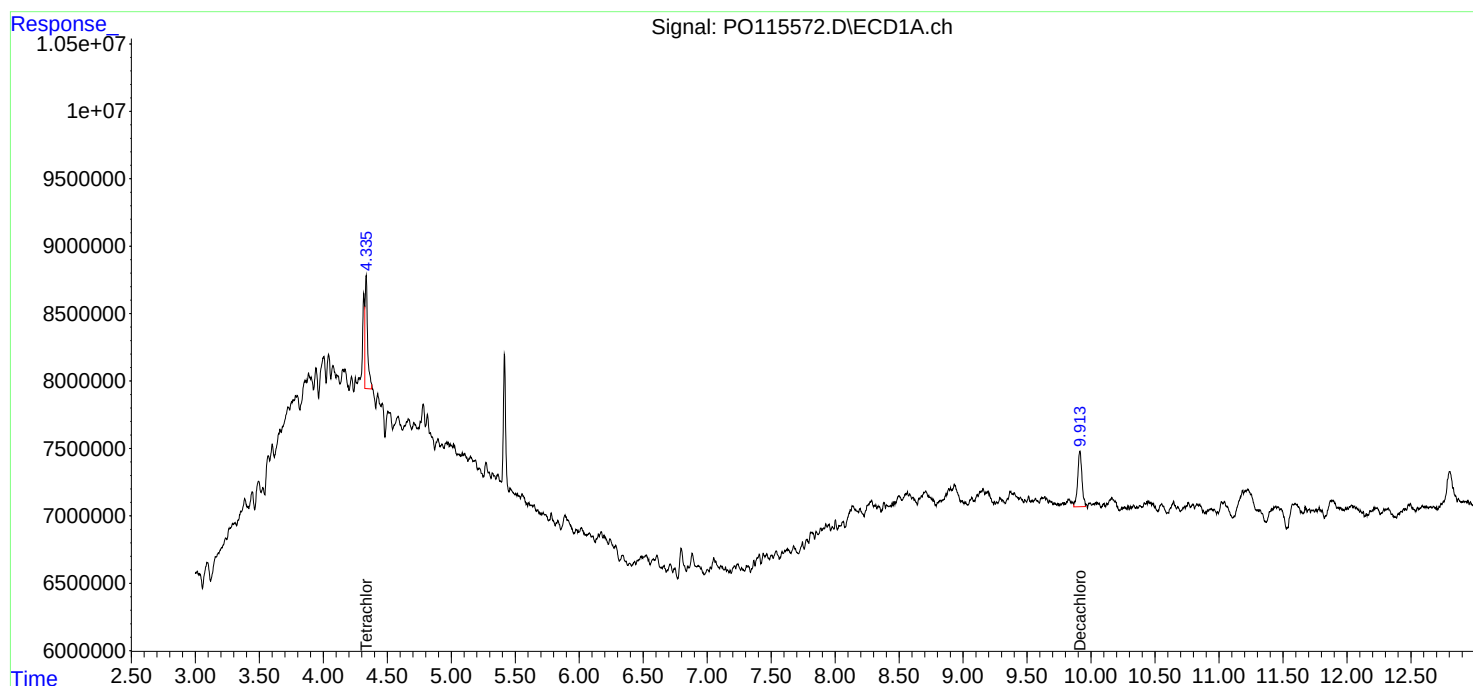

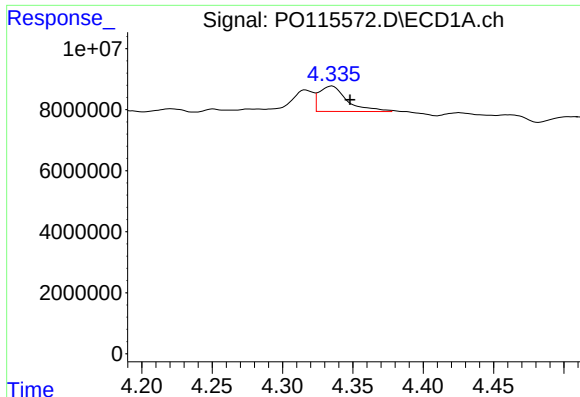


#1 Tetrachloro-m-xylene

R.T.: 4.335 min
Delta R.T.: -0.013 min
Response: 11368256
Conc: 1.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
Y2310-0306-B


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/04/2025
Supervised By :mohammad ahmed 12/05/2025

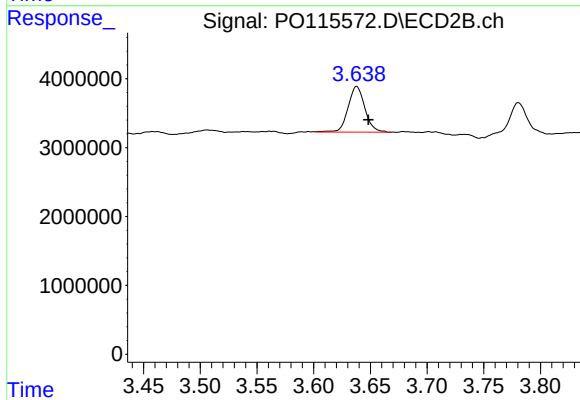


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: -0.011 min
Response: 6843482
Conc: 1.53 ng/ml m

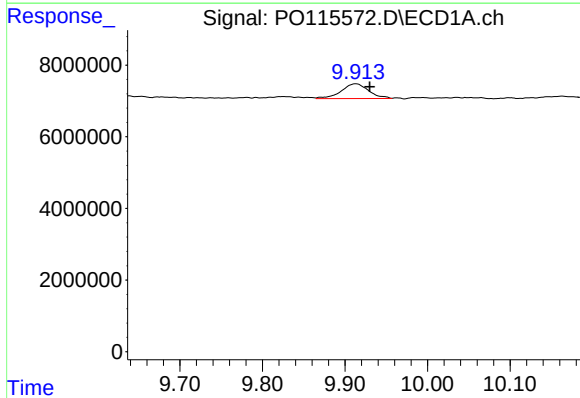

#2 Decachlorobiphenyl

R.T.: 9.913 min
Delta R.T.: -0.018 min
Response: 9557353
Conc: 2.16 ng/ml m

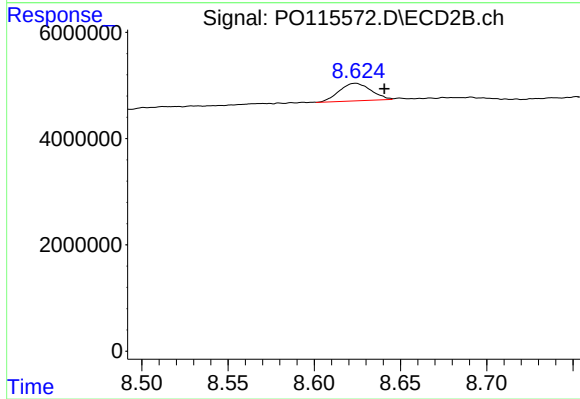

#2 Decachlorobiphenyl

R.T.: 8.624 min
Delta R.T.: -0.017 min
Response: 4248536
Conc: 1.09 ng/ml m