

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120419\
 Data File : P0064324.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Dec 2019 14:58
 Operator : SM/AJ
 Sample : K5956-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FAIRMOUNT-FOUNDATION-3

Manual Integrations
 APPROVED

mohammad
 12/5/2019 9:25:34 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 15:16:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 28 01:28:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.312	3.560	961167	819614	32.455	34.459
2) SA Decachlor...	9.945	8.527	792248	1141022	19.331m	27.932 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120419\
Data File : PO064324.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Dec 2019 14:58
Operator : SM/AJ
Sample : K5956-04
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FAIRMOUNT-FOUNDATION-3


Manual Integrations
APPROVED

mohammad
12/5/2019 9:25:34 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 15:16:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112719.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 28 01:28:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

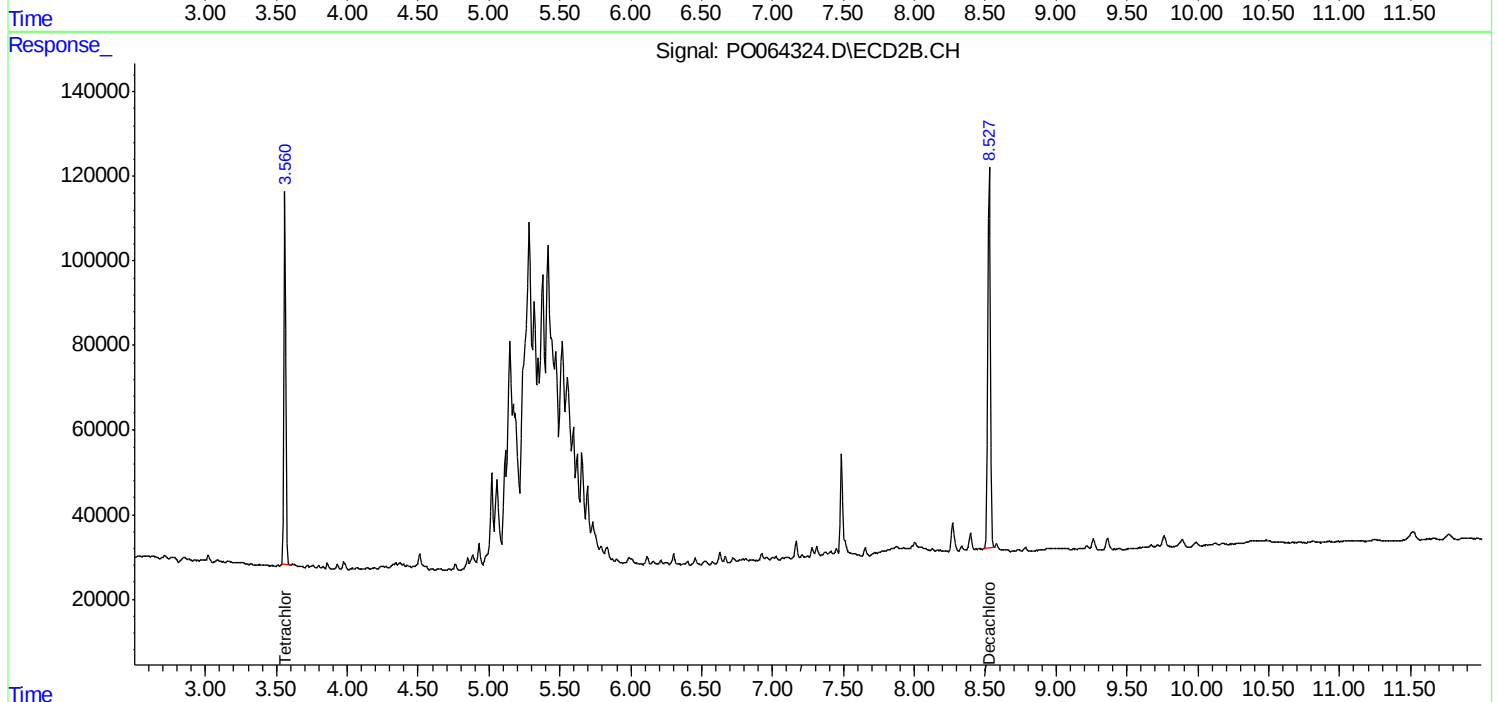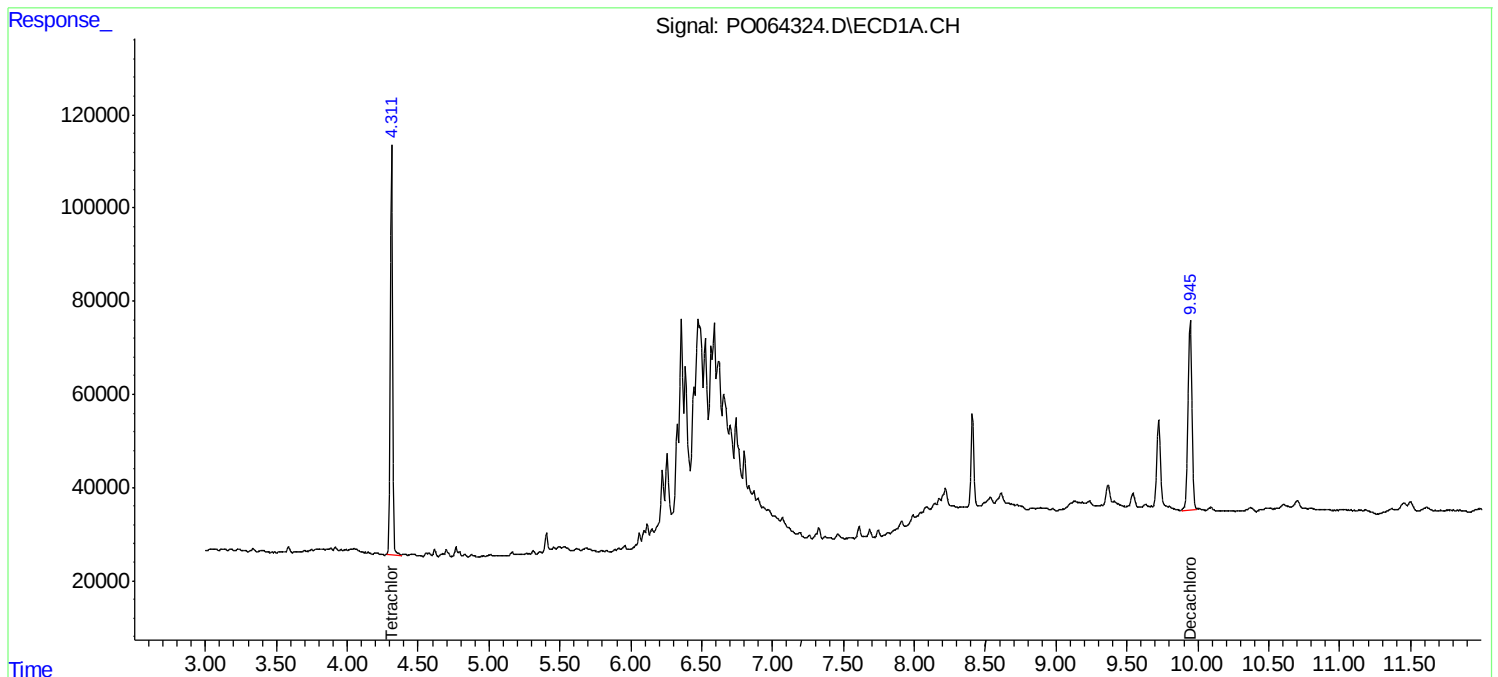

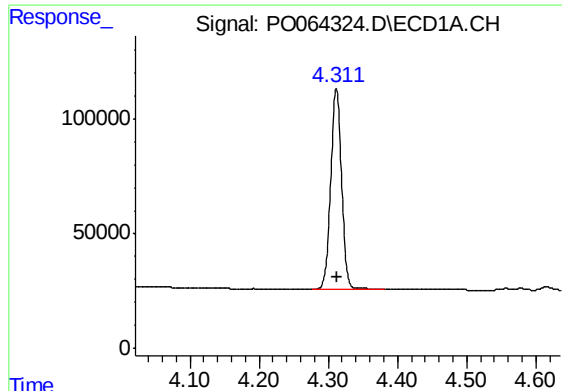


#1 Tetrachloro-m-xylene

R.T.: 4.312 min
Delta R.T.: -0.001 min
Response: 961167
Conc: 32.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
FAIRMOUNT-FOUNDATION-3


Manual Integrations
APPROVED

mohammad
12/5/2019 9:25:34 AM

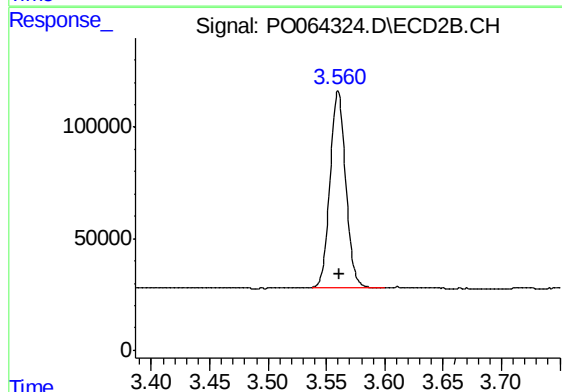


#1 Tetrachloro-m-xylene

R.T.: 3.560 min
Delta R.T.: -0.001 min
Response: 819614
Conc: 34.46 ng/ml

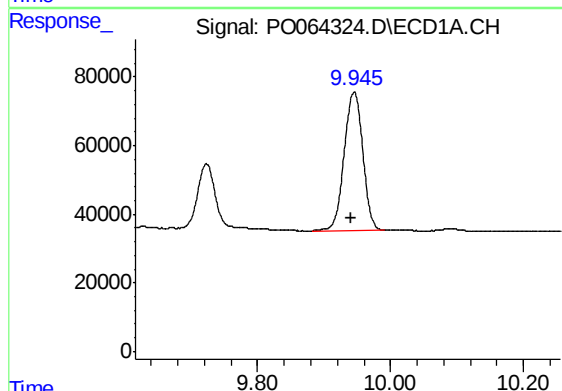

#2 Decachlorobiphenyl

R.T.: 9.945 min
Delta R.T.: 0.004 min
Response: 792248
Conc: 19.33 ng/ml m

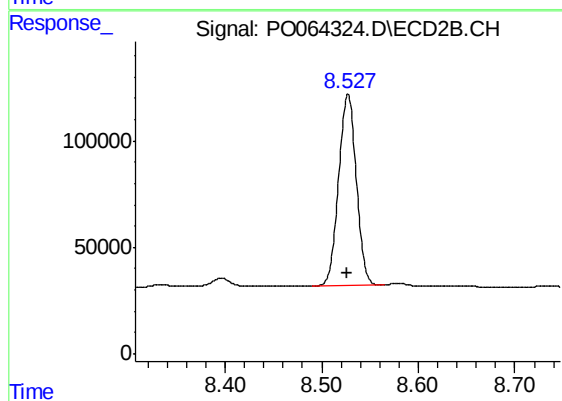

#2 Decachlorobiphenyl

R.T.: 8.527 min
Delta R.T.: 0.000 min
Response: 1141022
Conc: 27.93 ng/ml