

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120419\
 Data File : P0064331.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Dec 2019 16:55
 Operator : SM/AJ
 Sample : K6119-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-4-(8-10)

Manual Integrations
 APPROVED

mohammad
 12/5/2019 9:25:48 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 17:30:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 28 01:28:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.310	3.558	879036	787516	29.682	33.110
2)	SA Decachlor...	9.938	8.521	1441050	1693860	35.161m	41.465

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120419\
Data File : PO064331.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Dec 2019 16:55
Operator : SM/AJ
Sample : K6119-06
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-4-(8-10)


Manual Integrations
APPROVED

mohammad
12/5/2019 9:25:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 17:30:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112719.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 28 01:28:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

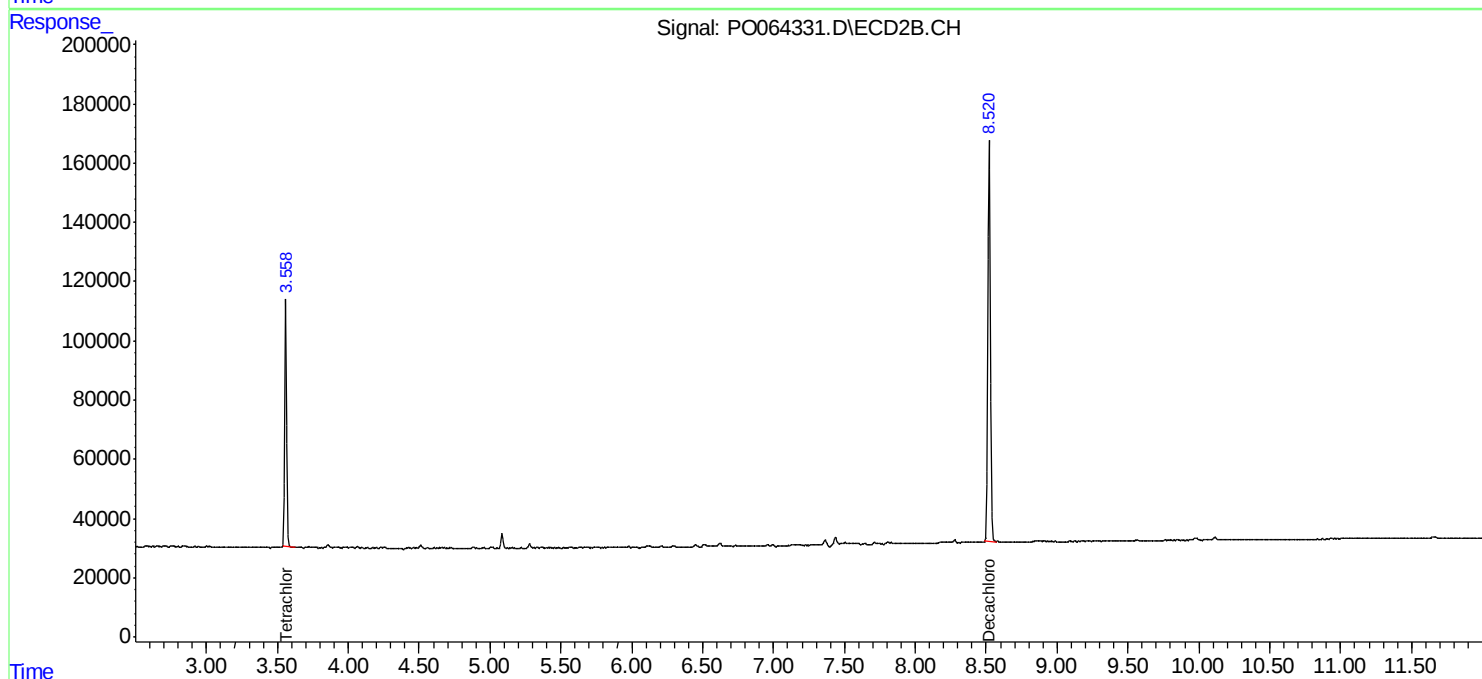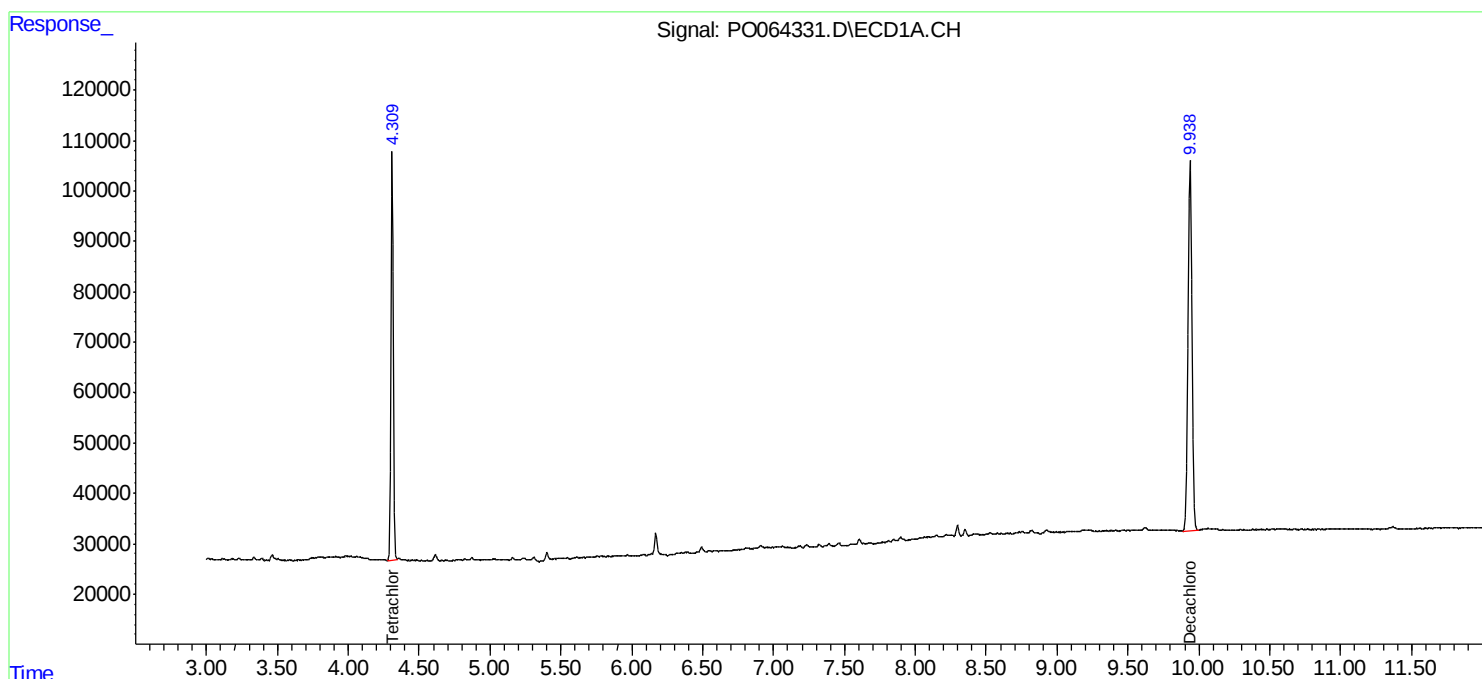

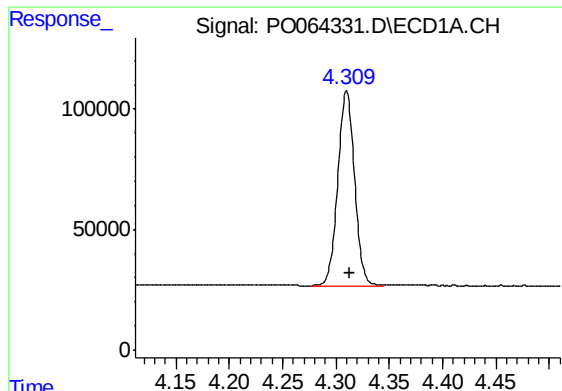


#1 Tetrachloro-m-xylene

R.T.: 4.310 min
Delta R.T.: -0.003 min
Response: 879036
Conc: 29.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-4-(8-10)


Manual Integrations
APPROVED

mohammad
12/5/2019 9:25:48 AM

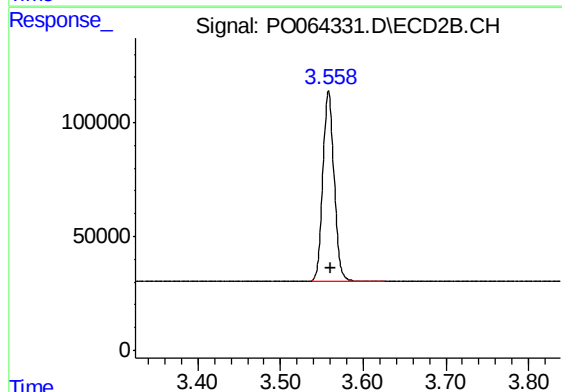


#1 Tetrachloro-m-xylene

R.T.: 3.558 min
Delta R.T.: -0.003 min
Response: 787516
Conc: 33.11 ng/ml

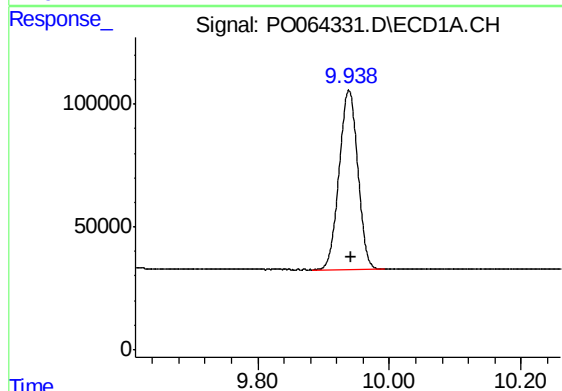

#2 Decachlorobiphenyl

R.T.: 9.938 min
Delta R.T.: -0.003 min
Response: 1441050
Conc: 35.16 ng/ml m

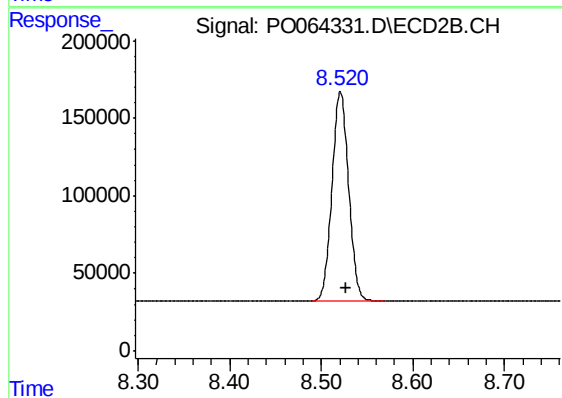

#2 Decachlorobiphenyl

R.T.: 8.521 min
Delta R.T.: -0.006 min
Response: 1693860
Conc: 41.46 ng/ml