

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0120419\
 Data File : P0064332.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Dec 2019 17:11
 Operator : SM/AJ
 Sample : K6119-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-5-(0-2)

Manual Integrations
 APPROVED

mohammad
 12/5/2019 9:25:51 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 17:31:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 28 01:28:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.310	3.557	724787	650294	24.473	27.340m
2)	SA Decachlor...	9.937	8.522	932415	1088256	22.751m	26.640

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120419\
Data File : PO064332.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Dec 2019 17:11
Operator : SM/AJ
Sample : K6119-07
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-5-(0-2)


Manual Integrations
APPROVED

mohammad
12/5/2019 9:25:51 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 17:31:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112719.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 28 01:28:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

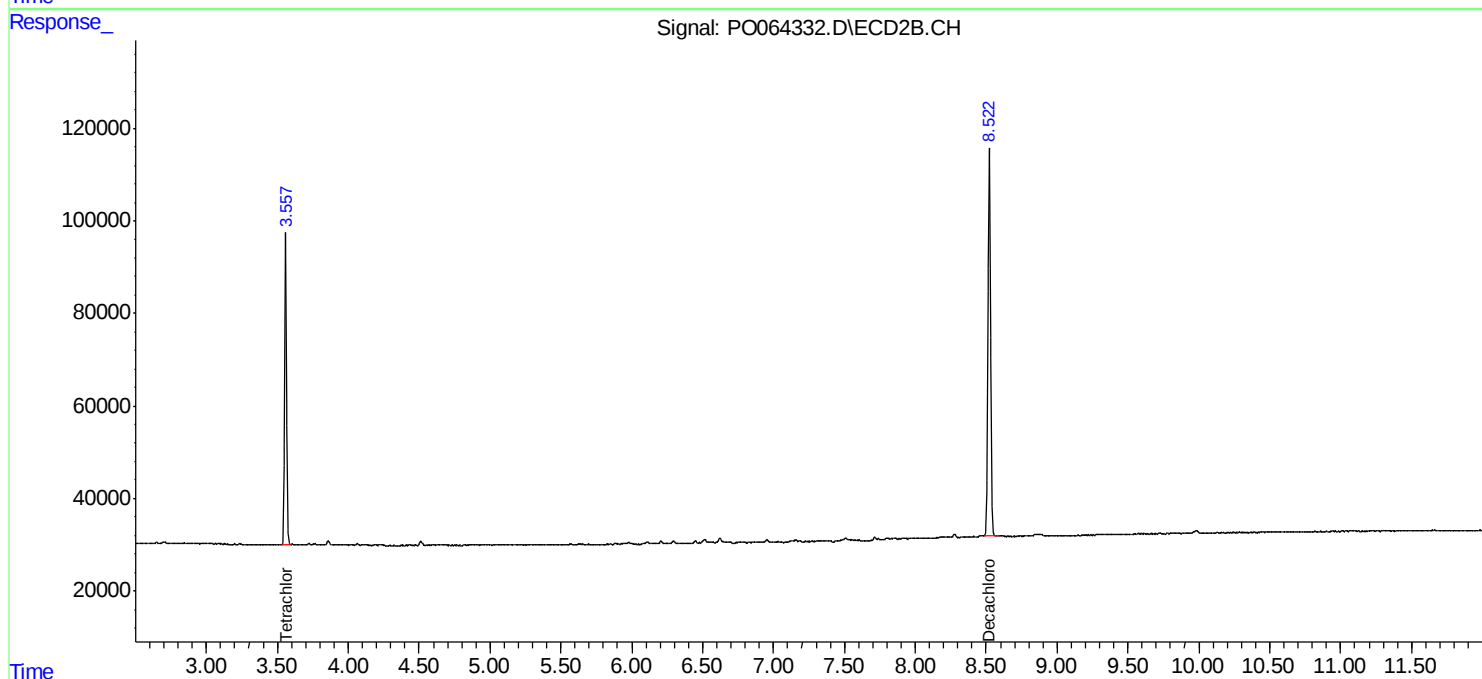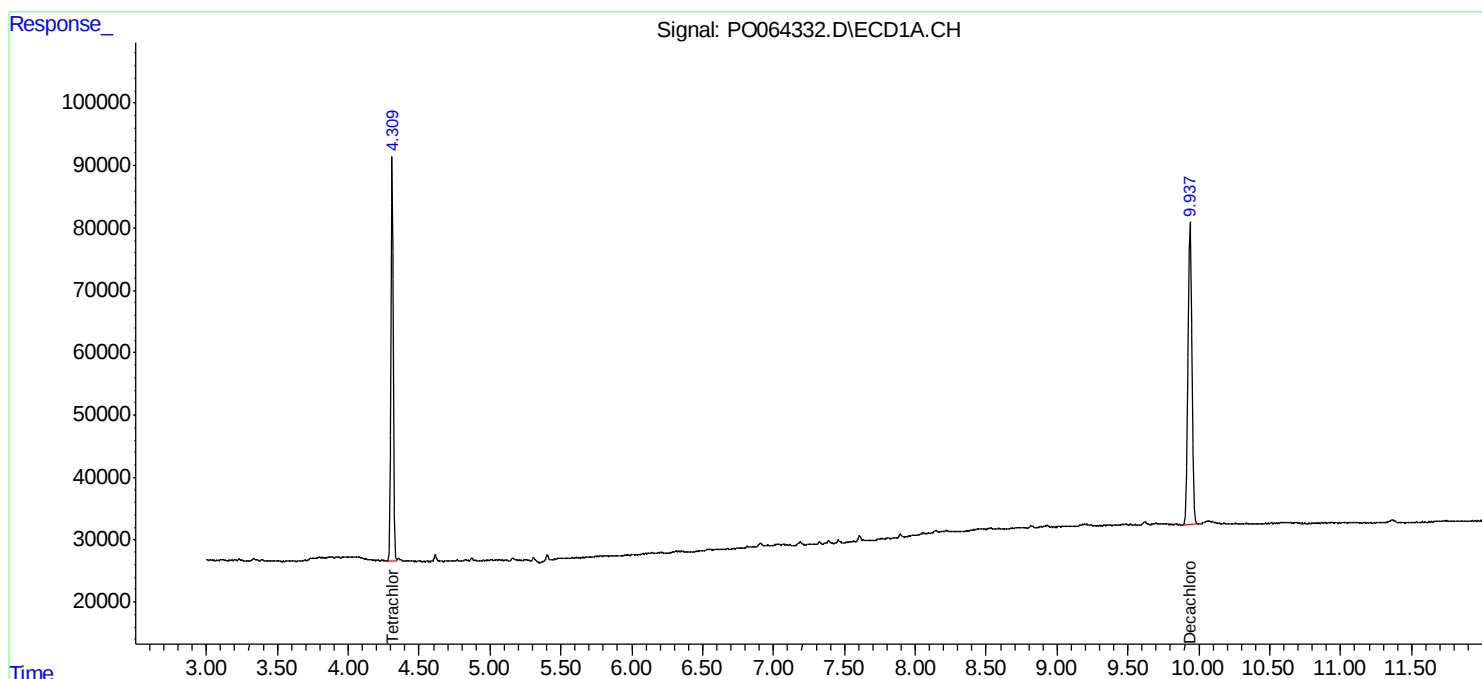

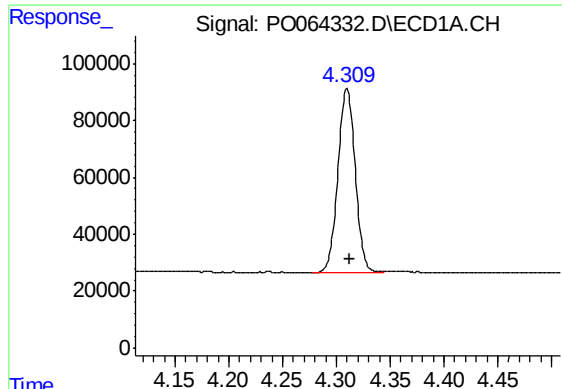


#1 Tetrachloro-m-xylene

R.T.: 4.310 min
Delta R.T.: -0.003 min
Response: 724787
Conc: 24.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-5-(0-2)


Manual Integrations
APPROVED

mohammad
12/5/2019 9:25:51 AM

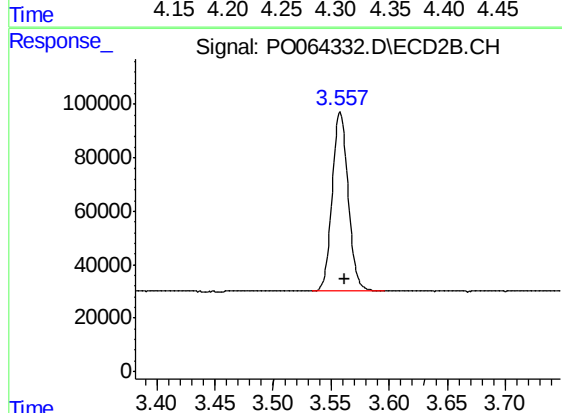


#1 Tetrachloro-m-xylene

R.T.: 3.557 min
Delta R.T.: -0.004 min
Response: 650294
Conc: 27.34 ng/ml m

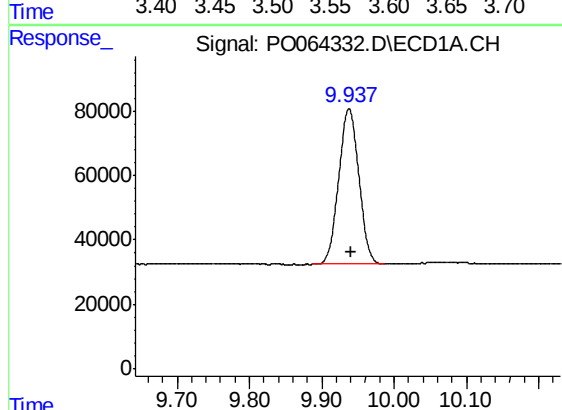

#2 Decachlorobiphenyl

R.T.: 9.937 min
Delta R.T.: -0.004 min
Response: 932415
Conc: 22.75 ng/ml m

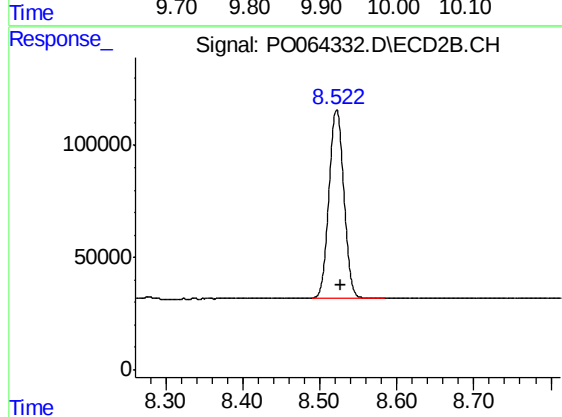

#2 Decachlorobiphenyl

R.T.: 8.522 min
Delta R.T.: -0.005 min
Response: 1088256
Conc: 26.64 ng/ml