

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120419\
 Data File : P0064338.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Dec 2019 18:51
 Operator : SM/AJ
 Sample : K6120-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TH-6

Manual Integrations
 APPROVED

mohammad
 12/5/2019 9:26:01 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 06:17:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 28 01:28:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.312	3.560	777075	720288	26.239	30.283
2)	SA Decachlor...	9.940	8.522	867657	989380	21.171m	24.220

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120419\
Data File : PO064338.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Dec 2019 18:51
Operator : SM/AJ
Sample : K6120-03
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TH-6


Manual Integrations
APPROVED

mohammad
12/5/2019 9:26:01 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 06:17:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112719.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 28 01:28:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

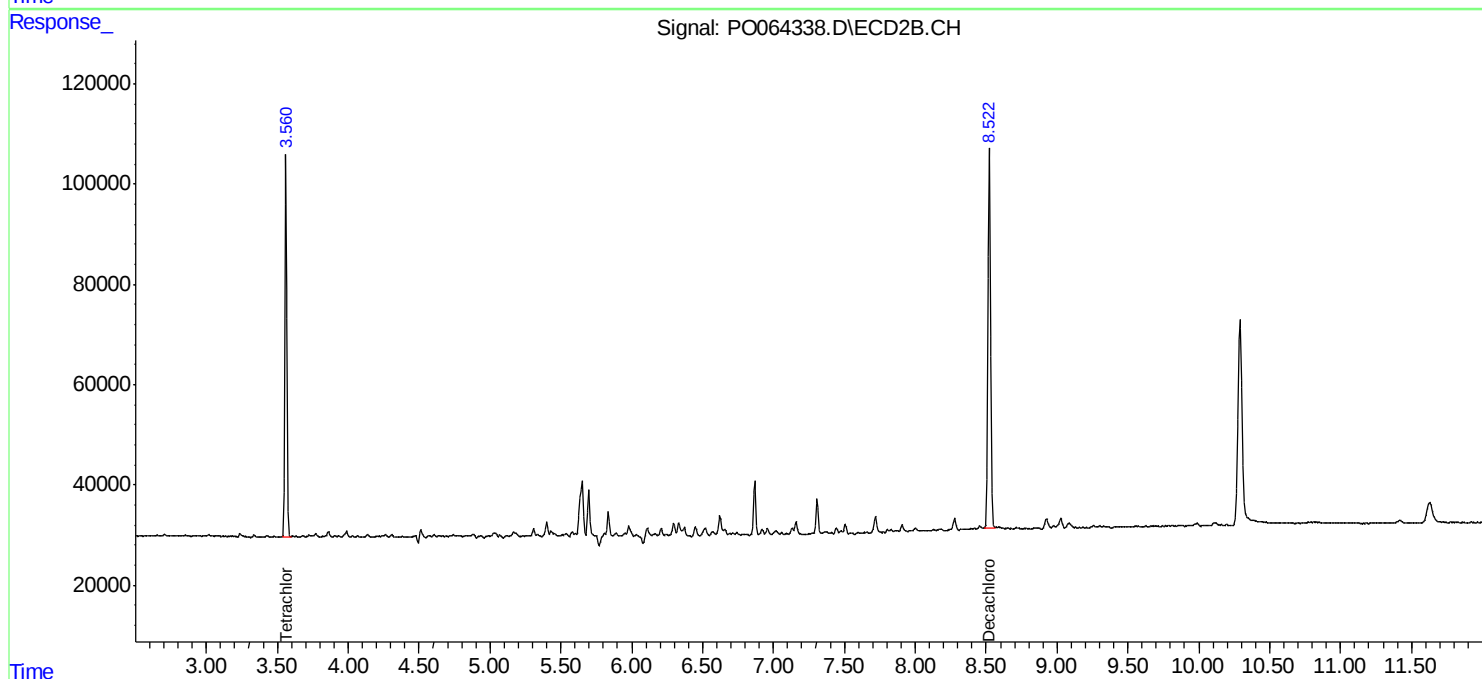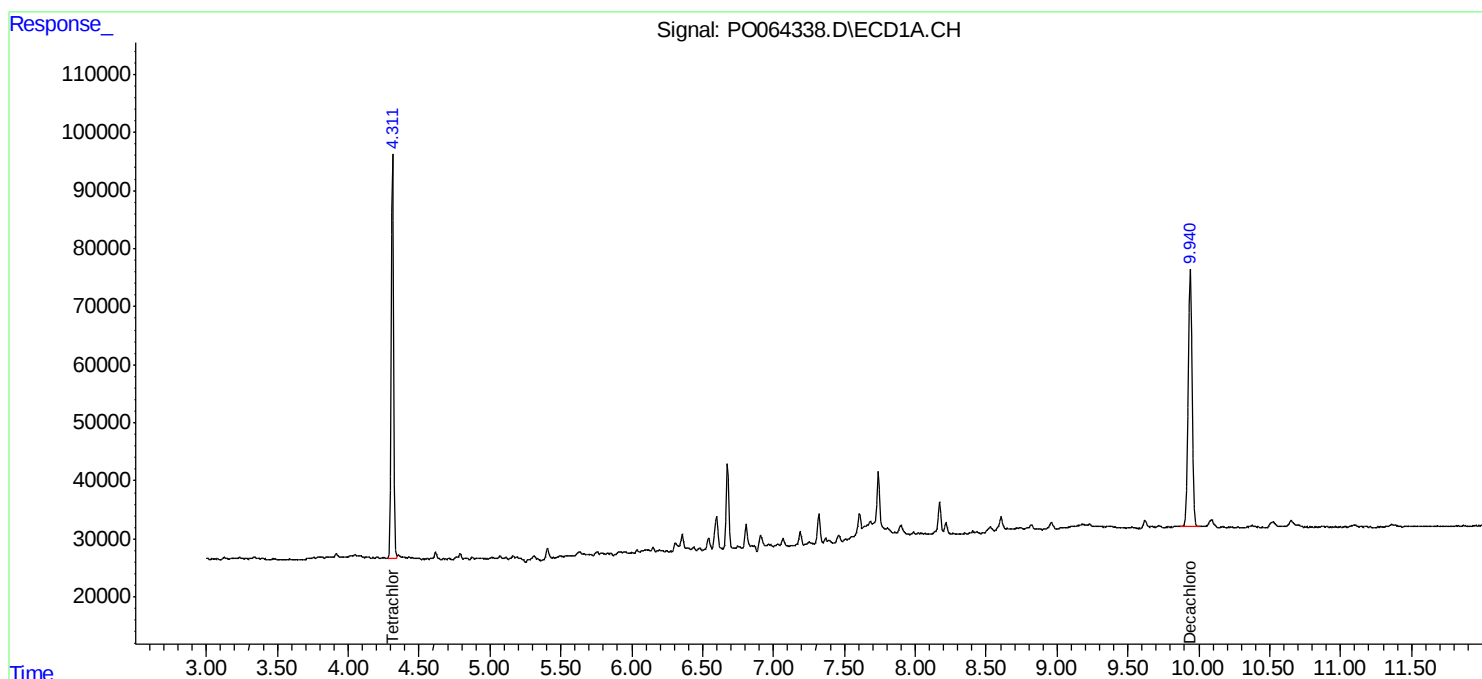

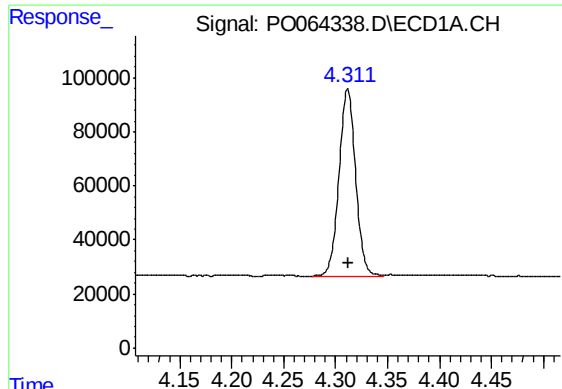


#1 Tetrachloro-m-xylene

R.T.: 4.312 min
Delta R.T.: -0.001 min
Response: 777075
Conc: 26.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
TH-6


Manual Integrations
APPROVED

mohammad
12/5/2019 9:26:01 AM

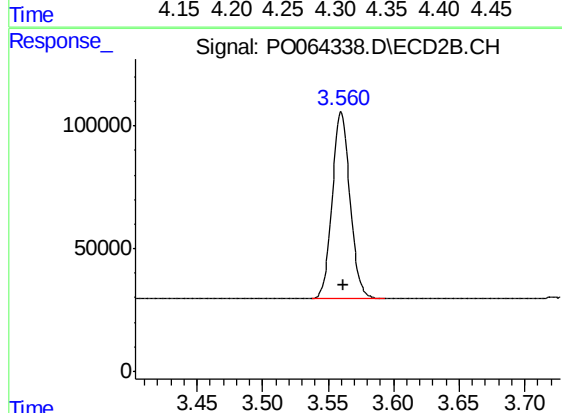


#1 Tetrachloro-m-xylene

R.T.: 3.560 min
Delta R.T.: -0.001 min
Response: 720288
Conc: 30.28 ng/ml

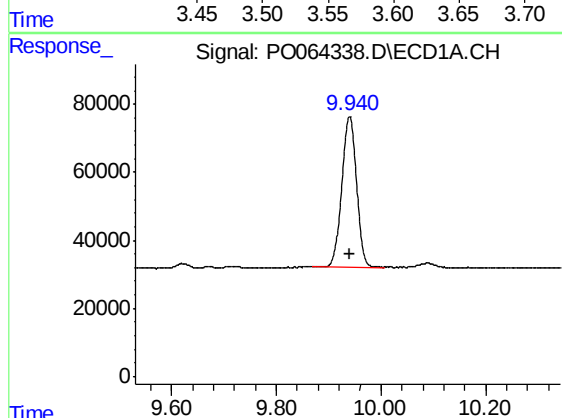

#2 Decachlorobiphenyl

R.T.: 9.940 min
Delta R.T.: -0.001 min
Response: 867657
Conc: 21.17 ng/ml m

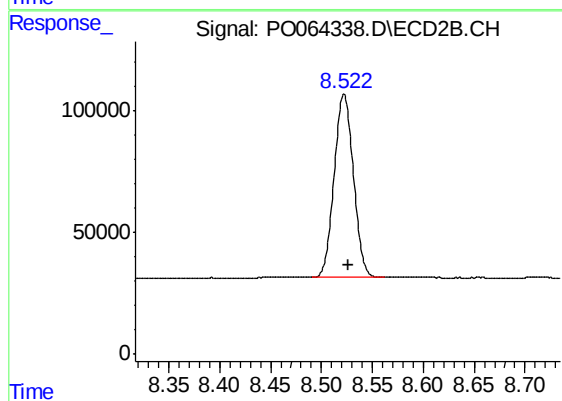

#2 Decachlorobiphenyl

R.T.: 8.522 min
Delta R.T.: -0.004 min
Response: 989380
Conc: 24.22 ng/ml