

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0120419\
 Data File : P0064345.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Dec 2019 21:38
 Operator : SM/AJ
 Sample : K6119-05
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-4-(0-2)

Manual Integrations
 APPROVED

mohammad
 12/5/2019 9:26:11 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 05:02:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 28 01:28:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.312	3.561	990028	956357	33.430	40.208
2)	SA Decachlor...	9.939	8.523	813110	788111	19.840m	19.293

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120419\
Data File : PO064345.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Dec 2019 21:38
Operator : SM/AJ
Sample : K6119-05
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-4-(0-2)


Manual Integrations
APPROVED

mohammad
12/5/2019 9:26:11 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 05:02:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112719.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 28 01:28:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

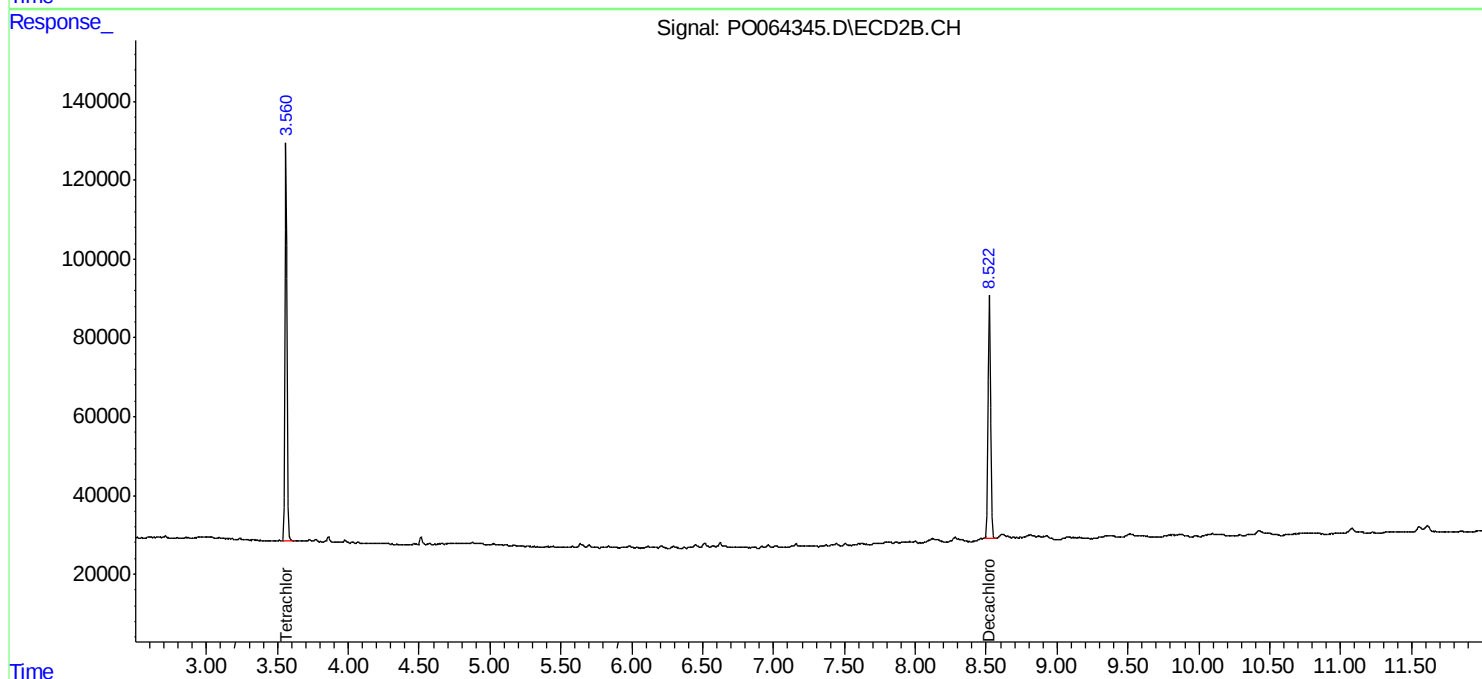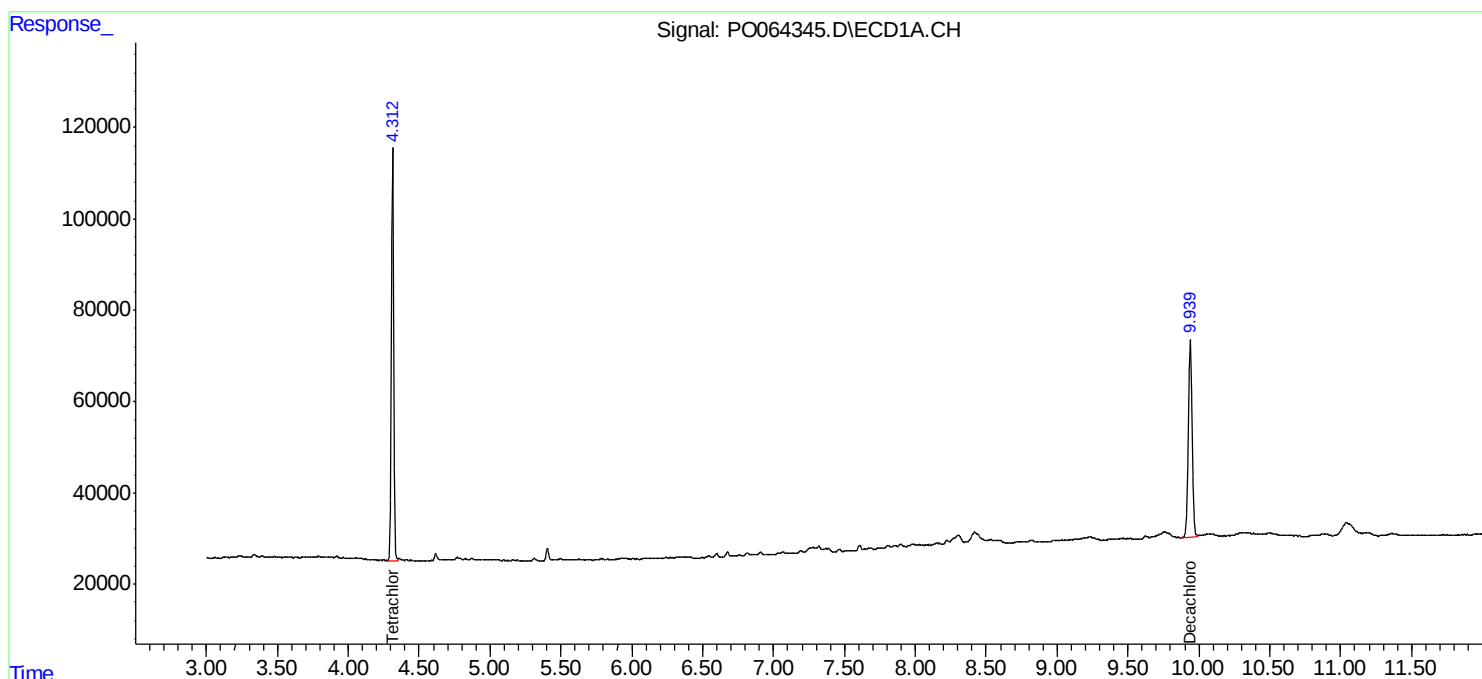

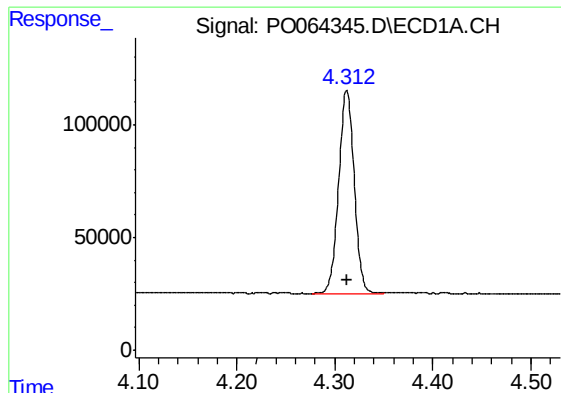


#1 Tetrachloro-m-xylene

R.T.: 4.312 min
Delta R.T.: 0.000 min
Response: 990028
Conc: 33.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-4-(0-2)


Manual Integrations
APPROVED

mohammad
12/5/2019 9:26:11 AM

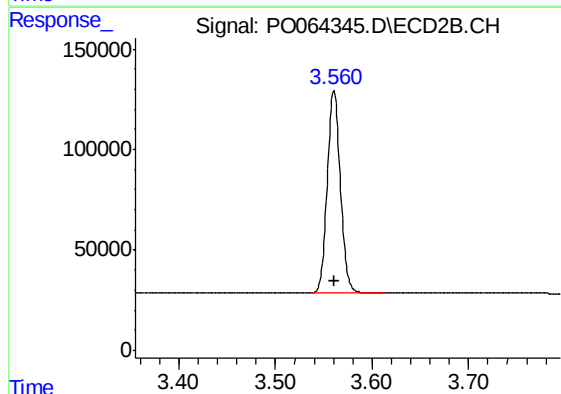


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: 0.000 min
Response: 956357
Conc: 40.21 ng/ml

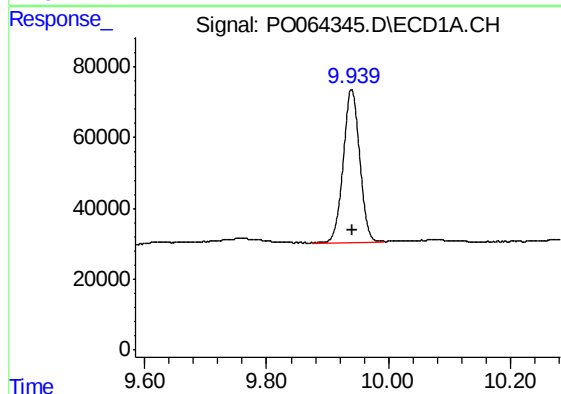

#2 Decachlorobiphenyl

R.T.: 9.939 min
Delta R.T.: -0.002 min
Response: 813110
Conc: 19.84 ng/ml m

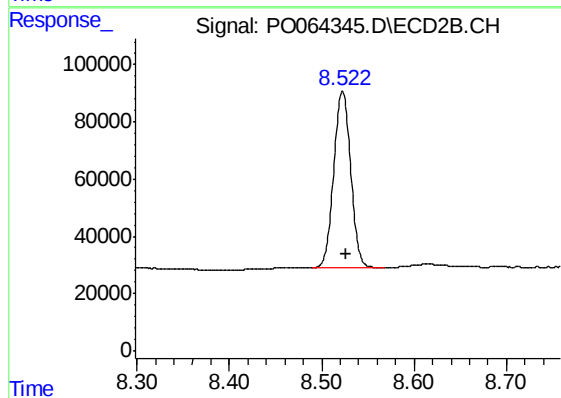

#2 Decachlorobiphenyl

R.T.: 8.523 min
Delta R.T.: -0.004 min
Response: 788111
Conc: 19.29 ng/ml