

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120423\
 Data File : PO100247.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2023 14:34
 Operator : YP/AJ
 Sample : 05599-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LKWD-BACKFILL-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 15:30:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 21 15:58:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.480	3.704	34318804	31938795	20.107	21.294
2) SA Decachlor...	10.364	8.796	19495731	28879886	26.841	25.809

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120423\
Data File : PO100247.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2023 14:34
Operator : YP/AJ
Sample : 05599-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LKWD-BACKFILL-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 15:30:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 21 15:58:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

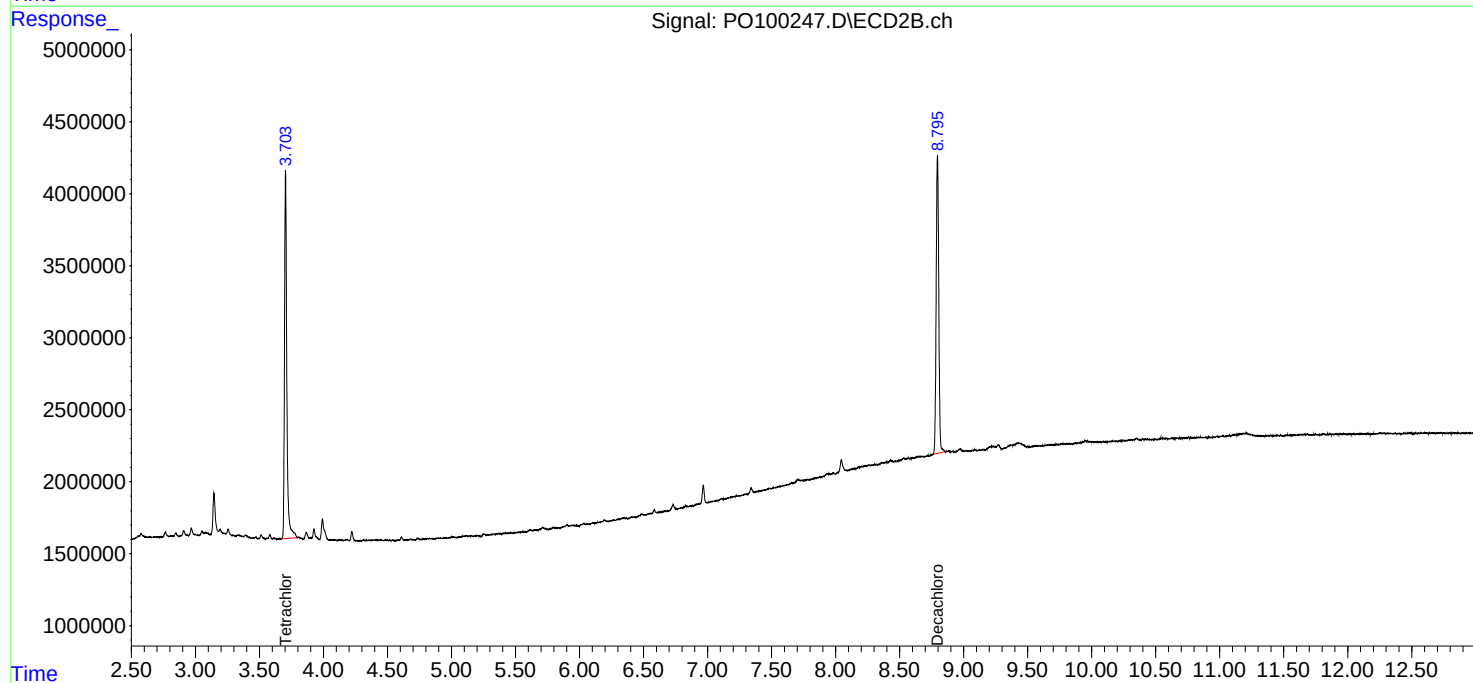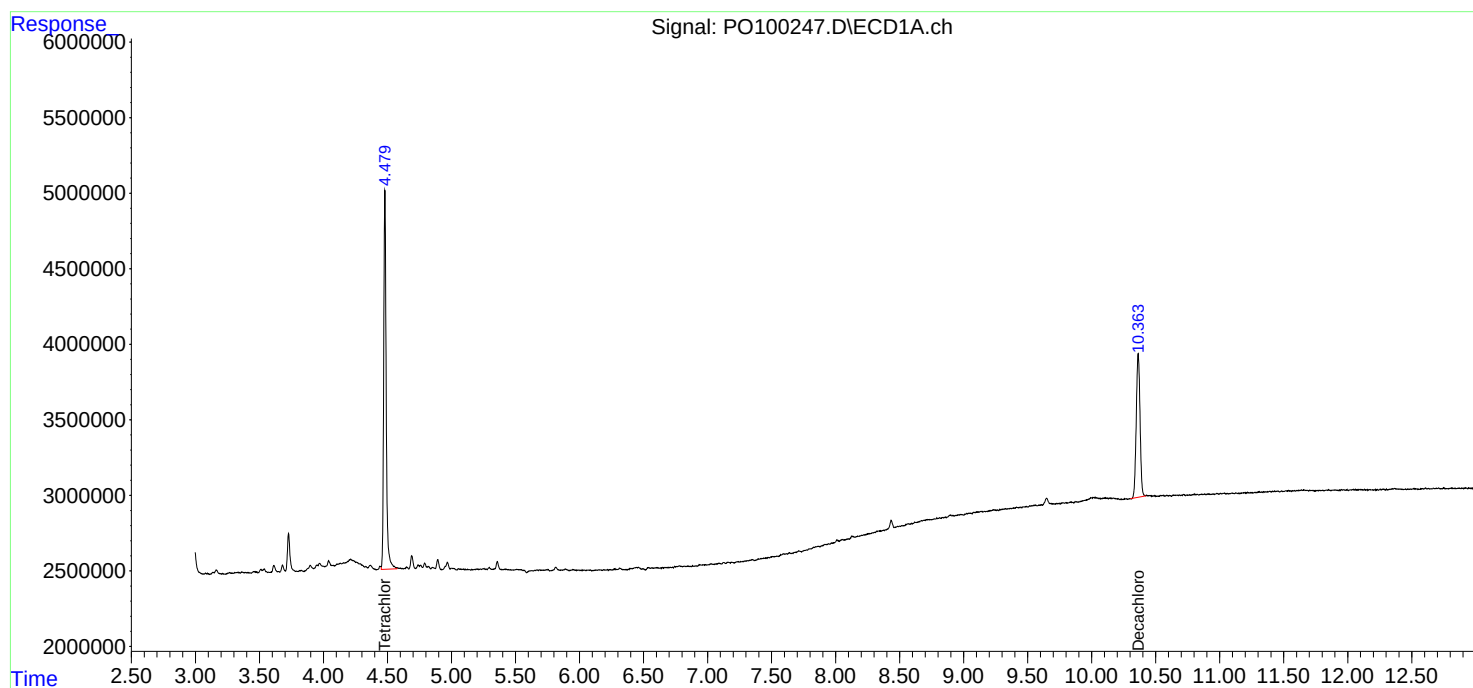


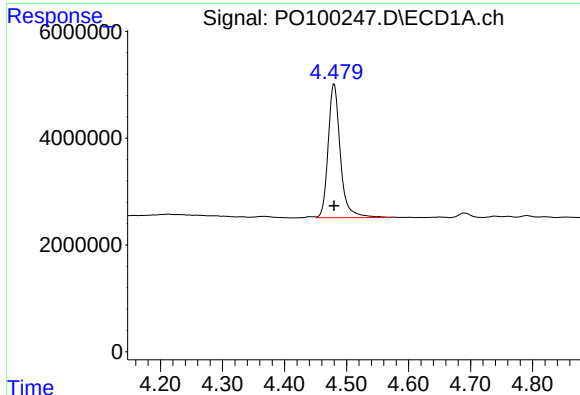

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 34318804
Conc: 20.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
LKWD-BACKFILL-03

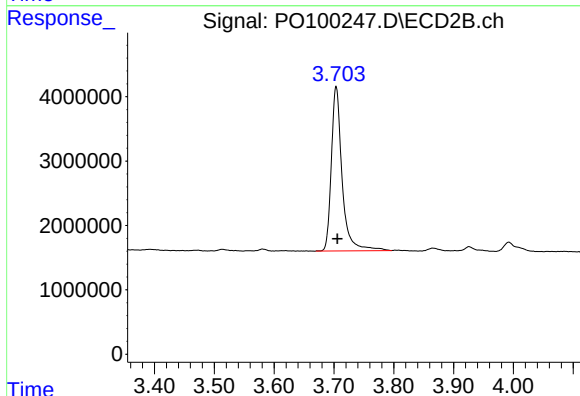


#1 Tetrachloro-m-xylene

R.T.: 3.704 min
Delta R.T.: -0.002 min
Response: 31938795
Conc: 21.29 ng/ml

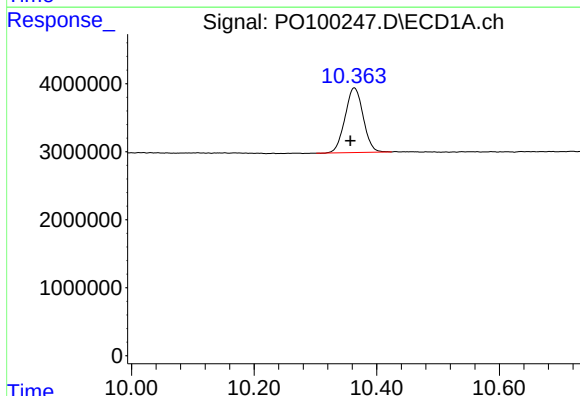

#2 Decachlorobiphenyl

R.T.: 10.364 min
Delta R.T.: 0.007 min
Response: 19495731
Conc: 26.84 ng/ml

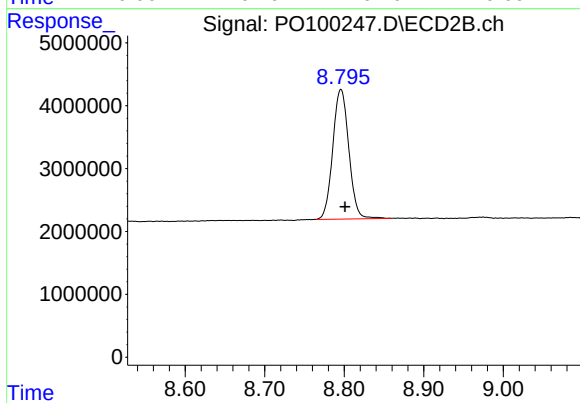

#2 Decachlorobiphenyl

R.T.: 8.796 min
Delta R.T.: -0.005 min
Response: 28879886
Conc: 25.81 ng/ml