

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120423\
 Data File : PO100250.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2023 15:25
 Operator : YP/AJ
 Sample : 05599-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LKWD-BACKFILL-06

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 16:48:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 21 15:58:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.480	3.703	35319455	32546488	20.693	21.699
2) SA Decachlor...	10.362	8.795	15679278	23424917	21.586	20.934

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120423\
Data File : PO100250.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2023 15:25
Operator : YP/AJ
Sample : 05599-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LKWD-BACKFILL-06

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 16:48:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 21 15:58:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

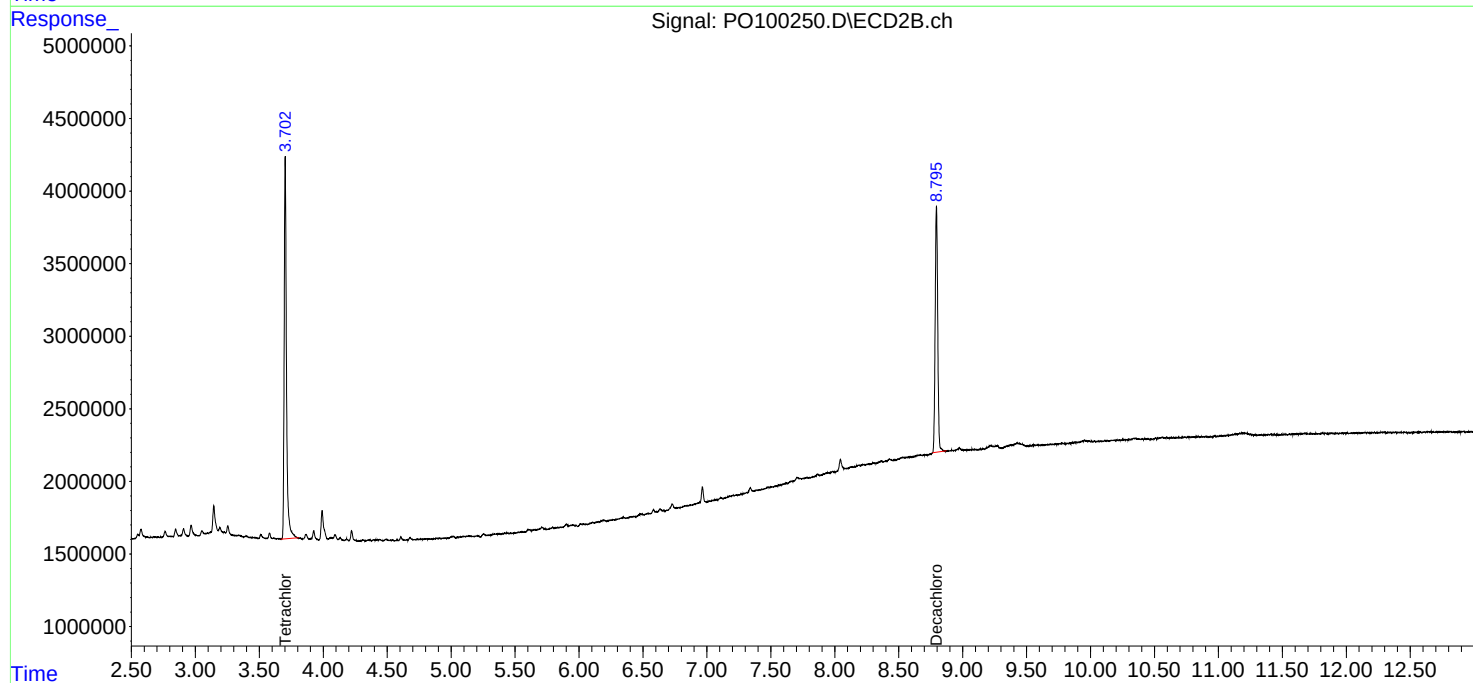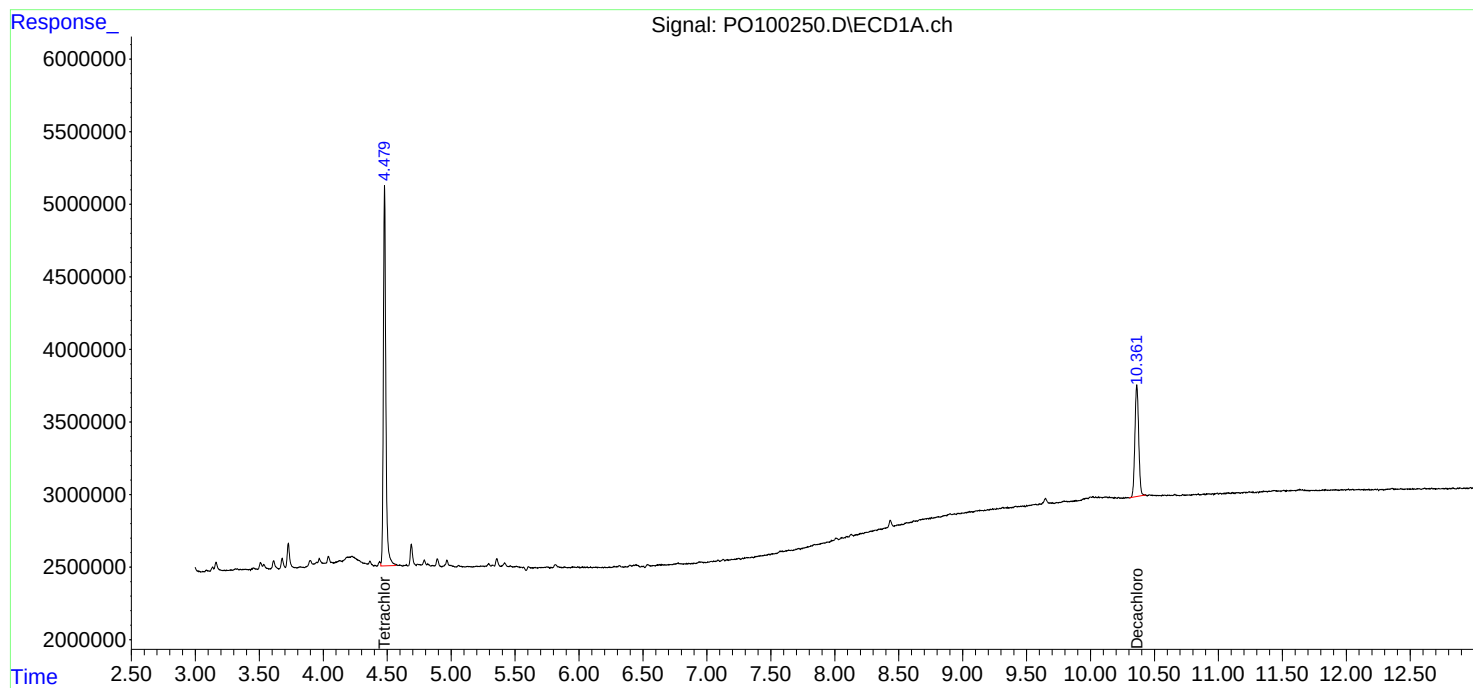


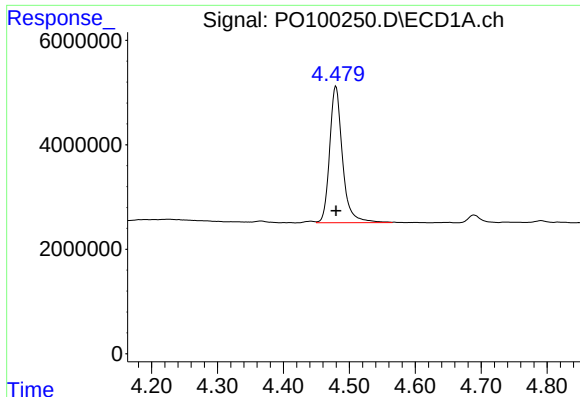

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 35319455
Conc: 20.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
LKWD-BACKFILL-06

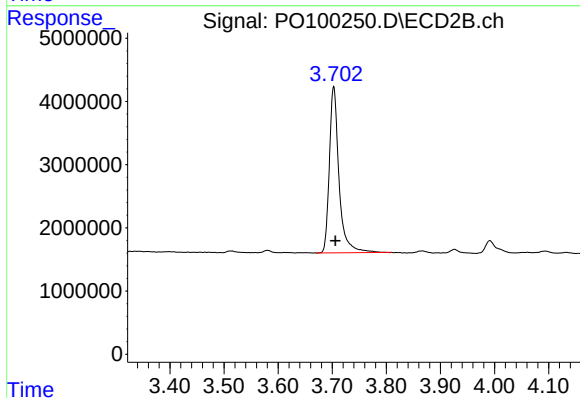


#1 Tetrachloro-m-xylene

R.T.: 3.703 min
Delta R.T.: -0.003 min
Response: 32546488
Conc: 21.70 ng/ml

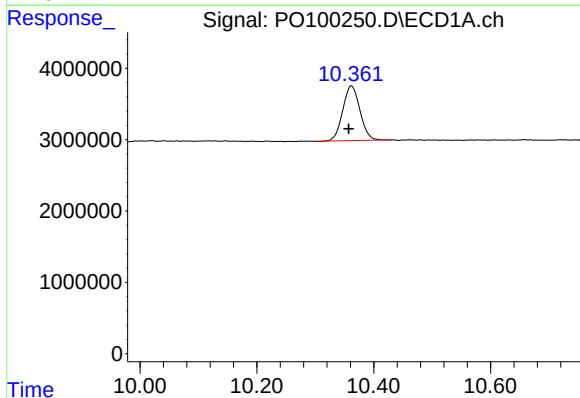

#2 Decachlorobiphenyl

R.T.: 10.362 min
Delta R.T.: 0.005 min
Response: 15679278
Conc: 21.59 ng/ml

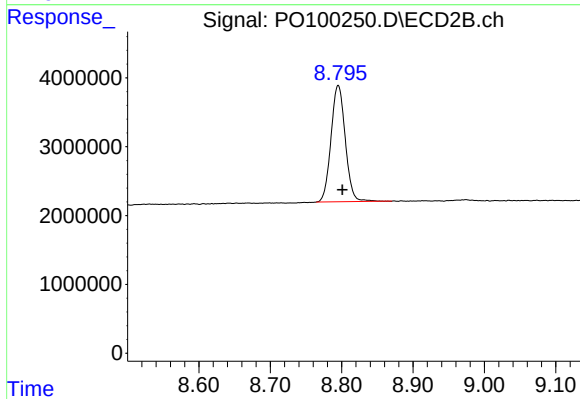

#2 Decachlorobiphenyl

R.T.: 8.795 min
Delta R.T.: -0.006 min
Response: 23424917
Conc: 20.93 ng/ml