

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120518\
 Data File : PO052270.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Dec 2018 20:18
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 03:27:51 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 04 03:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.277	3.294	21091384	5843665	24.499	26.201
2)	SA Decachlor...	9.850	7.990	9698146	4136177	19.379	19.840
Target Compounds							
7)	L1 AR-1016-5	0.000	4.720	0	50574	N.D.	7.316 #
15)	L3 AR-1232-5	0.000	4.720	0	50574	N.D.	20.176 #
24)	L5 AR-1248-4	0.000	4.720	0	50574	N.D.	6.128 #
30)	L6 AR-1254-5	7.573	0.000	49318	0	1.675	N.D. #
33)	L7 AR-1260-3	7.573	0.000	49318	0	2.039	N.D. #
34)	L7 AR-1260-4	7.857	0.000	156778	0	6.407	N.D. #
35)	L7 AR-1260-5	8.217	0.000	100740	0	2.050	N.D. #
36)	L8 AR-1262-1	7.573	0.000	49318	0	1.211	N.D. #
37)	L8 AR-1262-2	8.217	0.000	100740	0	1.553	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120518\
Data File : PO052270.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Dec 2018 20:18
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 03:27:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 04 03:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

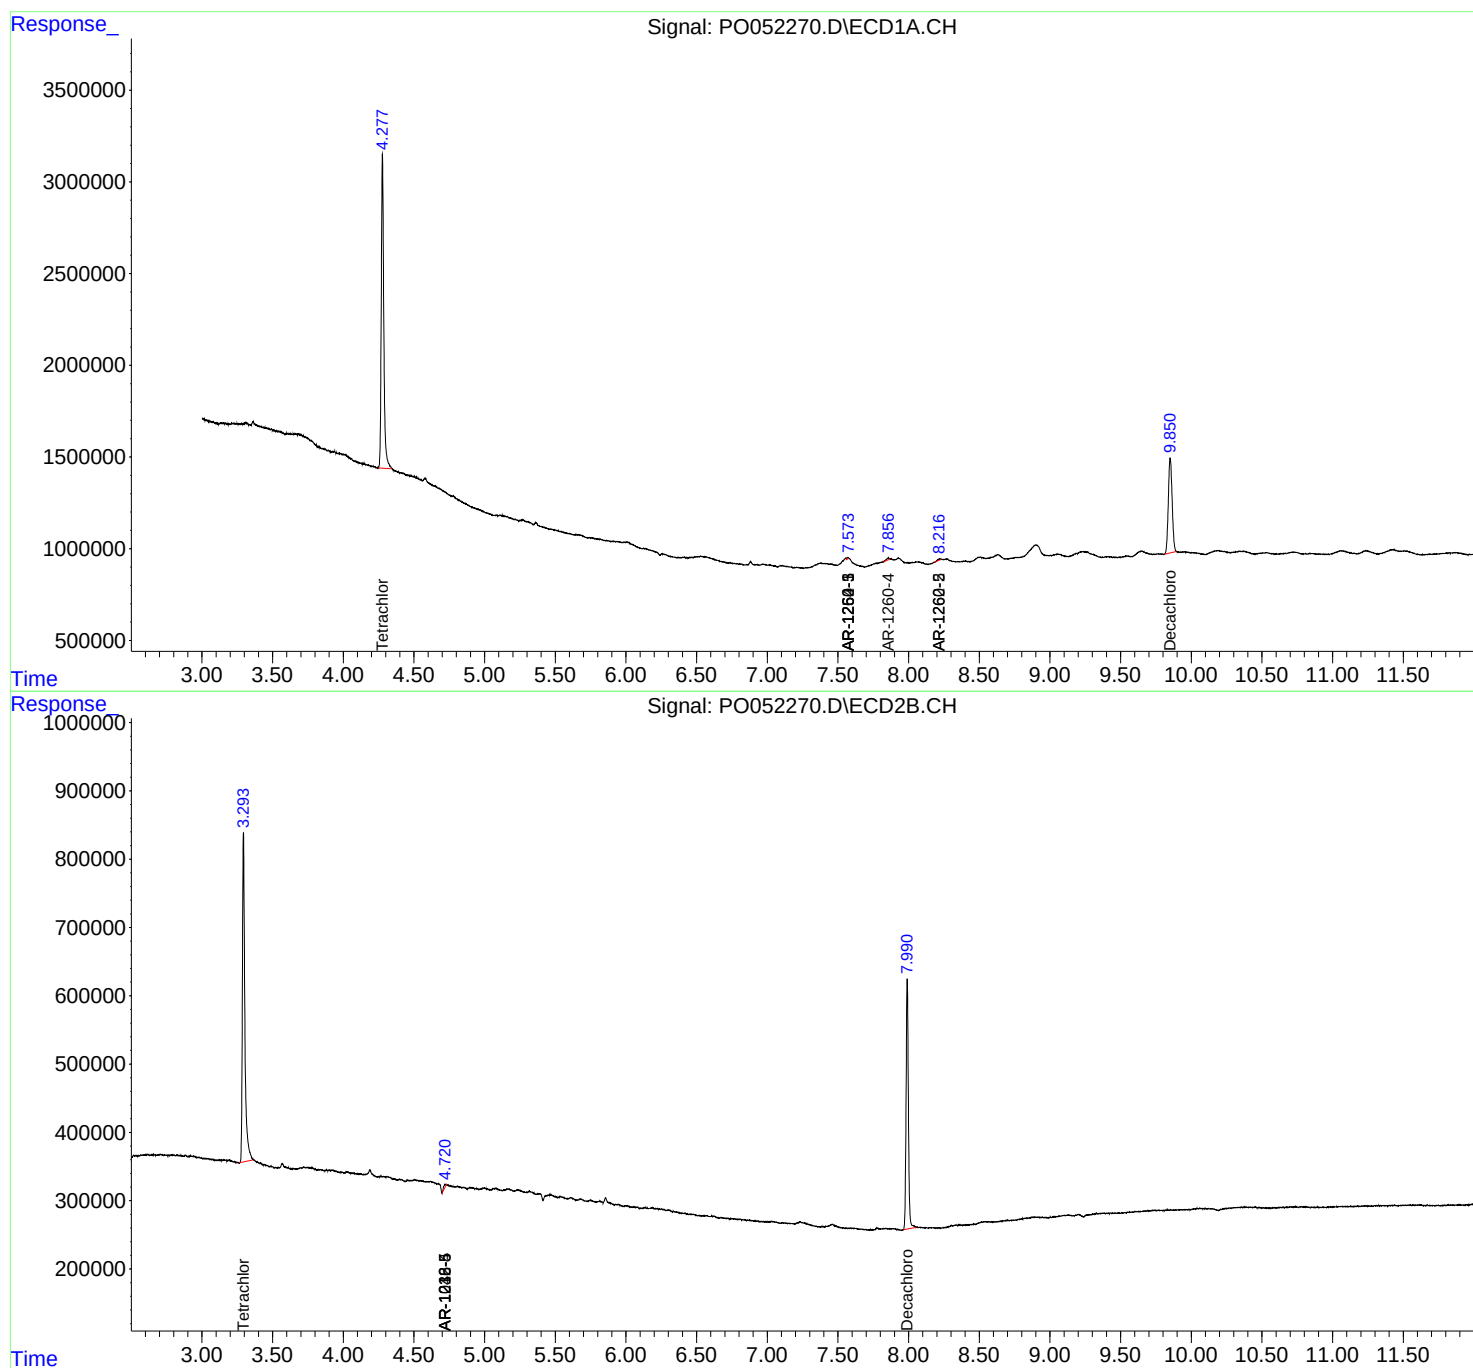


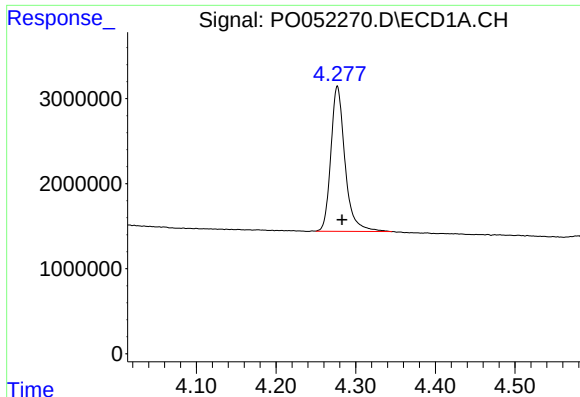

#1 Tetrachloro-m-xylene


R.T.: 4.277 min
Delta R.T.: -0.006 min
Response: 21091384
Conc: 24.50 ng/ml

Instrument :
ECD_O
ClientSampleId :

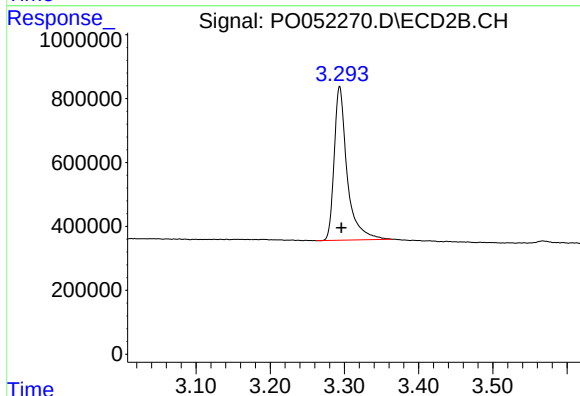


#1 Tetrachloro-m-xylene

R.T.: 3.294 min
Delta R.T.: -0.002 min
Response: 5843665
Conc: 26.20 ng/ml

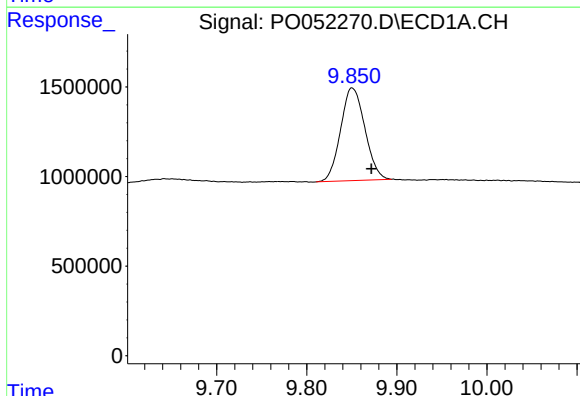


#2 Decachlorobiphenyl

R.T.: 9.850 min
Delta R.T.: -0.022 min
Response: 9698146
Conc: 19.38 ng/ml

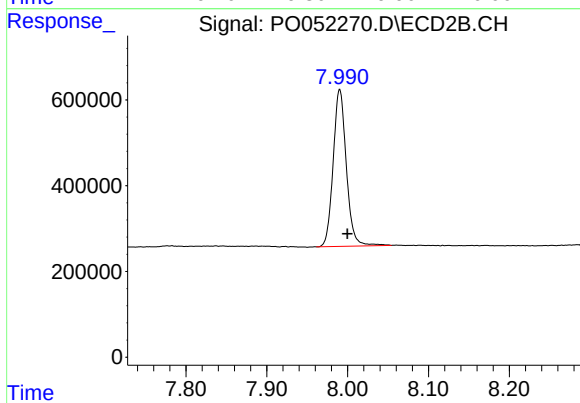

#2 Decachlorobiphenyl


R.T.: 7.990 min
Delta R.T.: -0.010 min
Response: 4136177
Conc: 19.84 ng/ml

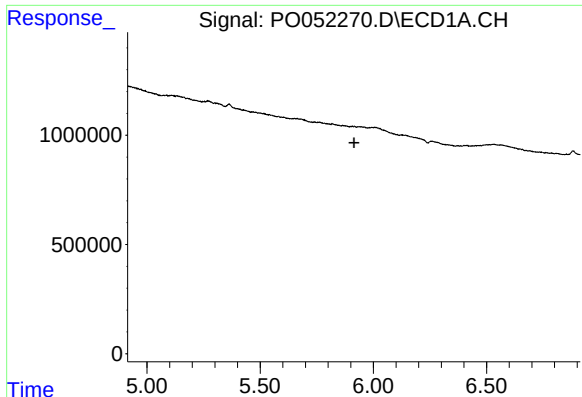

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 5.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

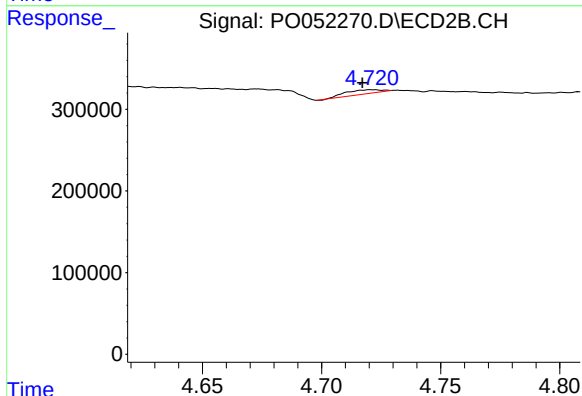


#7 AR-1016-5

R.T.: 4.720 min
Delta R.T.: 0.003 min
Response: 50574
Conc: 7.32 ng/ml

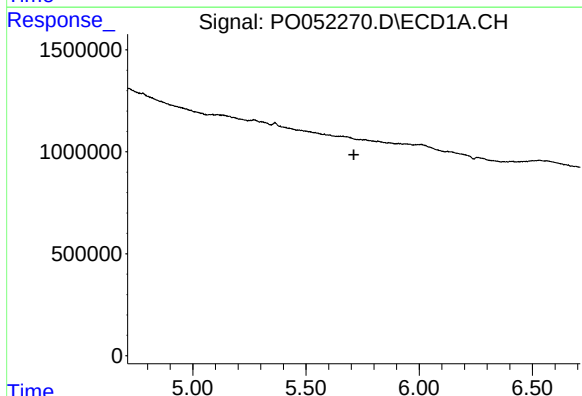


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.711 min
Response: 0
Conc: N.D.

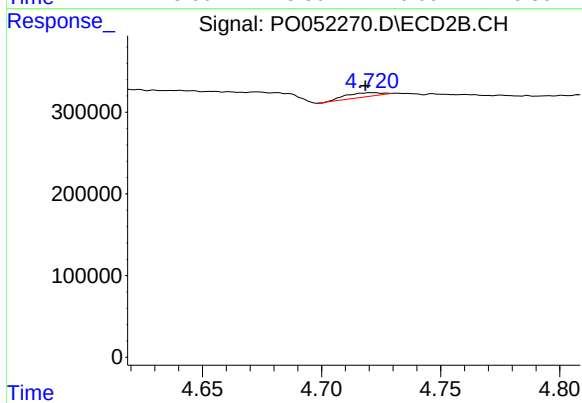

#15 AR-1232-5


R.T.: 4.720 min
Delta R.T.: 0.002 min
Response: 50574
Conc: 20.18 ng/ml

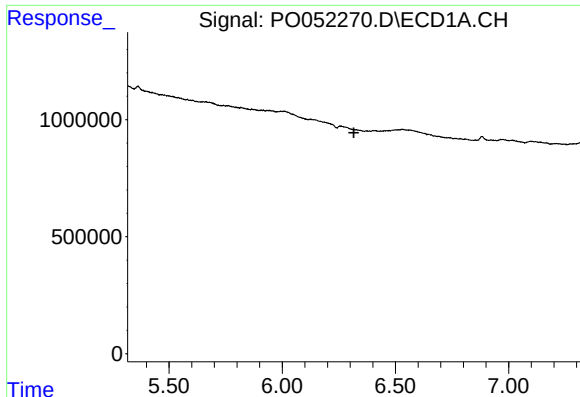

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 6.316 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

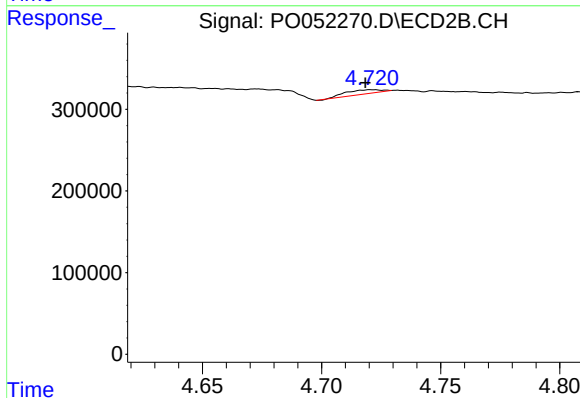


#24 AR-1248-4

R.T.: 4.720 min
Delta R.T.: 0.002 min
Response: 50574
Conc: 6.13 ng/ml

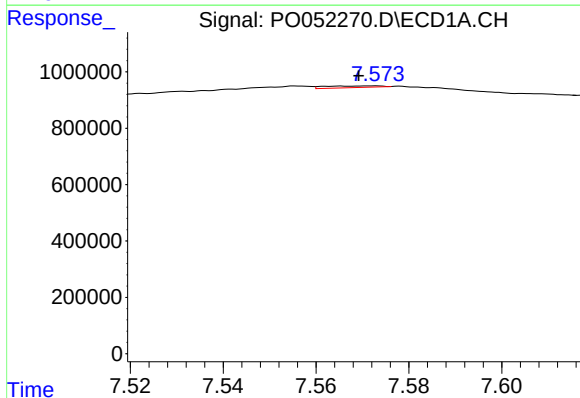


#30 AR-1254-5

R.T.: 7.573 min
Delta R.T.: 0.004 min
Response: 49318
Conc: 1.67 ng/ml

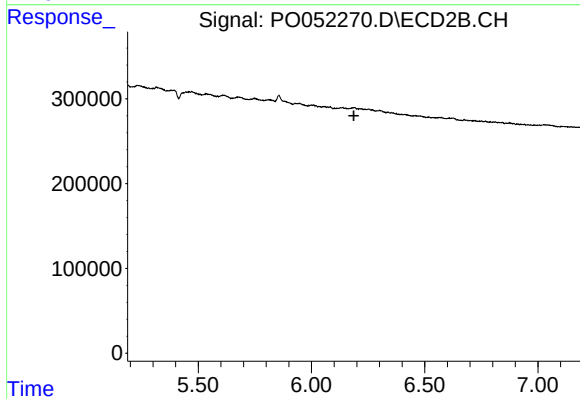

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T.: 6.187 min
Response: 0
Conc: N.D.

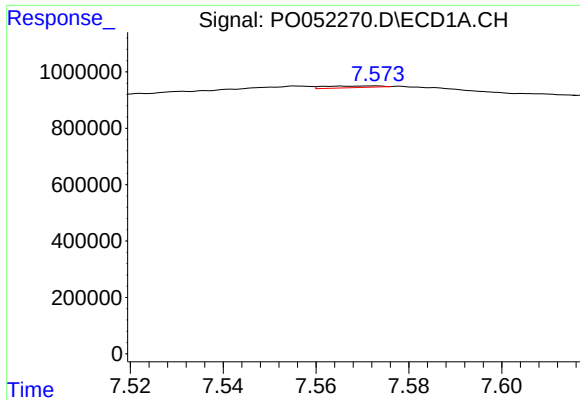

#33 AR-1260-3


R.T.: 7.573 min
Delta R.T.: -0.068 min
Response: 49318
Conc: 2.04 ng/ml

Instrument :
ECD_O
ClientSampleId :

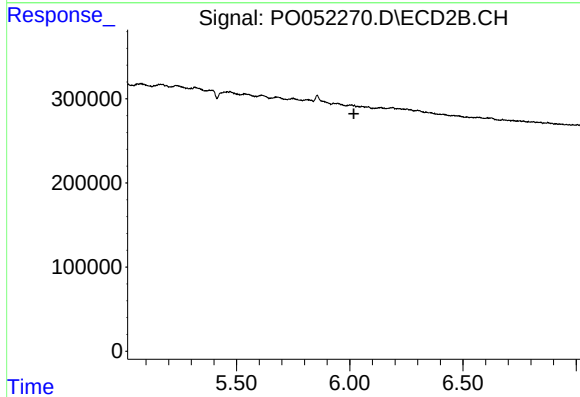


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.018 min
Response: 0
Conc: N.D.

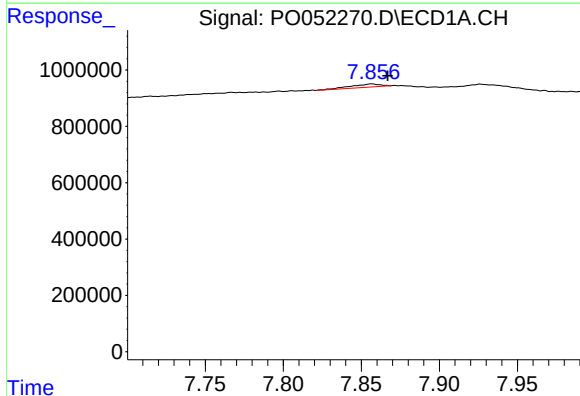


#34 AR-1260-4

R.T.: 7.857 min
Delta R.T.: -0.010 min
Response: 156778
Conc: 6.41 ng/ml

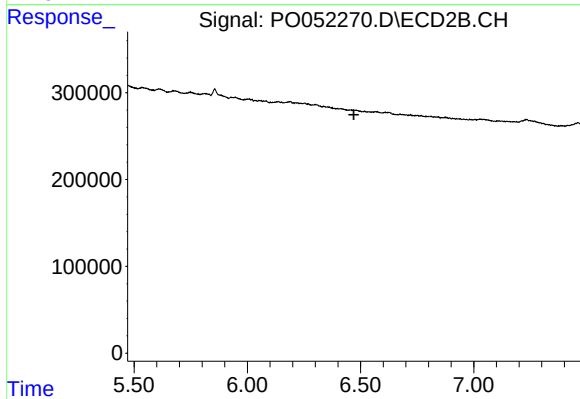

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 6.471 min
Response: 0
Conc: N.D.

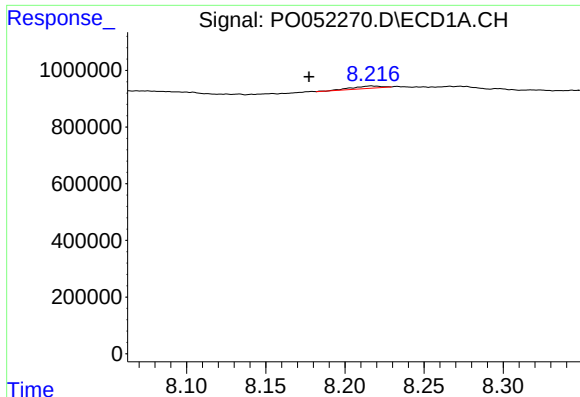

#35 AR-1260-5


R.T.: 8.217 min
Delta R.T.: 0.039 min
Response: 100740
Conc: 2.05 ng/ml

Instrument :
ECD_O
ClientSampleId :

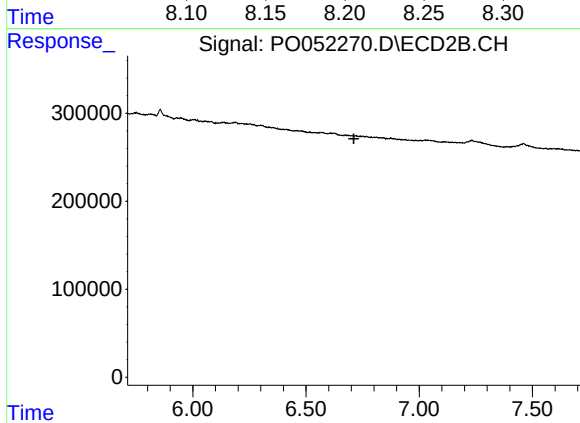


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 6.711 min
Response: 0
Conc: N.D.

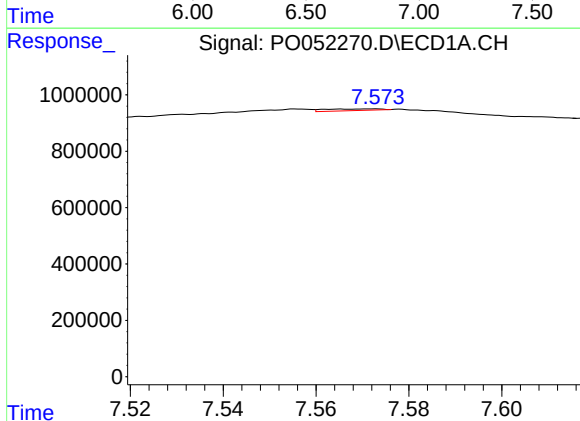


#36 AR-1262-1

R.T.: 7.573 min
Delta R.T.: -0.068 min
Response: 49318
Conc: 1.21 ng/ml

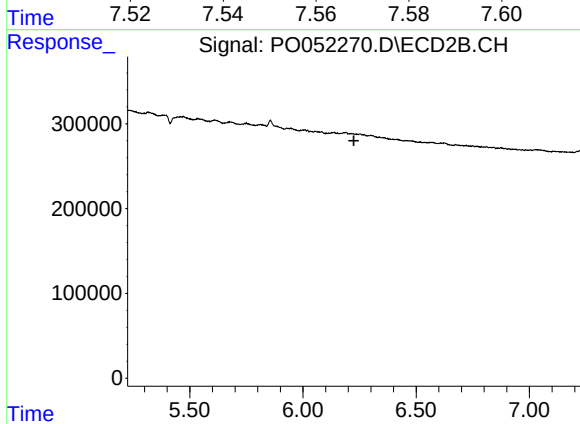

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 6.225 min
Response: 0
Conc: N.D.

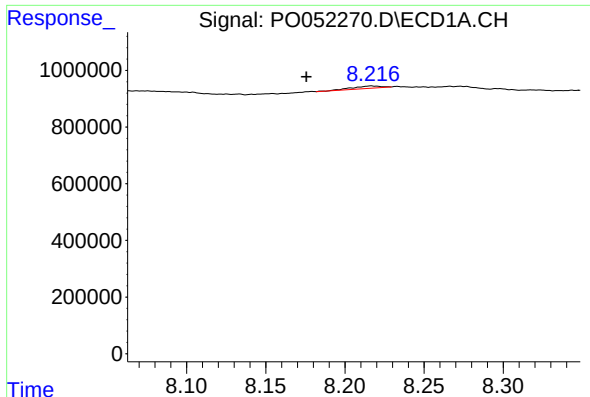

#37 AR-1262-2

R.T.: 8.217 min
Delta R.T.: 0.041 min
Response: 100740
Conc: 1.55 ng/ml

Instrument :
ECD_O
ClientSampleId :

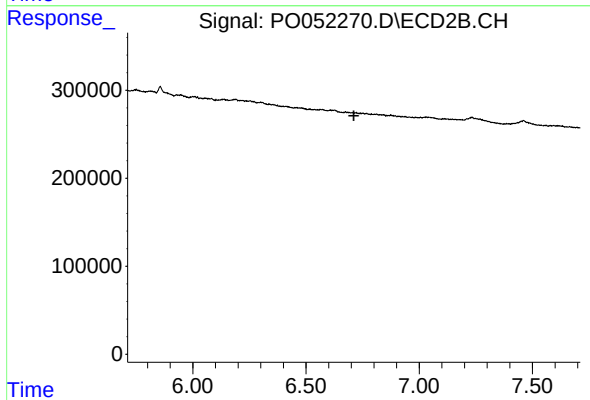

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 6.712 min
Response: 0
Conc: N.D.