

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0120518\
 Data File : P0052262.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Dec 2018 18:03
 Operator : SM/SJ
 Sample : J6194-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-02-120418-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 03:26:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0120318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 04 03:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.278	3.293	18922721	4719169	21.980	21.159
2) SA Decachlor...	9.853	7.990	7563107	2939026	15.113	14.098

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120518\
Data File : PO052262.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Dec 2018 18:03
Operator : SM/SJ
Sample : J6194-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OK-02-120418-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 03:26:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 04 03:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

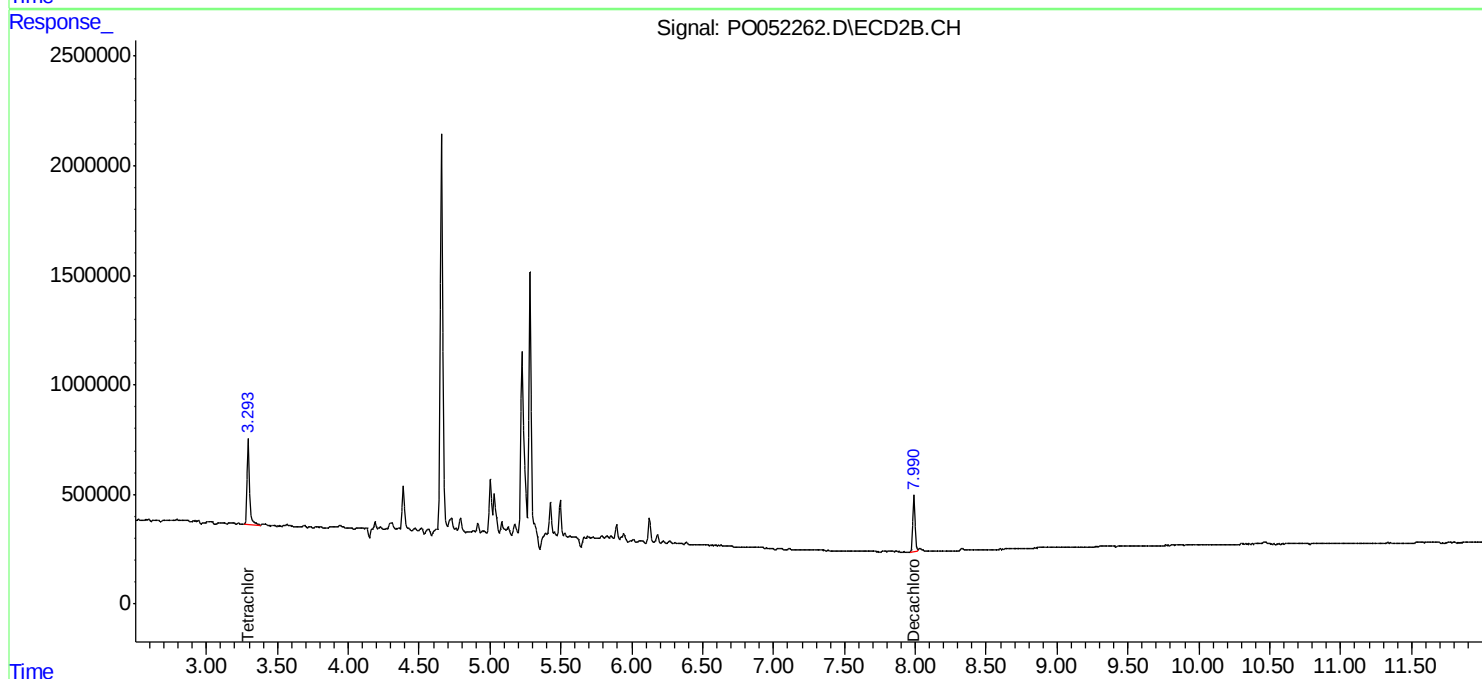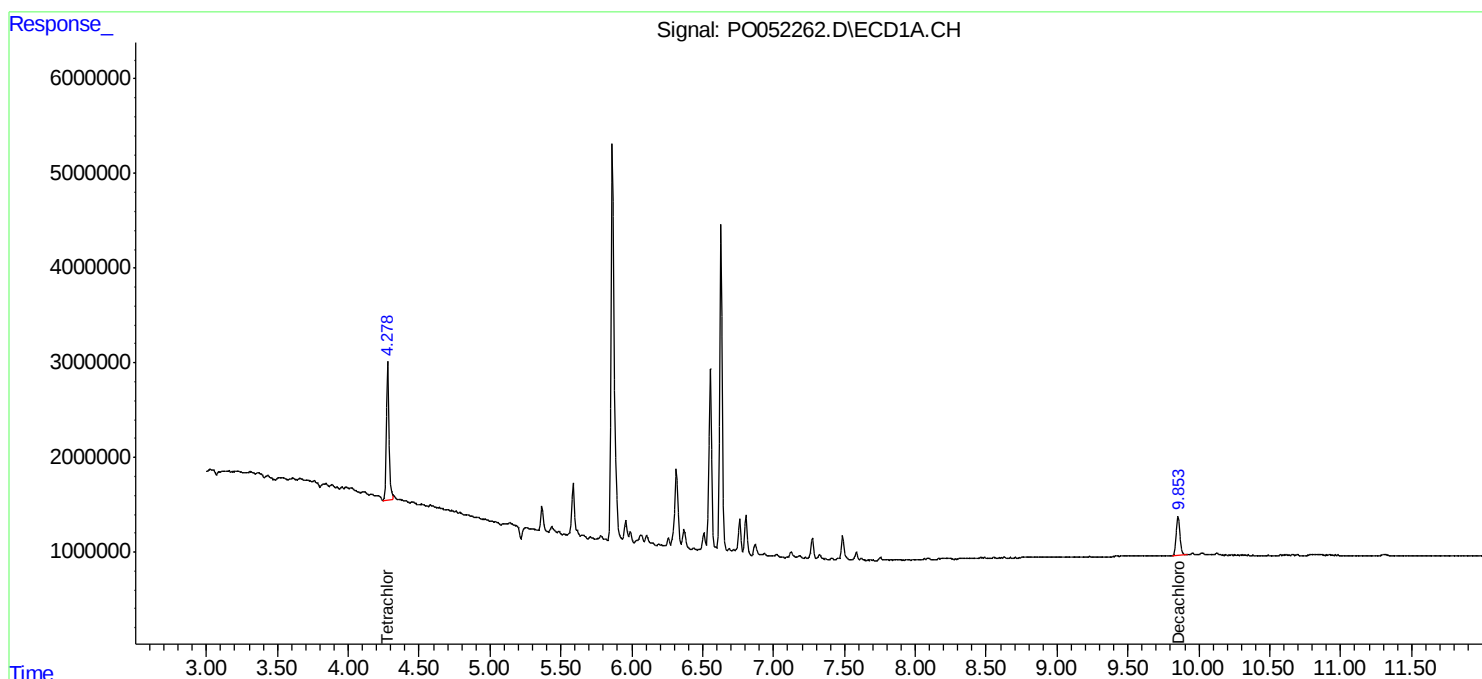


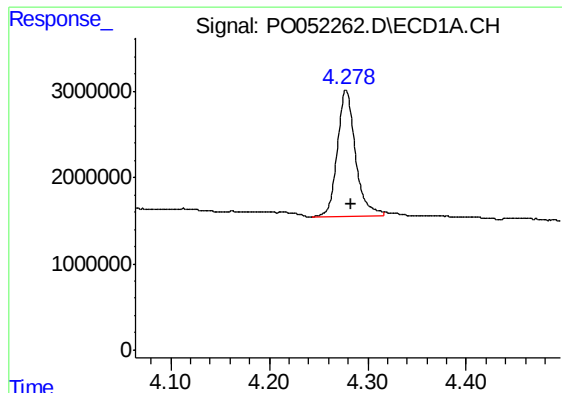

#1 Tetrachloro-m-xylene


R.T.: 4.278 min
Delta R.T.: -0.005 min
Response: 18922721
Conc: 21.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-02-120418-A

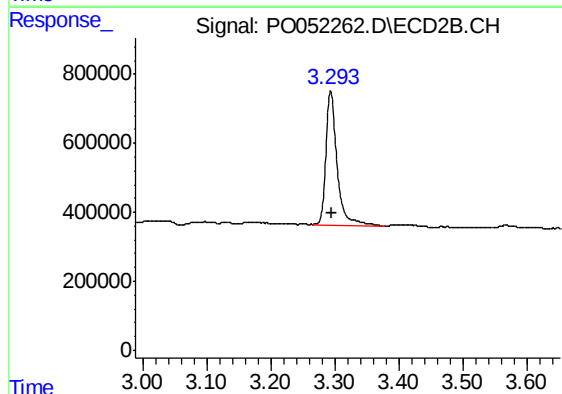


#1 Tetrachloro-m-xylene

R.T.: 3.293 min
Delta R.T.: -0.003 min
Response: 4719169
Conc: 21.16 ng/ml

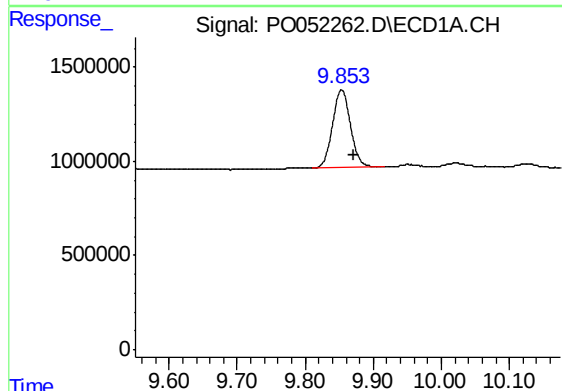

#2 Decachlorobiphenyl

R.T.: 9.853 min
Delta R.T.: -0.018 min
Response: 7563107
Conc: 15.11 ng/ml

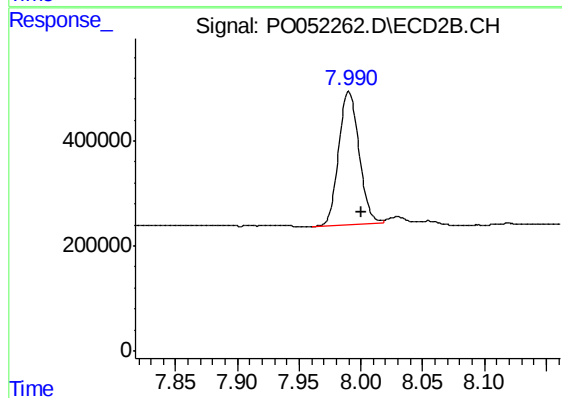

#2 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.010 min
Response: 2939026
Conc: 14.10 ng/ml