

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120518\
 Data File : P0052267.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Dec 2018 19:28
 Operator : SM/SJ
 Sample : J6214-23
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-3-(0-2)

Manual Integrations
 APPROVED

mohammad
 12/6/2018 11:08:40 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 03:27:20 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 04 03:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.276	3.293	8583484	2844836	9.970m	12.755m#
2)	SA Decachlor...	9.851	7.990	4463493	1910130	8.919	9.162

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120518\
Data File : PO052267.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Dec 2018 19:28
Operator : SM/SJ
Sample : J6214-23
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-3-(0-2)


Manual Integrations
APPROVED

mohammad
12/6/2018 11:08:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 03:27:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 04 03:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

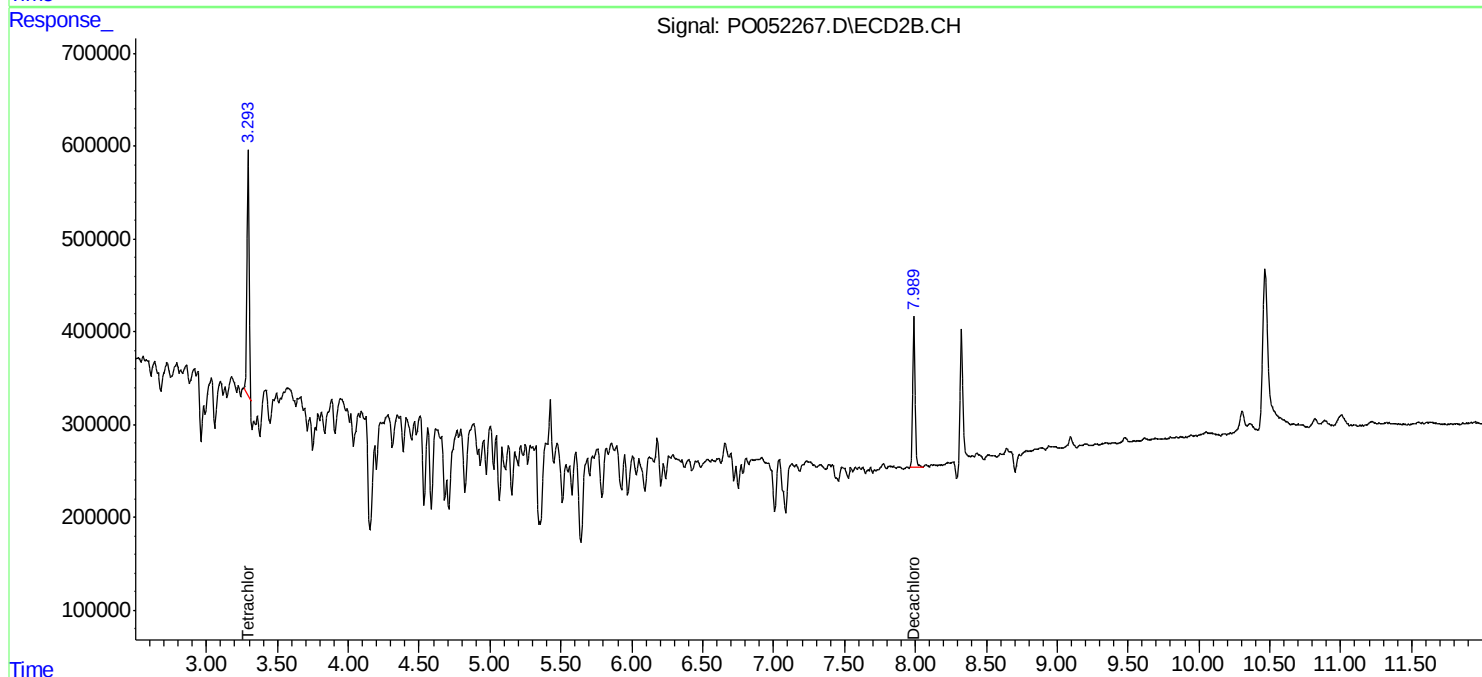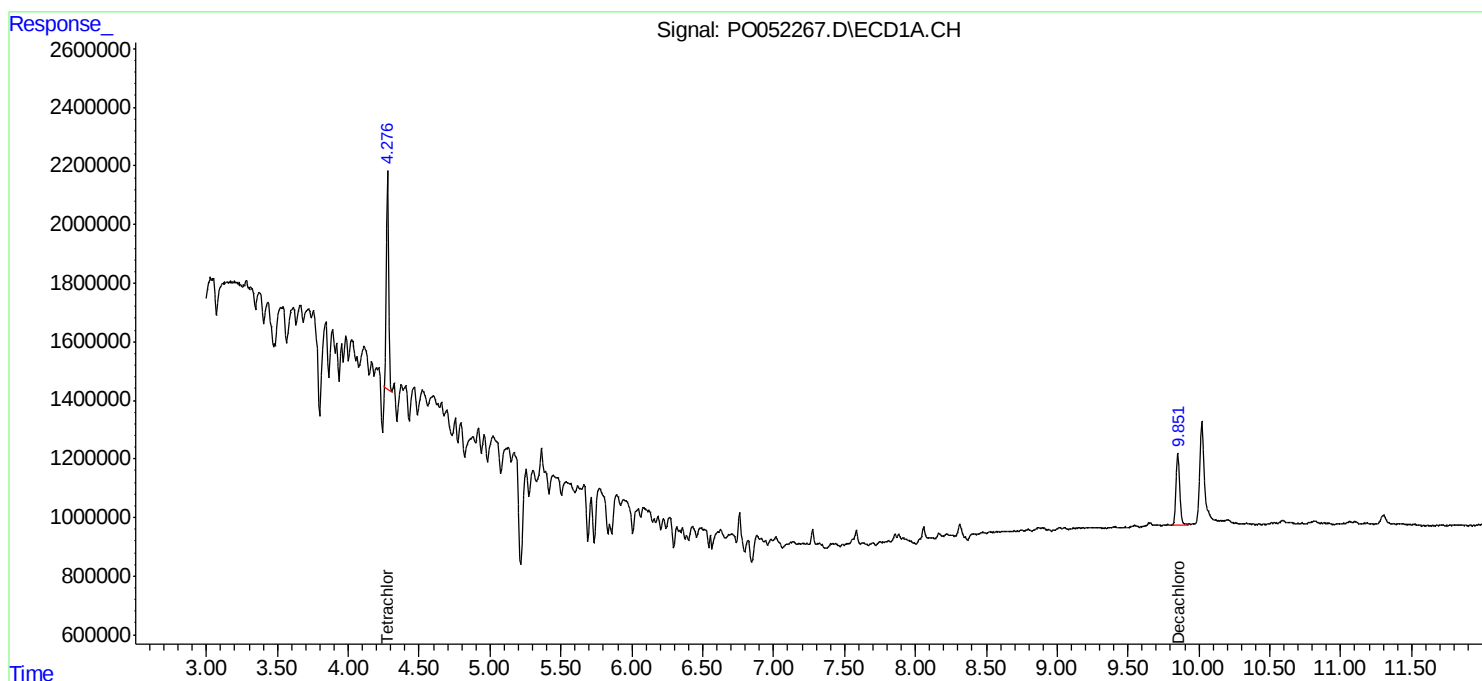

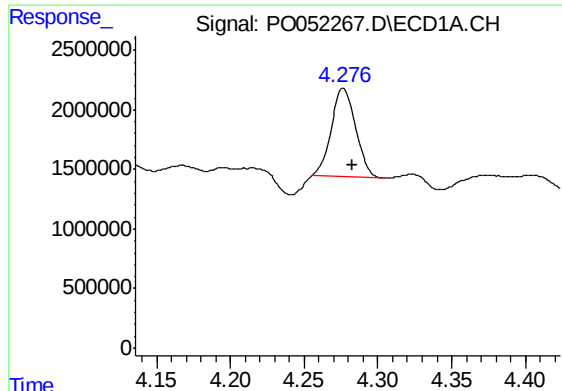


#1 Tetrachloro-m-xylene

R.T.: 4.276 min
Delta R.T.: -0.007 min
Response: 8583484
Conc: 9.97 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-3-(0-2)


Manual Integrations
APPROVED

mohammad
12/6/2018 11:08:40 AM

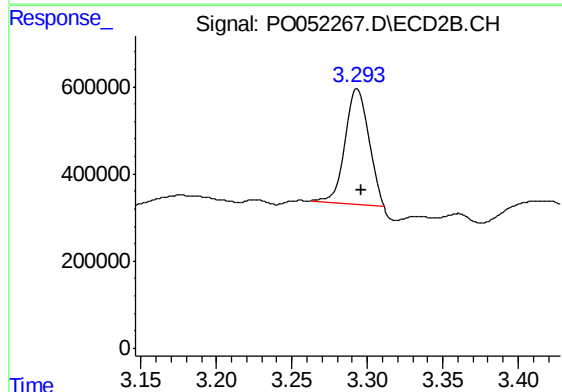


#1 Tetrachloro-m-xylene

R.T.: 3.293 min
Delta R.T.: -0.003 min
Response: 2844836
Conc: 12.76 ng/ml m

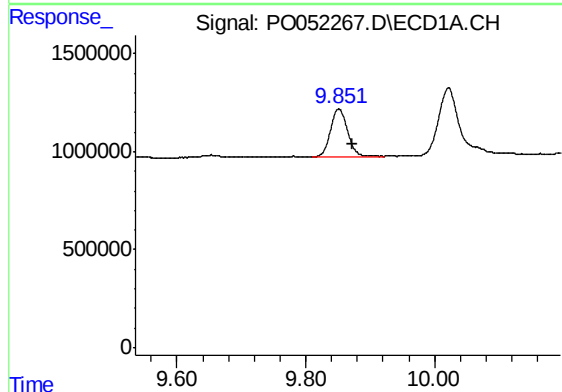

#2 Decachlorobiphenyl

R.T.: 9.851 min
Delta R.T.: -0.020 min
Response: 4463493
Conc: 8.92 ng/ml

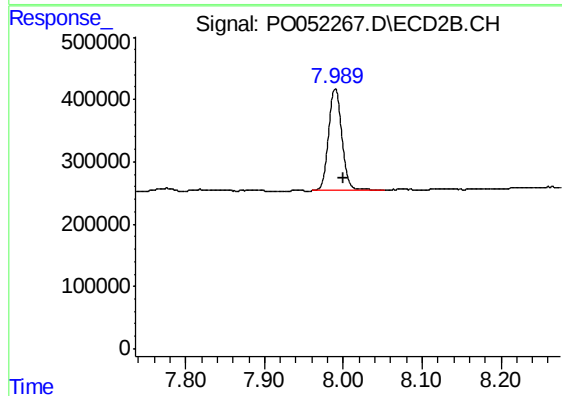

#2 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.010 min
Response: 1910130
Conc: 9.16 ng/ml