

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120522\
 Data File : P0091053.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2022 23:02
 Operator : YP/AJ
 Sample : N5876-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HILL-12-02-SIL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/06/2022
 Supervised By :Ankita Jodhani 12/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 01:29:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 28 11:25:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.291	3.480	62382014	175.5E6	18.450m	167.165m#
2) SA Decachlor...	10.042	8.477	44762674	18372292	16.852	18.924

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120522\
Data File : PO091053.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2022 23:02
Operator : YP/AJ
Sample : N5876-04
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HILL-12-02-SIL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/06/2022
Supervised By :Ankita Jodhani 12/06/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 01:29:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112522.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 28 11:25:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

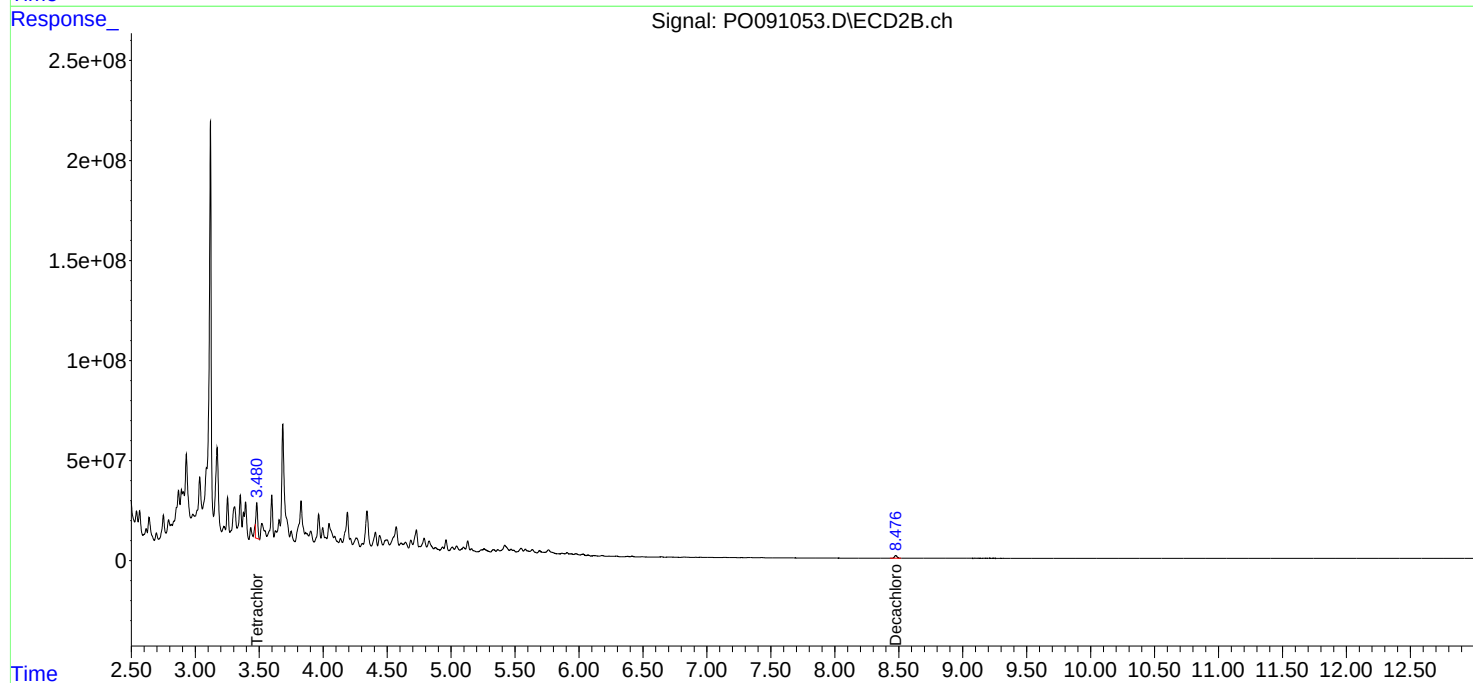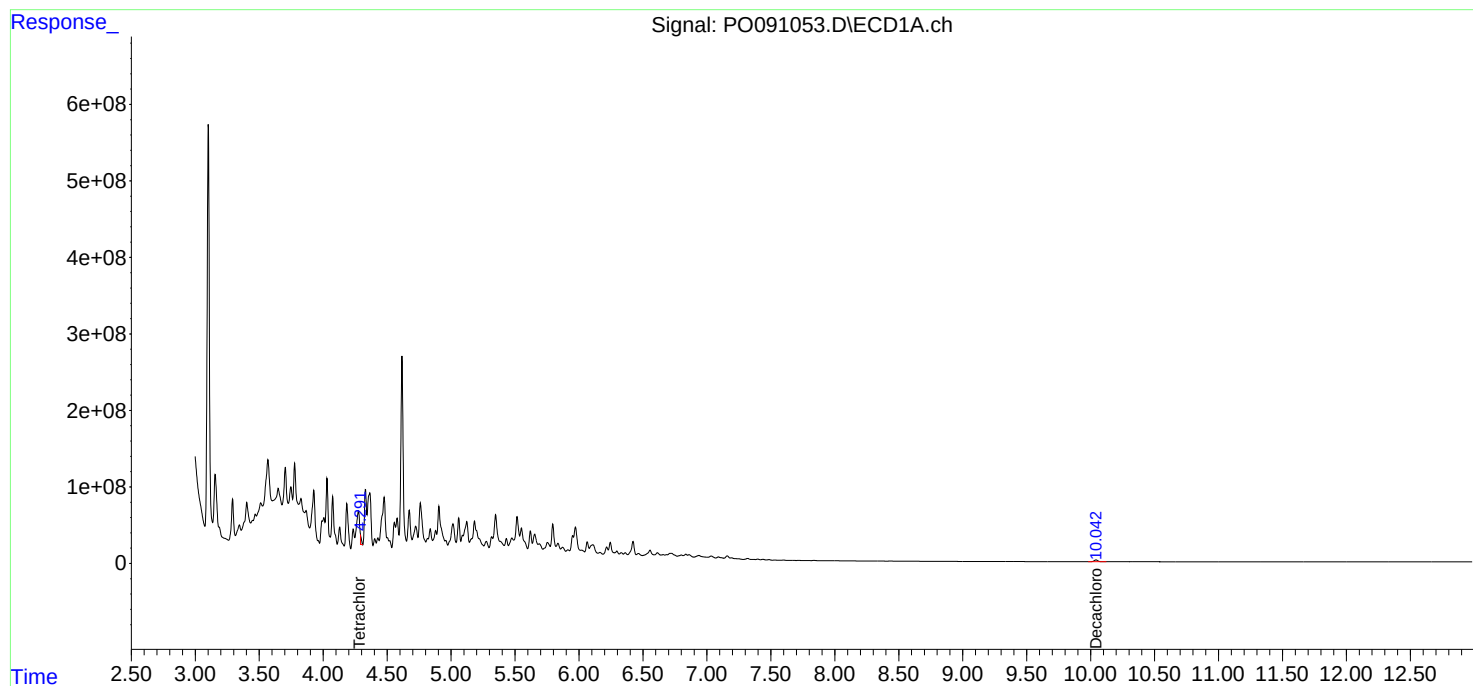

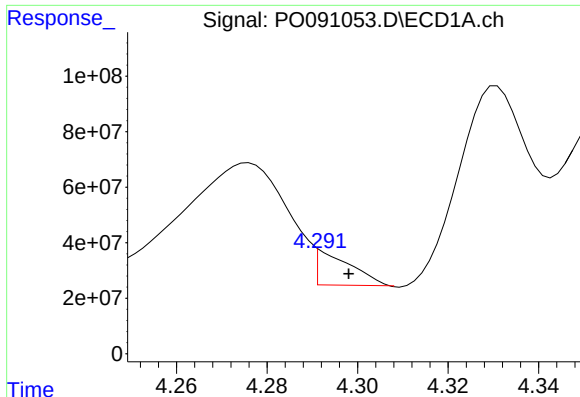


#1 Tetrachloro-m-xylene

R.T.: 4.291 min
Delta R.T.: -0.007 min
Response: 62382014
Conc: 18.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
HILL-12-02-SIL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/06/2022
Supervised By :Ankita Jodhani 12/06/2022

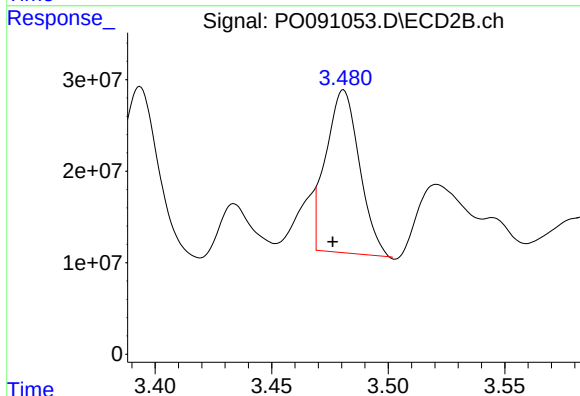


#1 Tetrachloro-m-xylene

R.T.: 3.480 min
Delta R.T.: 0.004 min
Response: 175450287
Conc: 167.17 ng/ml m

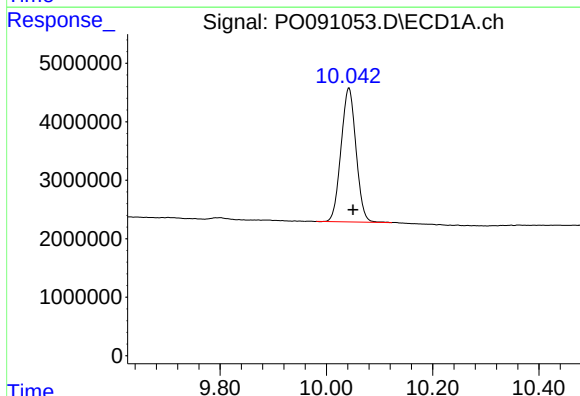

#2 Decachlorobiphenyl

R.T.: 10.042 min
Delta R.T.: -0.007 min
Response: 44762674
Conc: 16.85 ng/ml

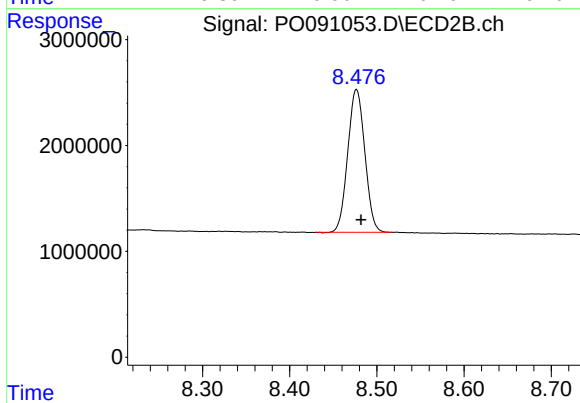

#2 Decachlorobiphenyl

R.T.: 8.477 min
Delta R.T.: -0.005 min
Response: 18372292
Conc: 18.92 ng/ml