

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120522\
 Data File : PO091068.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2022 04:13
 Operator : YP/AJ
 Sample : N5857-01
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-SAMPLE-TANK-10-11-12-31-33

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 05:12:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 28 11:25:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.298	3.475	48943252	15869785	14.476	15.120
2) SA Decachlor...	10.042	8.476	23741607	10060165	8.938	10.362

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120522\
Data File : PO091068.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2022 04:13
Operator : YP/AJ
Sample : N5857-01
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
COMP-SAMPLE-TANK-10-11-12-31-33

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 05:12:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112522.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 28 11:25:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

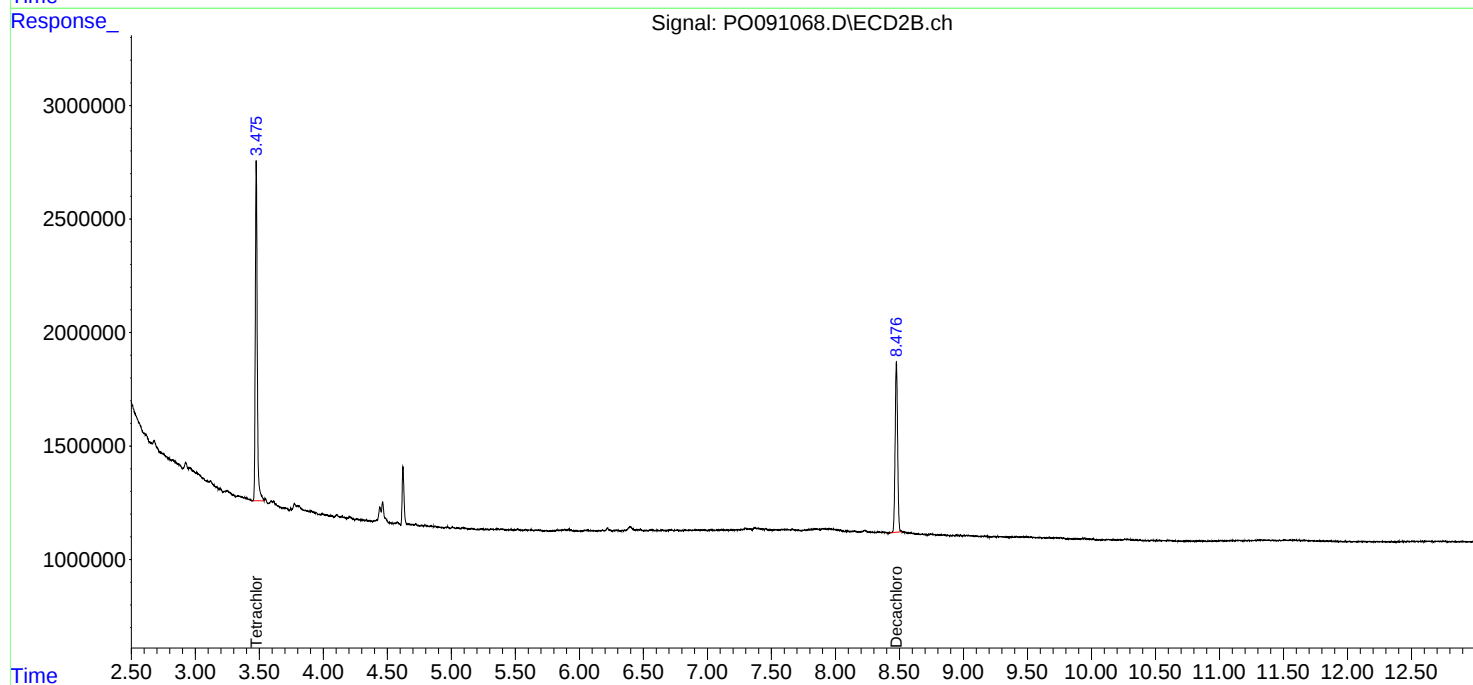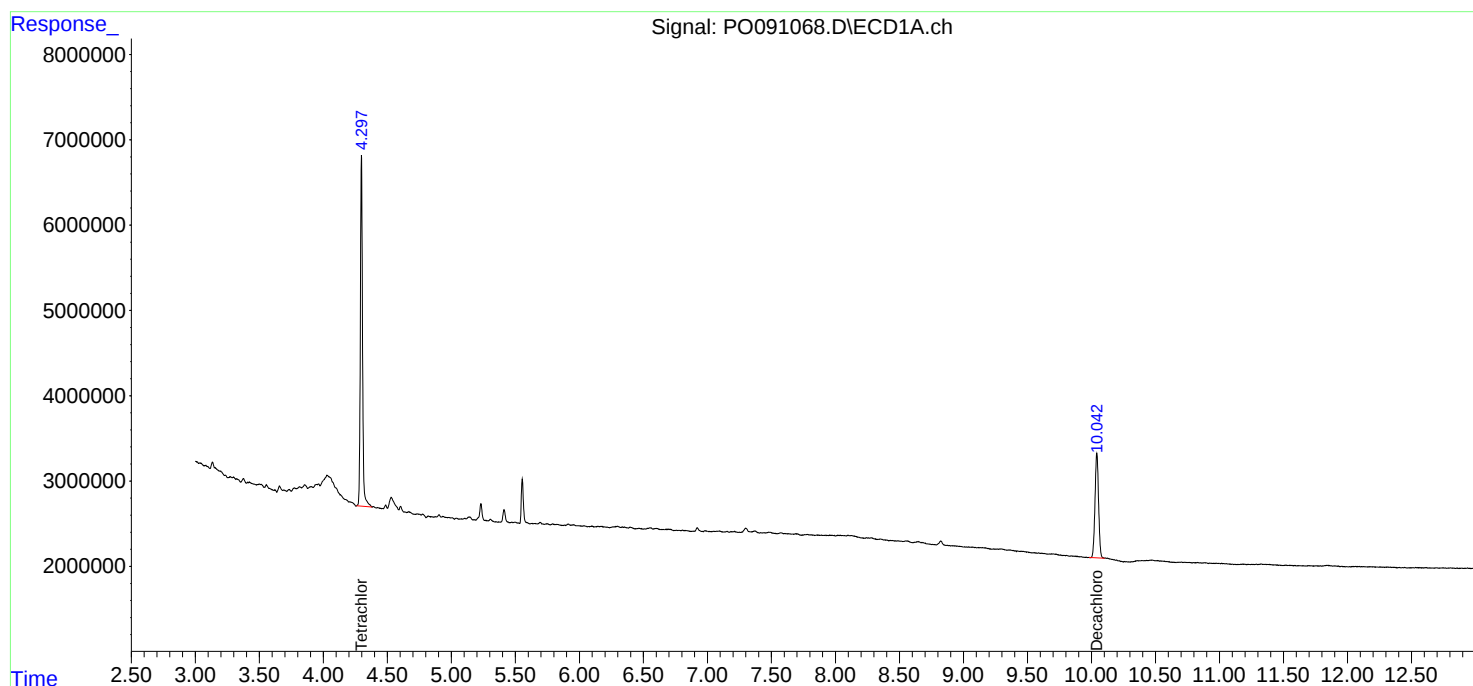

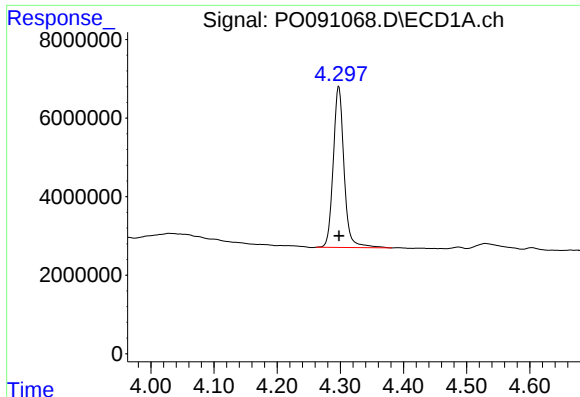

#1 Tetrachloro-m-xylene


R.T.: 4.298 min
Delta R.T.: 0.000 min
Response: 48943252
Conc: 14.48 ng/ml

Instrument :

ECD_O


ClientSampleId :

COMP-SAMPLE-TANK-10-11-12-31-33

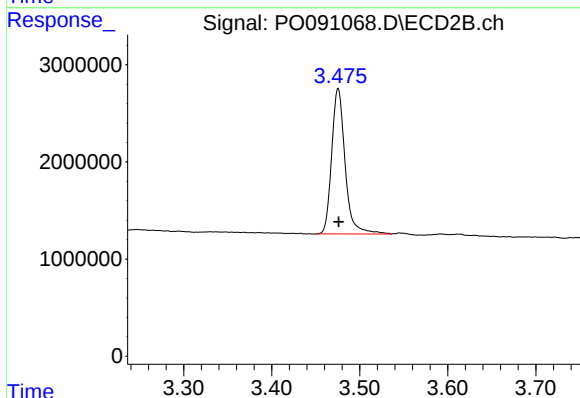


#1 Tetrachloro-m-xylene

R.T.: 3.475 min
Delta R.T.: 0.000 min
Response: 15869785
Conc: 15.12 ng/ml

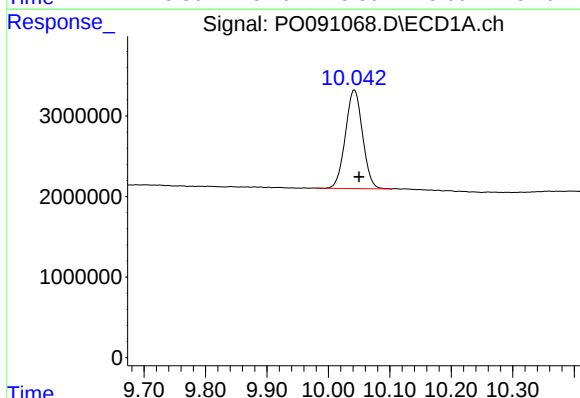

#2 Decachlorobiphenyl

R.T.: 10.042 min
Delta R.T.: -0.008 min
Response: 23741607
Conc: 8.94 ng/ml

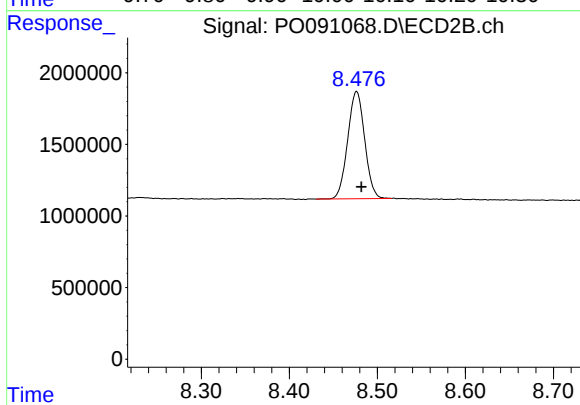

#2 Decachlorobiphenyl

R.T.: 8.476 min
Delta R.T.: -0.005 min
Response: 10060165
Conc: 10.36 ng/ml