

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0120618\
 Data File : P0052288.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Dec 2018 8:43
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

mohammad
 12/7/2018 11:39:24 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 00:19:14 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0120318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 04 03:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.279	3.293	22900267	6307829	26.600	28.282
2) SA Decachlor...	9.853	7.988	10047685	4641407	20.077m	22.264

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120618\
Data File : PO052288.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Dec 2018 8:43
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

mohammad
12/7/2018 11:39:24 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 00:19:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 04 03:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

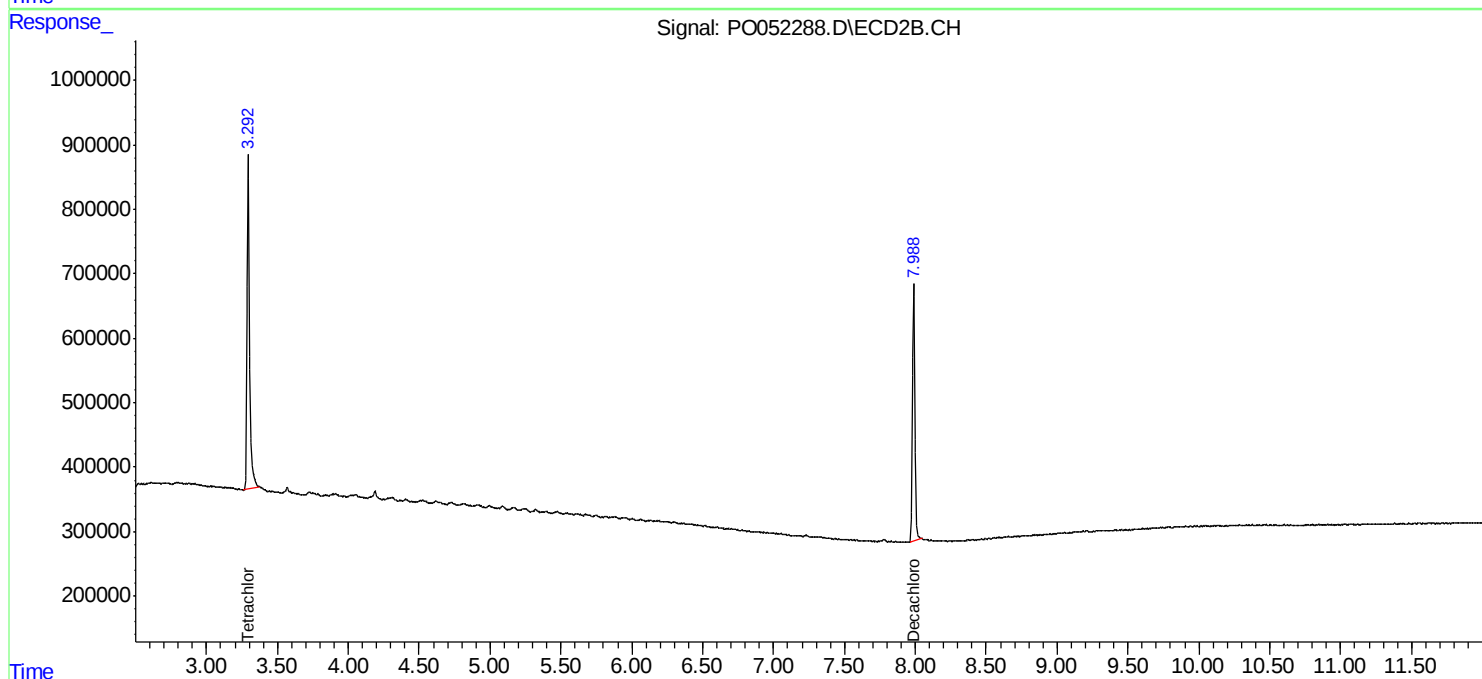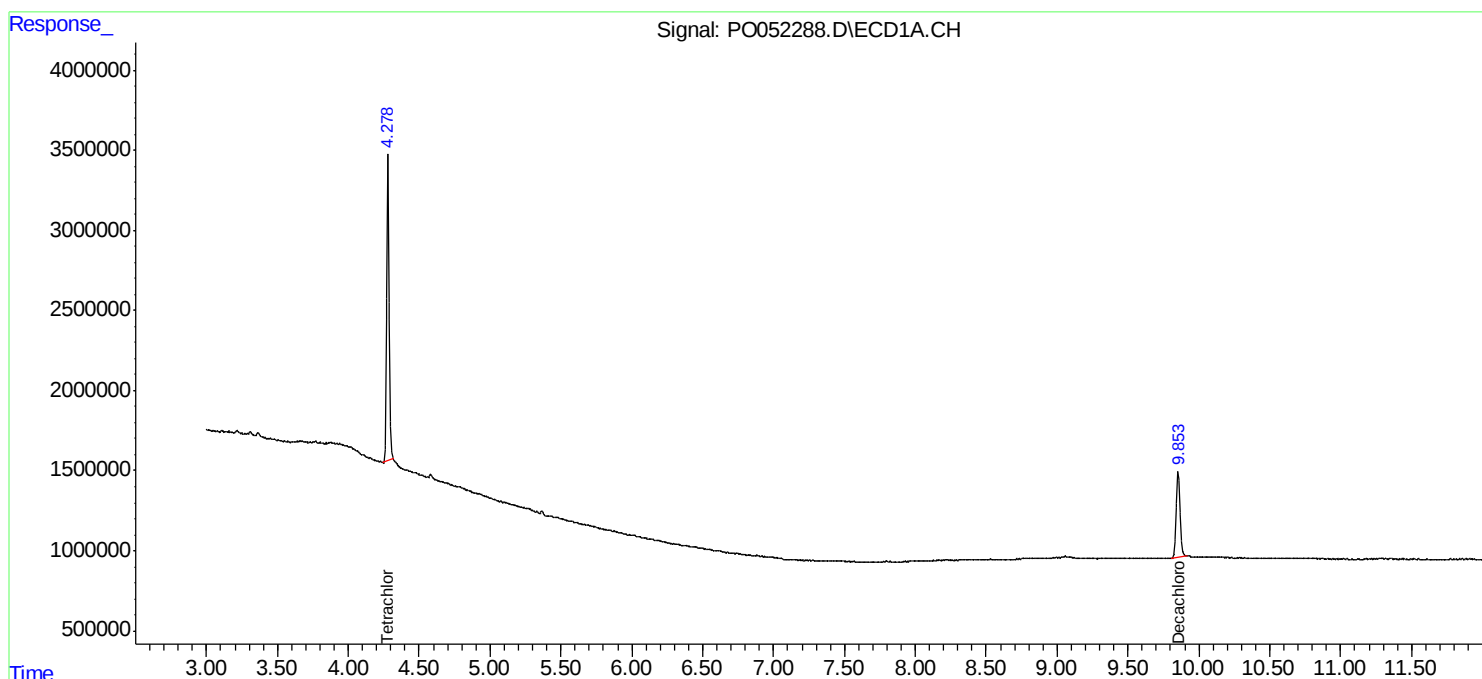

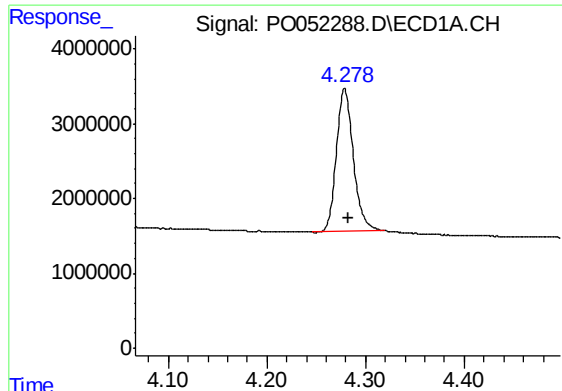


#1 Tetrachloro-m-xylene

R.T.: 4.279 min
Delta R.T.: -0.004 min
Response: 22900267
Conc: 26.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

mohammad
12/7/2018 11:39:24 AM

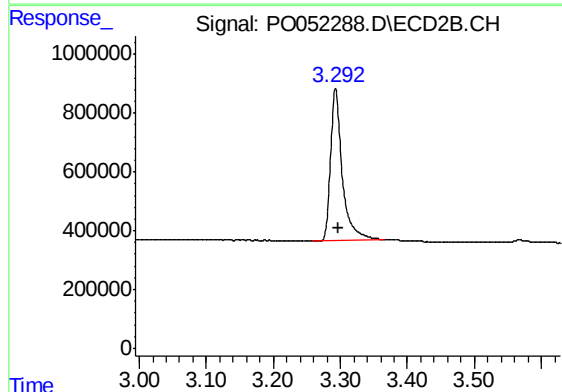


#1 Tetrachloro-m-xylene

R.T.: 3.293 min
Delta R.T.: -0.003 min
Response: 6307829
Conc: 28.28 ng/ml

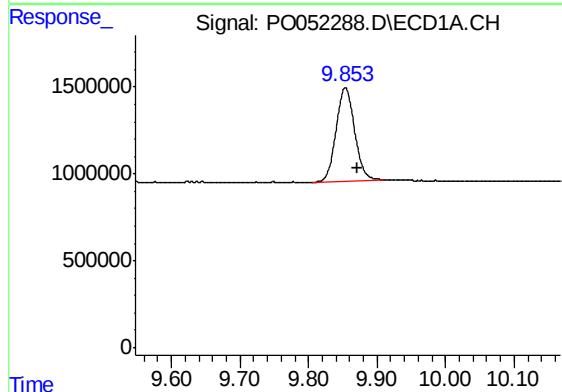

#2 Decachlorobiphenyl

R.T.: 9.853 min
Delta R.T.: -0.018 min
Response: 10047685
Conc: 20.08 ng/ml m

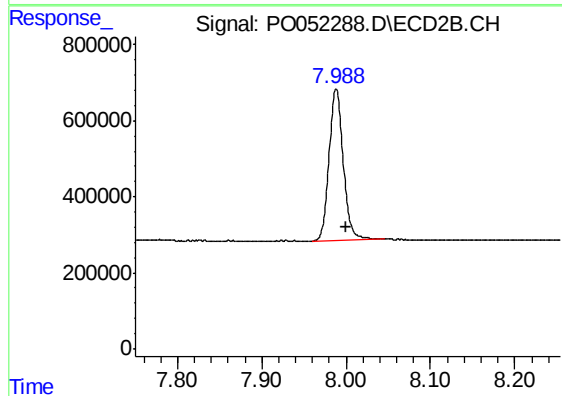

#2 Decachlorobiphenyl

R.T.: 7.988 min
Delta R.T.: -0.012 min
Response: 4641407
Conc: 22.26 ng/ml