

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120619\
 Data File : P0064450.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Dec 2019 20:52
 Operator : SM/AJ
 Sample : K6133-01
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ROLL-OFF-362

Manual Integrations
 APPROVED

mohammad
 12/9/2019 12:06:14 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 22:55:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 28 01:28:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.313	3.561	858792	736587	28.998	30.968
2) SA Decachlor...	9.934	8.517	700330	658520	17.088m	16.120m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120619\
Data File : P0064450.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Dec 2019 20:52
Operator : SM/AJ
Sample : K6133-01
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ROLL-OFF-362


Manual Integrations
APPROVED

mohammad
12/9/2019 12:06:14 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 22:55:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112719.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 28 01:28:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

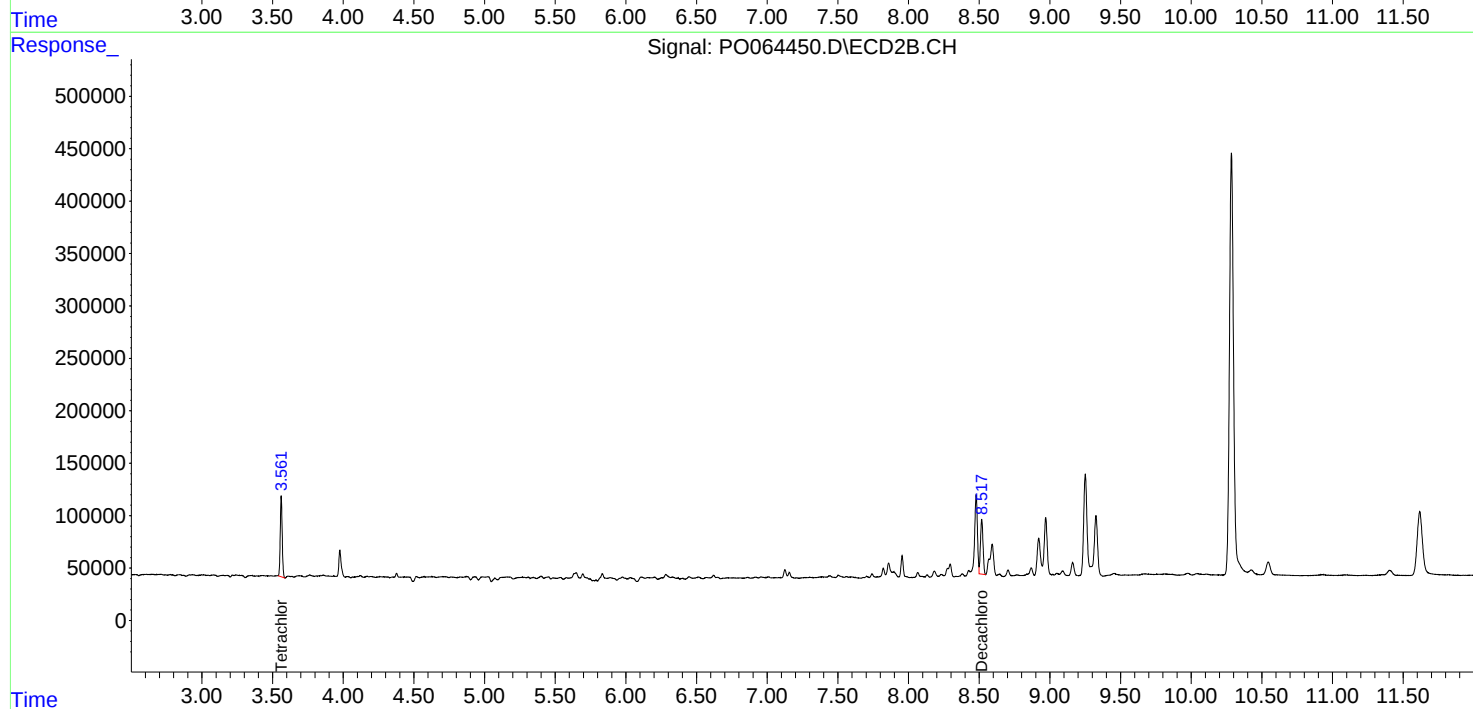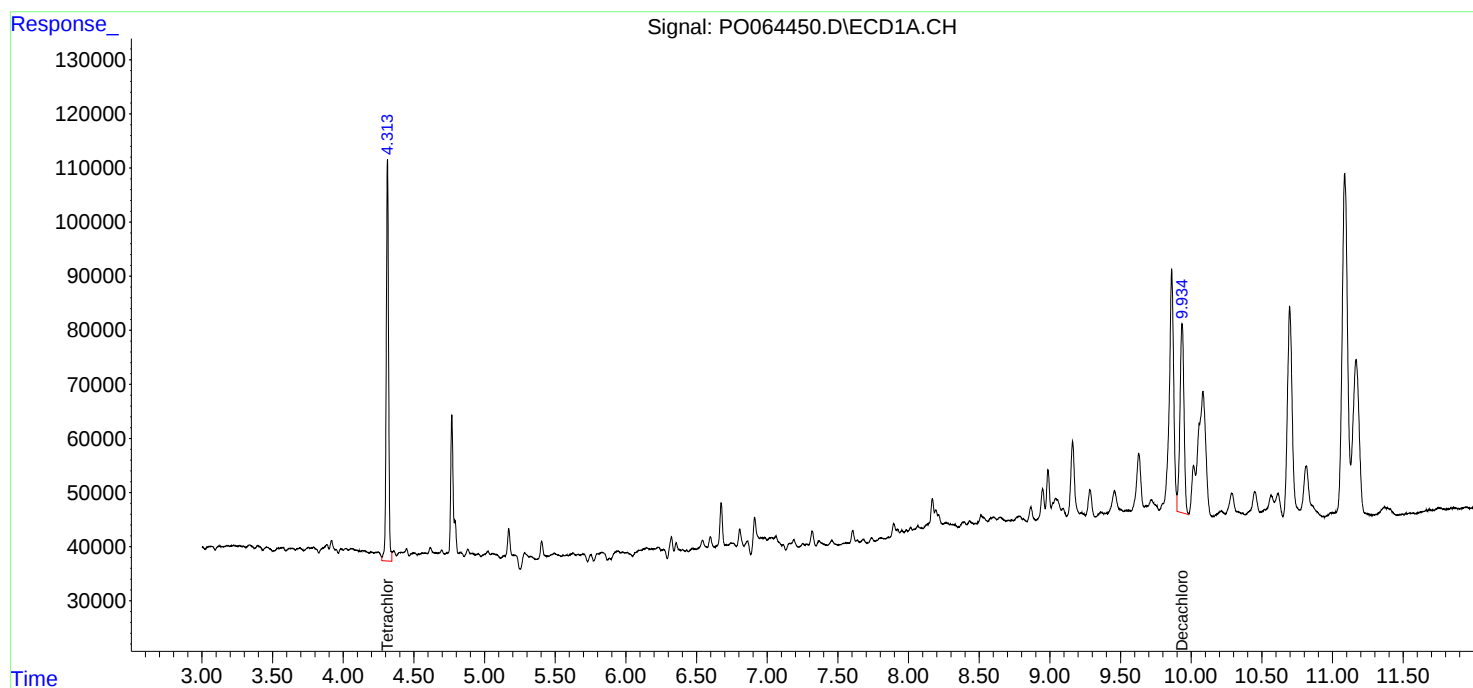

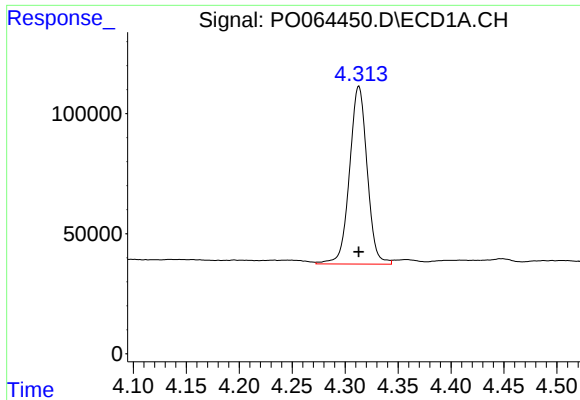


#1 Tetrachloro-m-xylene

R.T.: 4.313 min
Delta R.T.: 0.000 min
Response: 858792
Conc: 29.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
ROLL-OFF-362


Manual Integrations
APPROVED

mohammad
12/9/2019 12:06:14 PM

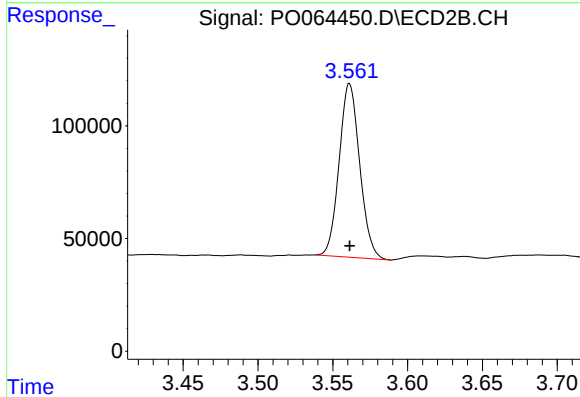


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: 0.000 min
Response: 736587
Conc: 30.97 ng/ml

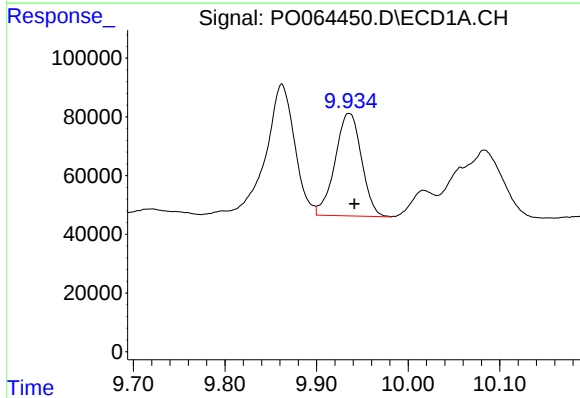

#2 Decachlorobiphenyl

R.T.: 9.934 min
Delta R.T.: -0.007 min
Response: 700330
Conc: 17.09 ng/ml m

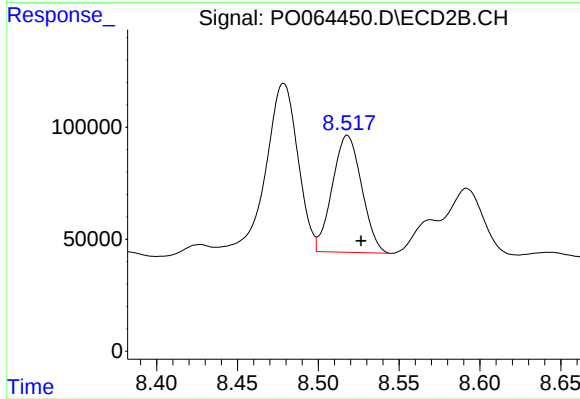

#2 Decachlorobiphenyl

R.T.: 8.517 min
Delta R.T.: -0.009 min
Response: 658520
Conc: 16.12 ng/ml m