

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120623\
 Data File : PO100335.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2023 18:01
 Operator : YP/AJ
 Sample : 05633-13 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 02-9015WBV5-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/07/2023
 Supervised By :Ankita Jodhani 12/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 00:25:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 21 15:58:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.477	3.701	2695463	2706705	1.579	1.805
2) SA Decachlor...	10.354	8.791	1500005	2337671	2.065m	2.089m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120623\
Data File : PO100335.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2023 18:01
Operator : YP/AJ
Sample : 05633-13 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
02-9015WBV5-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/07/2023
Supervised By :Ankita Jodhani 12/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 00:25:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 21 15:58:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

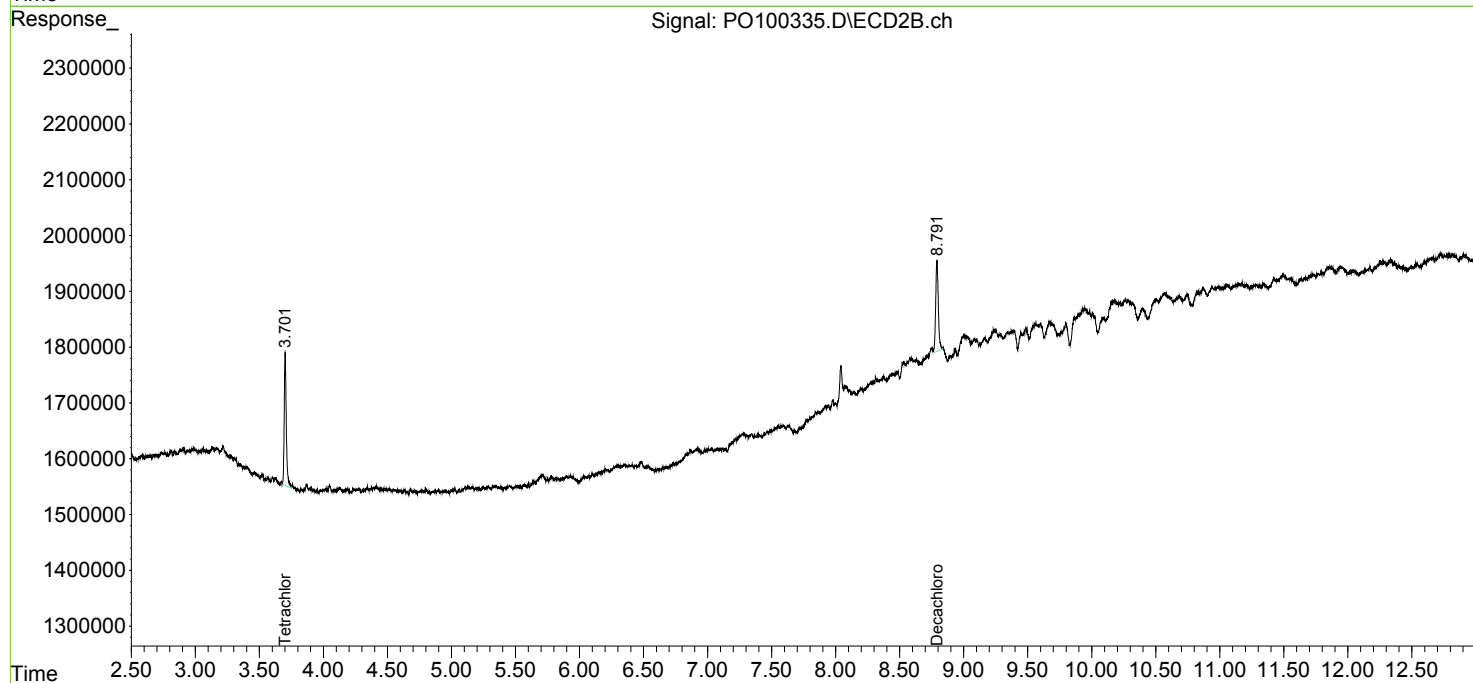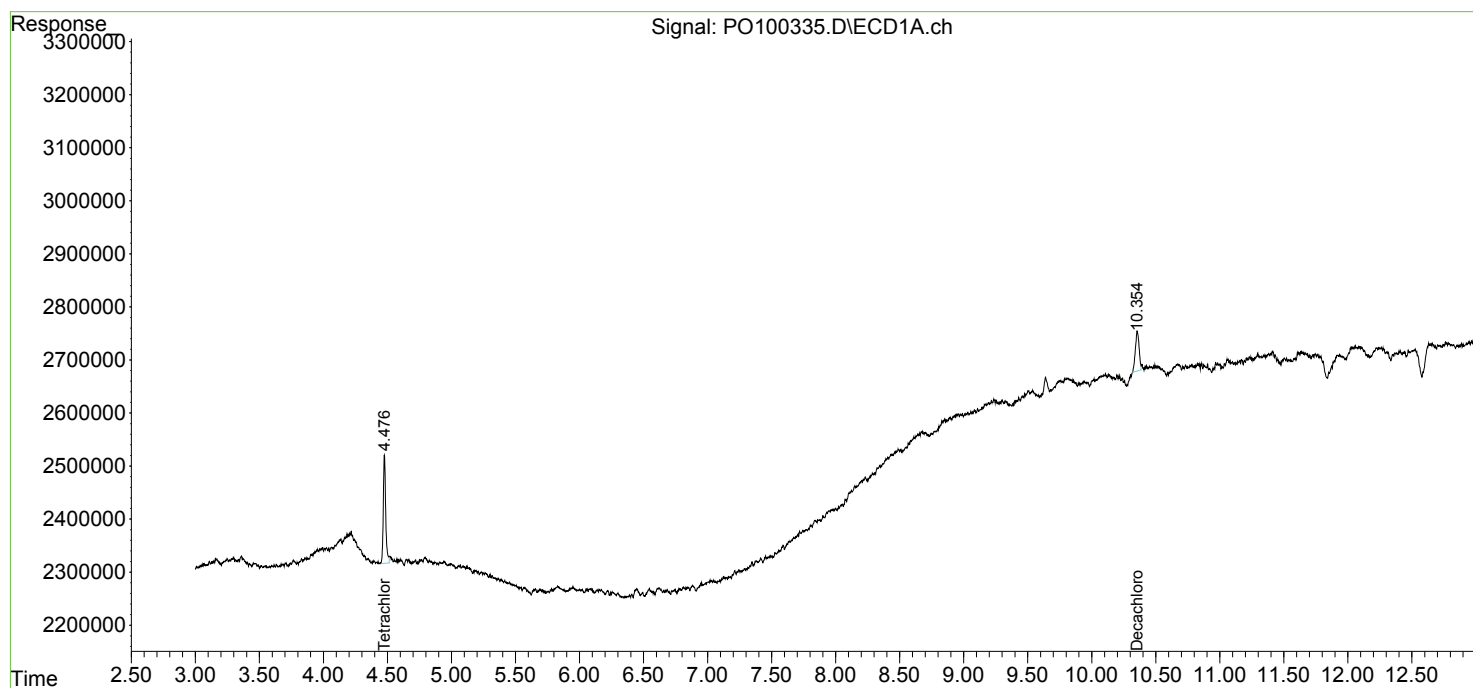

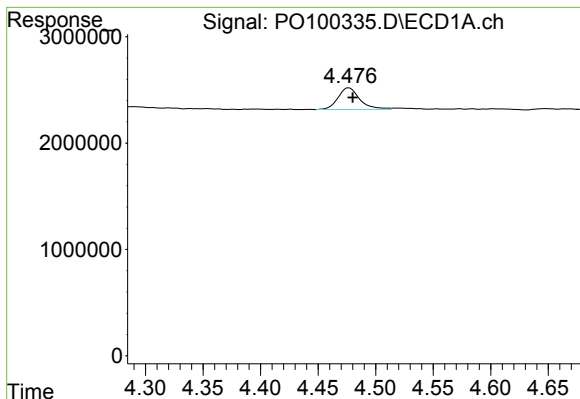


#1 Tetrachloro-m-xylene

R.T.: 4.477 min
Delta R.T.: -0.003 min
Response: 2695463
Conc: 1.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
02-9015WBV5-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/07/2023
Supervised By :Ankita Jodhani 12/07/2023

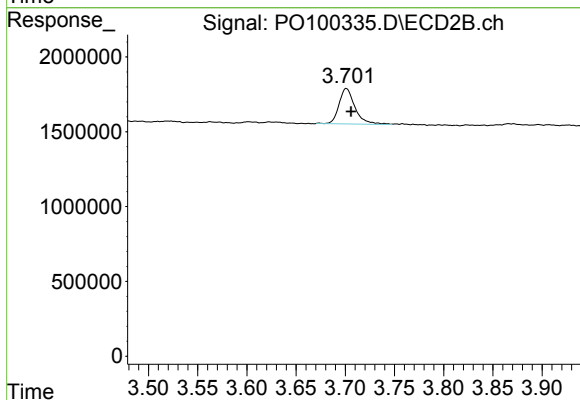


#1 Tetrachloro-m-xylene

R.T.: 3.701 min
Delta R.T.: -0.005 min
Response: 2706705
Conc: 1.80 ng/ml

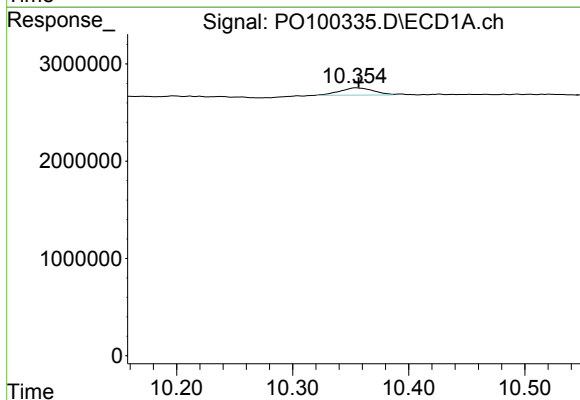

#2 Decachlorobiphenyl

R.T.: 10.354 min
Delta R.T.: -0.003 min
Response: 1500005
Conc: 2.07 ng/ml m

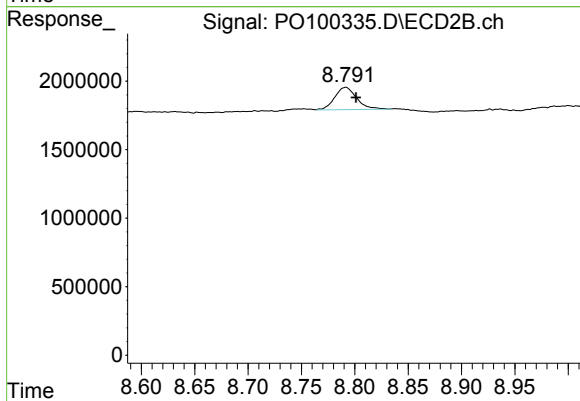

#2 Decachlorobiphenyl

R.T.: 8.791 min
Delta R.T.: -0.010 min
Response: 2337671
Conc: 2.09 ng/ml m