

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120821\
 Data File : PO083487.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Dec 2021 12:16
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 00:32:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 07 13:18:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.943	3.946	1967829	637406	20.626	20.492
2)	SA Decachlor...	11.024	9.248	1493480	680715	20.906	20.866
Target Compounds							
8)	L2 AR-1221-1	5.185	0.000	54579	0	54.275	N.D. #
9)	L2 AR-1221-2	5.298	0.000	24258	0	33.679	N.D. #
10)	L2 AR-1221-3	0.000	4.390	0	24842	N.D.	26.746 #
11)	L3 AR-1232-1	0.000	4.390	0	24842	N.D.	31.427 #
21)	L5 AR-1248-1	0.000	5.160f	0	7579	N.D.	10.403 #
32)	L7 AR-1260-2	8.270f	0.000	18999	0	4.552	N.D. #
35)	L7 AR-1260-5	0.000	7.877	0	6120	N.D.	1.303 #
37)	L8 AR-1262-2	0.000	7.877	0	6120	N.D.	1.305 #
44)	L9 AR-1268-4	0.000	8.698f	0	2995	N.D.	1.737 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120821\
Data File : PO083487.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Dec 2021 12:16
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 00:32:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 07 13:18:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

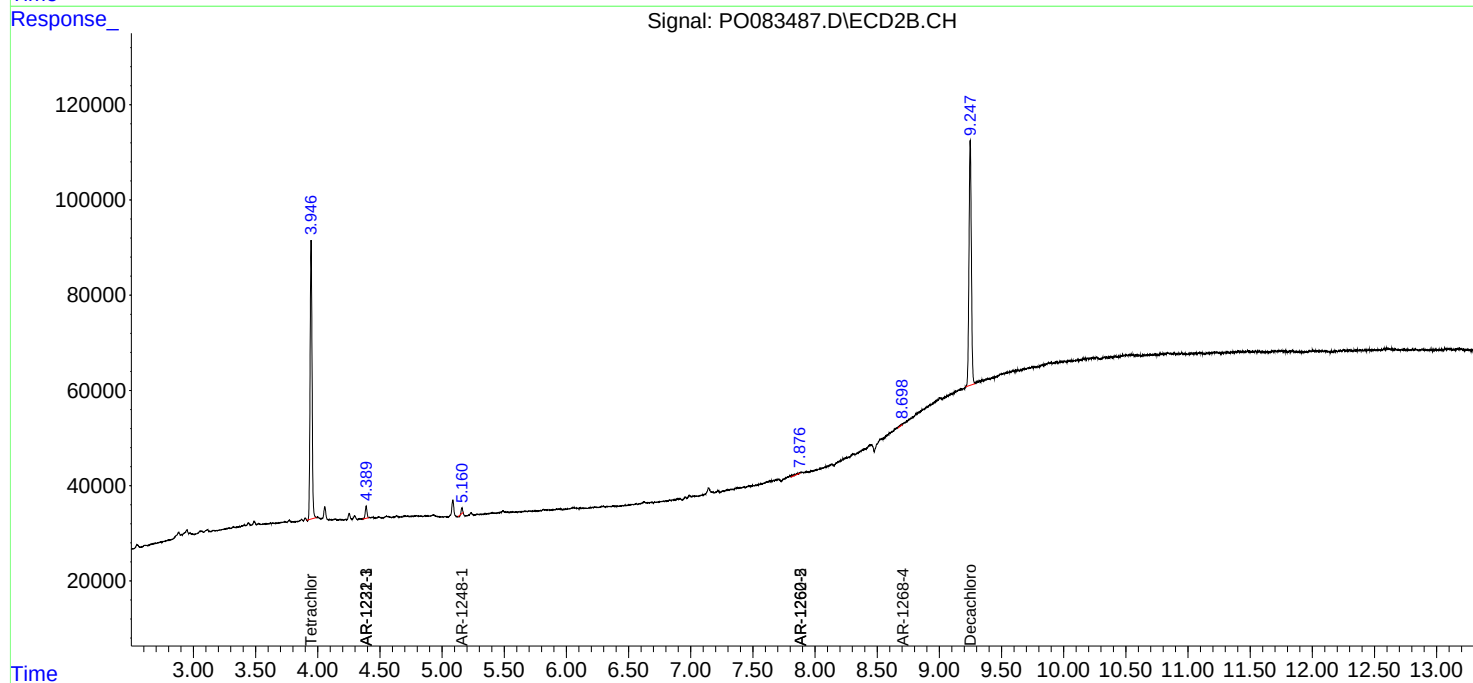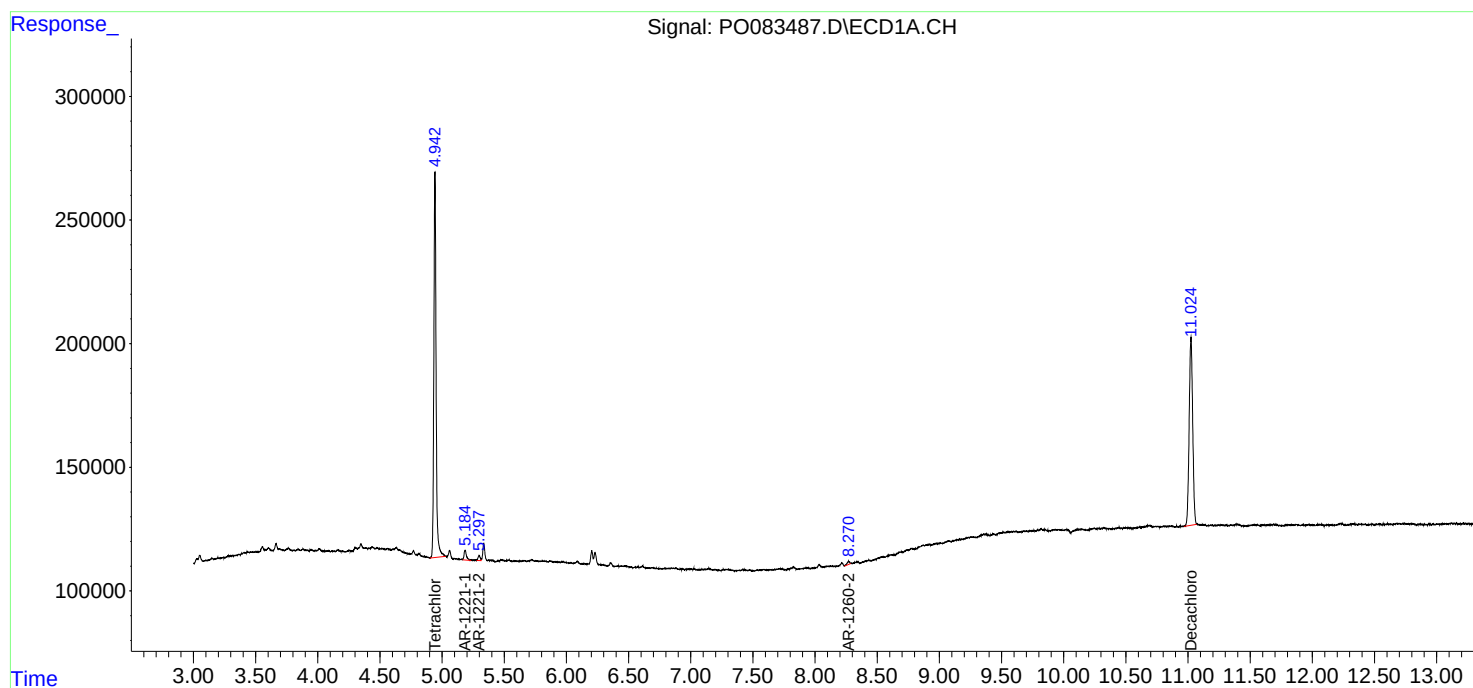


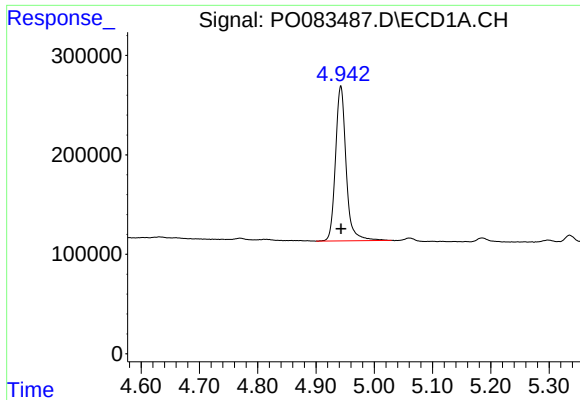

#1 Tetrachloro-m-xylene


R.T.: 4.943 min
Delta R.T.: 0.000 min
Response: 1967829
Conc: 20.63 ng/ml

Instrument :
ECD_O
ClientSampleId :

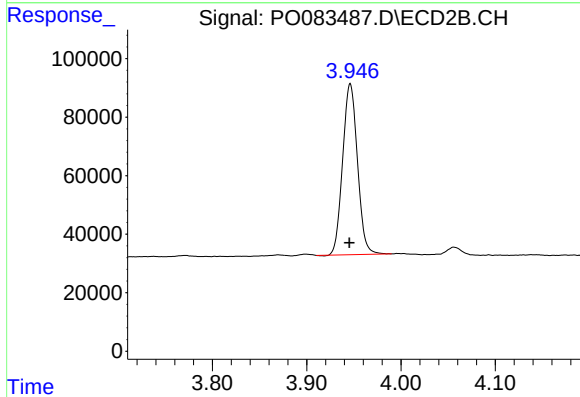


#1 Tetrachloro-m-xylene

R.T.: 3.946 min
Delta R.T.: 0.000 min
Response: 637406
Conc: 20.49 ng/ml

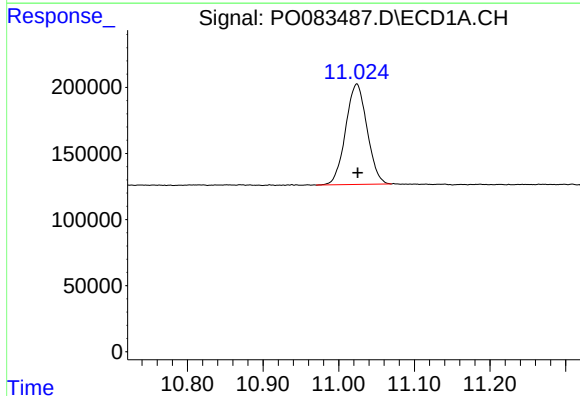


#2 Decachlorobiphenyl

R.T.: 11.024 min
Delta R.T.: -0.001 min
Response: 1493480
Conc: 20.91 ng/ml

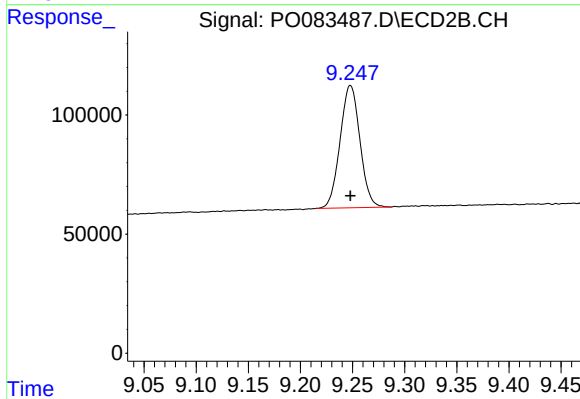

#2 Decachlorobiphenyl


R.T.: 9.248 min
Delta R.T.: 0.000 min
Response: 680715
Conc: 20.87 ng/ml

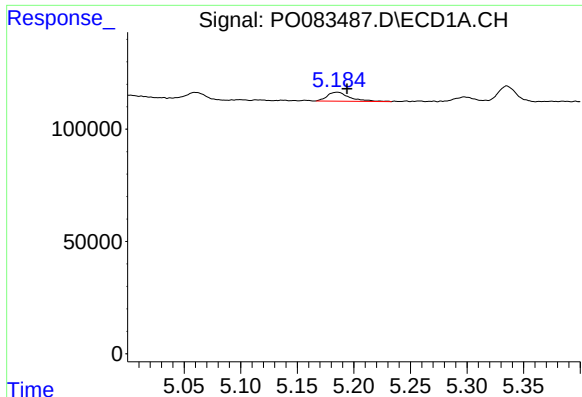

#8 AR-1221-1


R.T.: 5.185 min
Delta R.T.: -0.009 min
Response: 54579
Conc: 54.27 ng/ml

Instrument :
ECD_O
ClientSampleId :

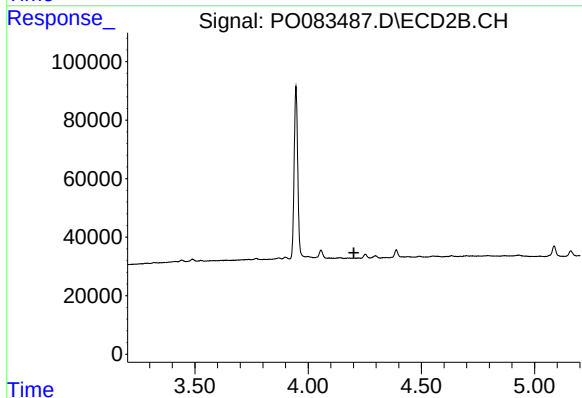


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.202 min
Response: 0
Conc: N.D.

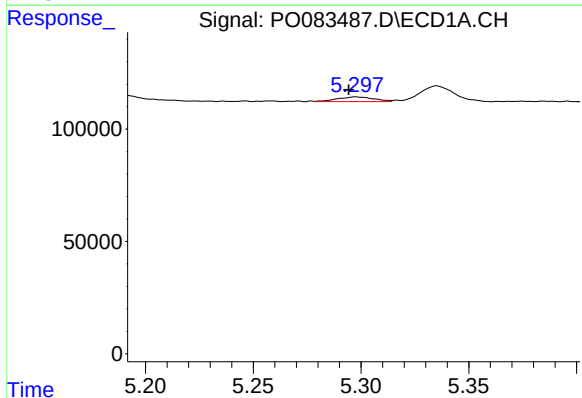


#9 AR-1221-2

R.T.: 5.298 min
Delta R.T.: 0.003 min
Response: 24258
Conc: 33.68 ng/ml

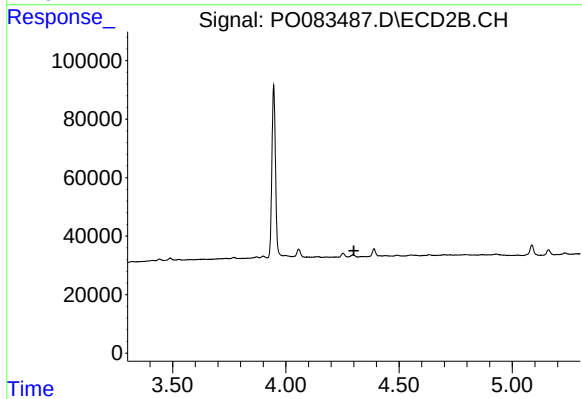

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.301 min
Response: 0
Conc: N.D.

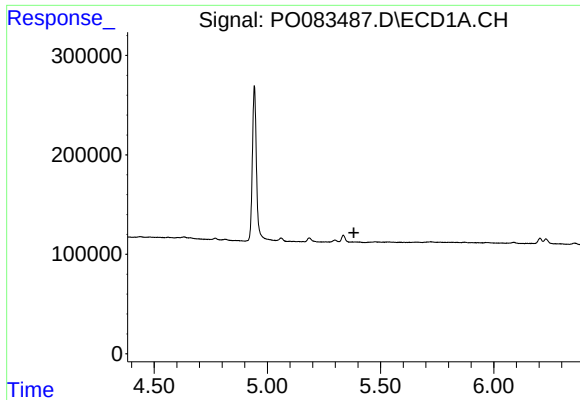

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 5.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

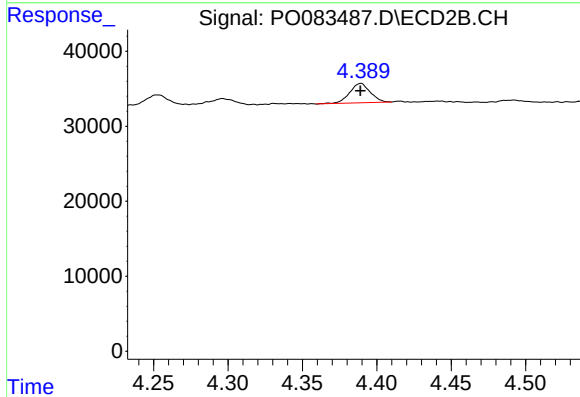


#10 AR-1221-3

R.T.: 4.390 min
Delta R.T.: 0.000 min
Response: 24842
Conc: 26.75 ng/ml

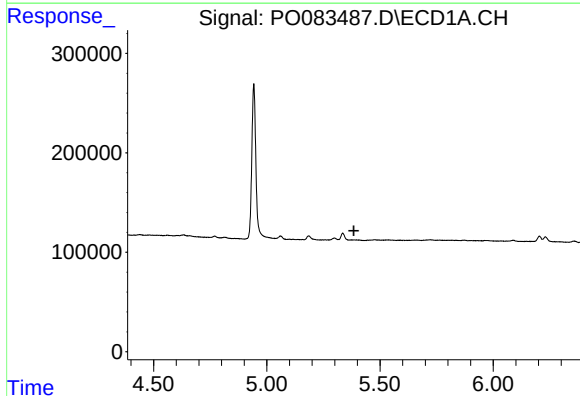


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 5.384 min
Response: 0
Conc: N.D.

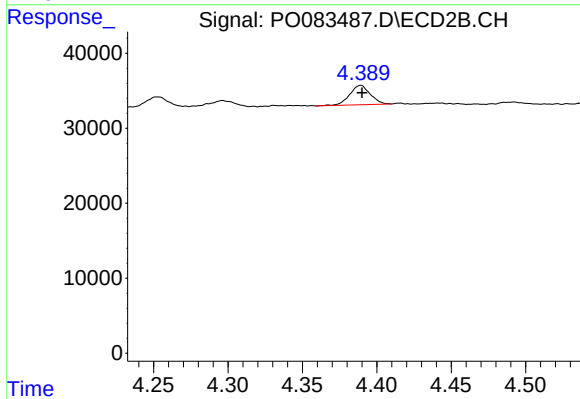

#11 AR-1232-1


R.T.: 4.390 min
Delta R.T.: 0.000 min
Response: 24842
Conc: 31.43 ng/ml

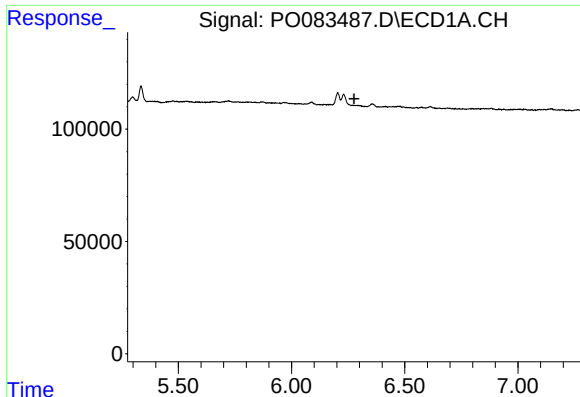

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 6.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

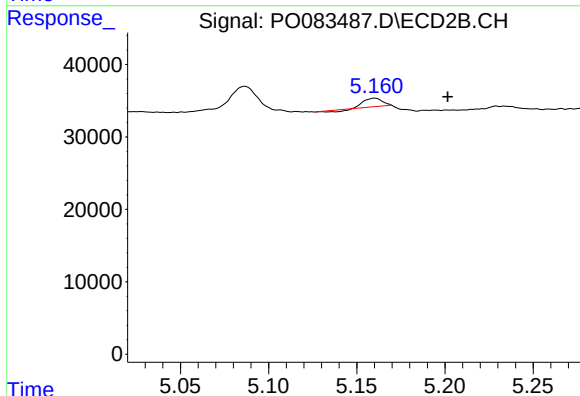


#21 AR-1248-1

R.T.: 5.160 min
Delta R.T.: -0.041 min
Response: 7579
Conc: 10.40 ng/ml

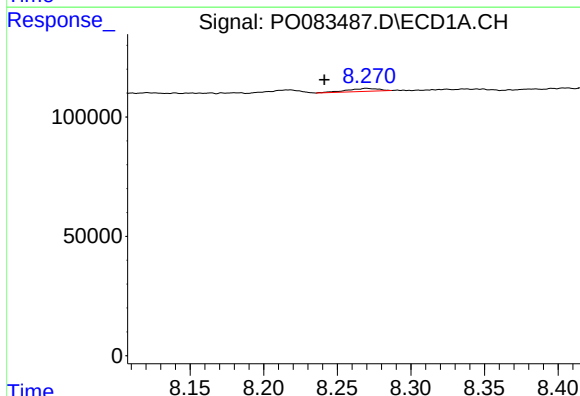


#32 AR-1260-2

R.T.: 8.270 min
Delta R.T.: 0.029 min
Response: 18999
Conc: 4.55 ng/ml

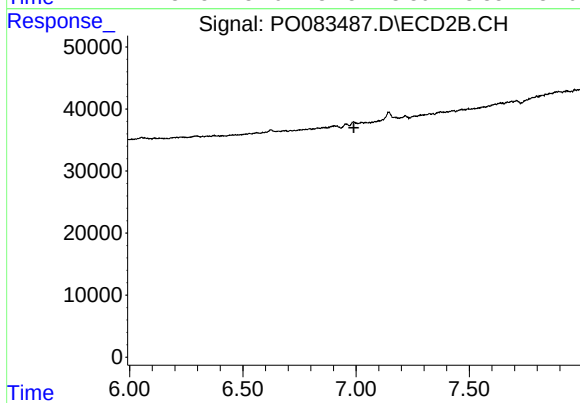

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 6.990 min
Response: 0
Conc: N.D.

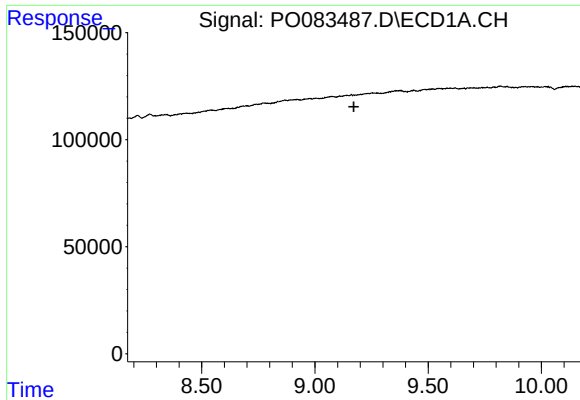

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

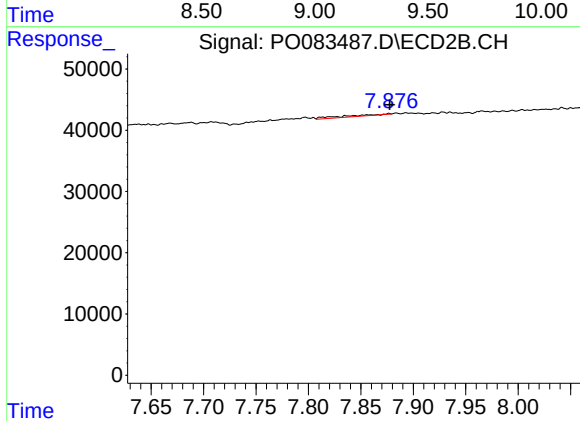


#35 AR-1260-5

R.T.: 7.877 min
Delta R.T.: 0.000 min
Response: 6120
Conc: 1.30 ng/ml

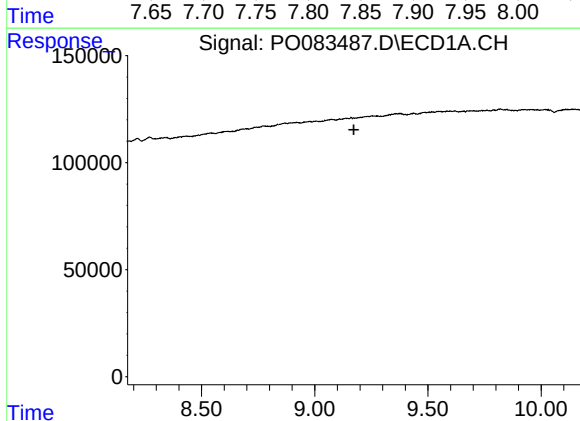


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 9.173 min
Response: 0
Conc: N.D.

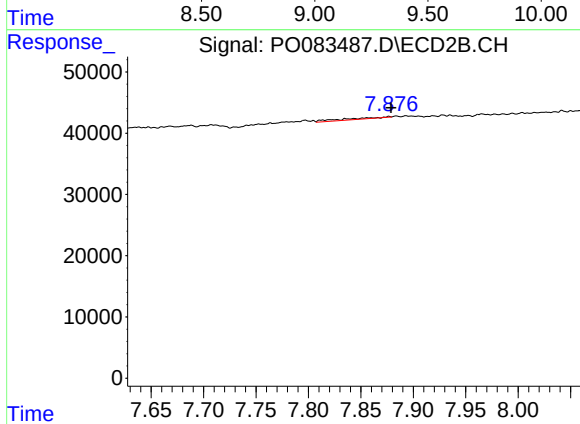

#37 AR-1262-2


R.T.: 7.877 min
Delta R.T.: -0.002 min
Response: 6120
Conc: 1.31 ng/ml

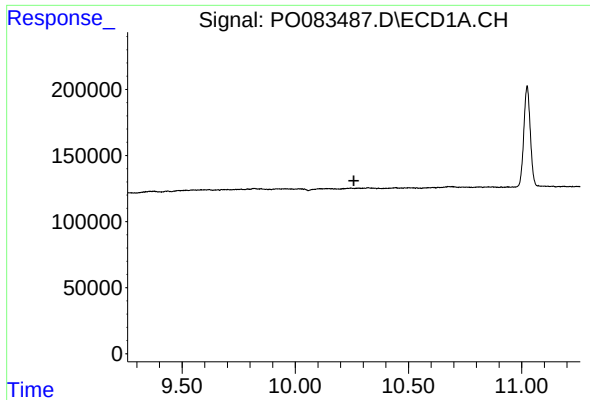

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 10.259 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

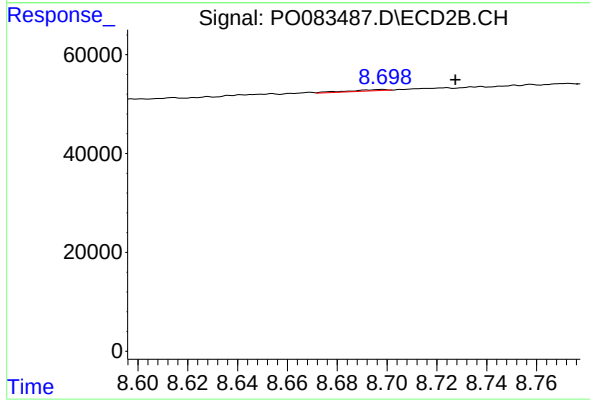

#44 AR-1268-4

R.T.: 8.698 min
Delta R.T.: -0.029 min
Response: 2995
Conc: 1.74 ng/ml