

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120821\
 Data File : PO083492.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Dec 2021 16:55
 Operator : AJ\MA
 Sample : M4953-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 00:34:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 07 13:18:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.942	3.946	1888981	639884	19.800	20.571
2) SA Decachlor...	11.029	9.249	233875	110204	3.274	3.378
Target Compounds						
8) L2 AR-1221-1	5.200	0.000	39481	0	39.261	N.D. #
20) L4 AR-1242-5	7.269	0.000	24800	0	14.222	N.D. #
25) L5 AR-1248-5	7.269	0.000	24800	0	8.669	N.D. #
29) L6 AR-1254-4	8.097	0.000	4400	0	1.234	N.D. #
30) L6 AR-1254-5	8.533	0.000	8276	0	2.307	N.D. #
33) L7 AR-1260-3	8.615	0.000	19838	0	6.328	N.D. #
34) L7 AR-1260-4	8.860f	0.000	23326	0	6.662	N.D. #
36) L8 AR-1262-1	8.615	0.000	19838	0	4.775	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120821\
Data File : PO083492.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Dec 2021 16:55
Operator : AJ\MA
Sample : M4953-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 00:34:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 07 13:18:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

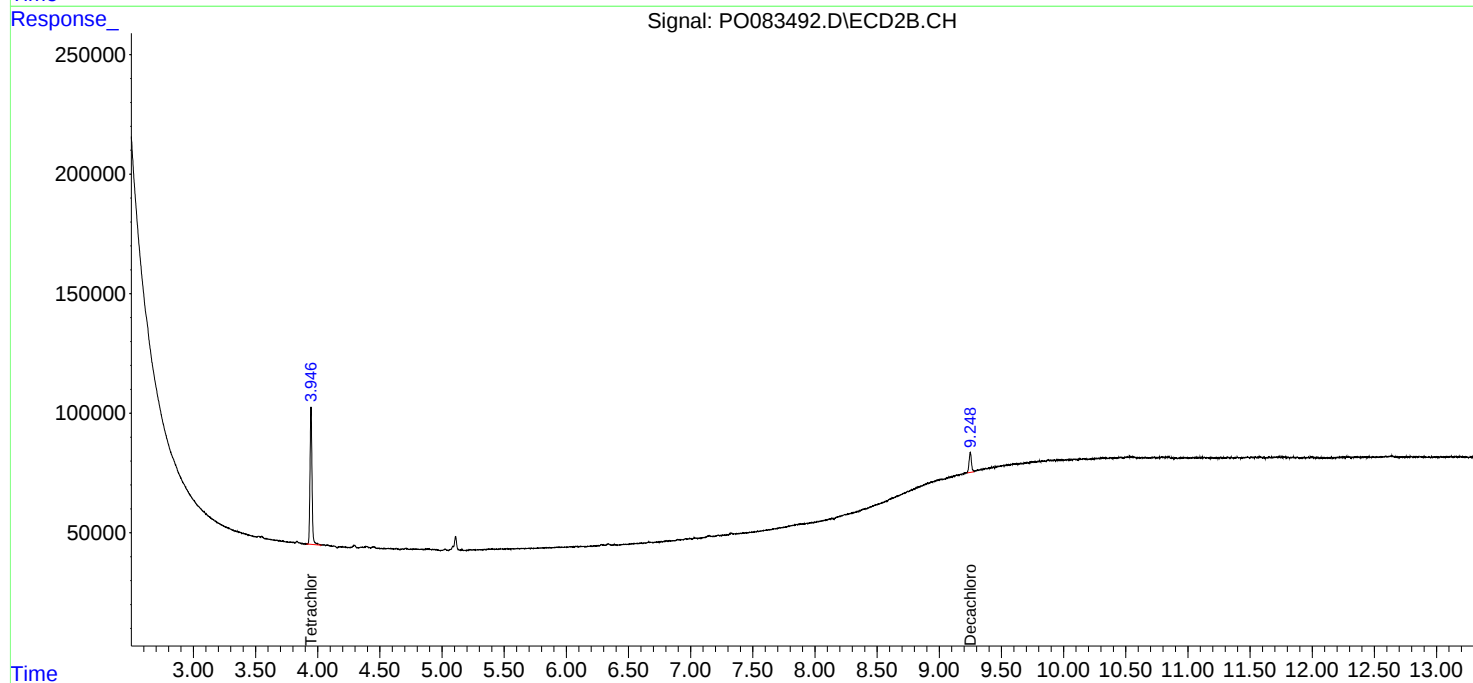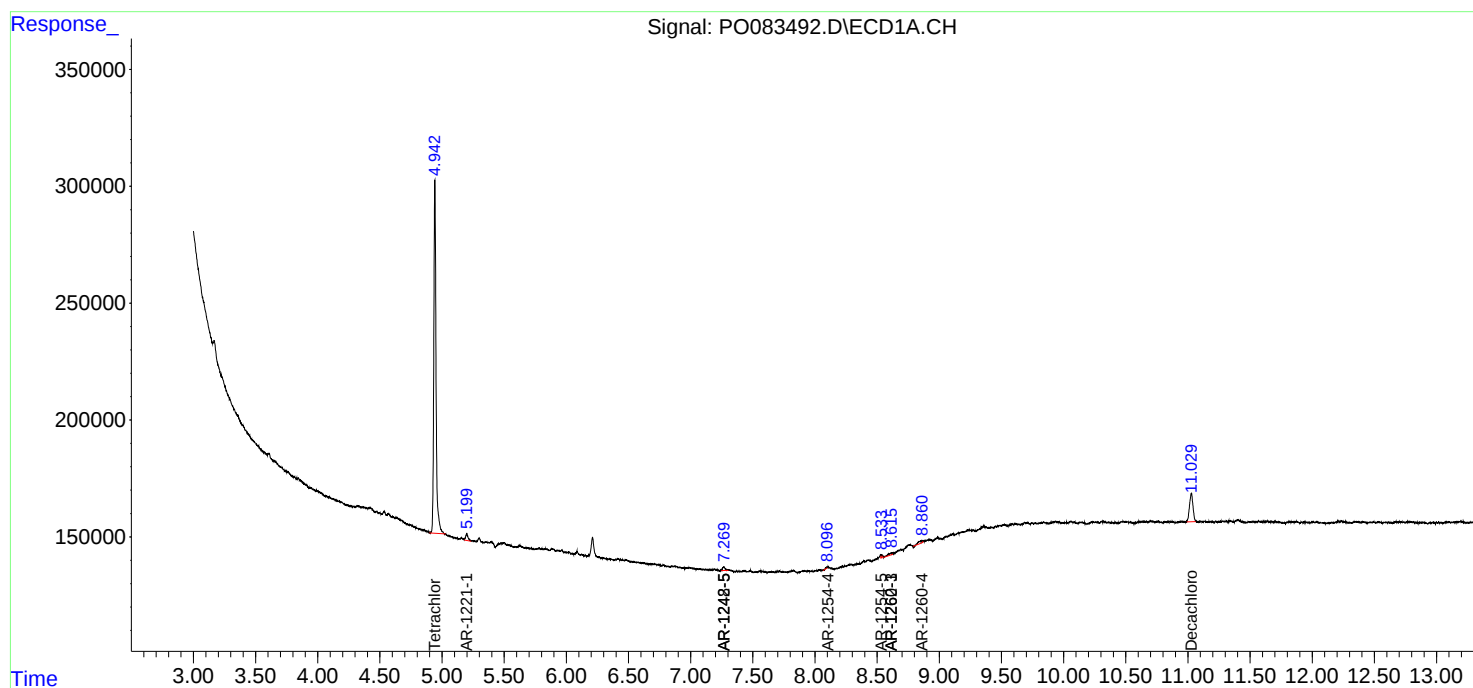


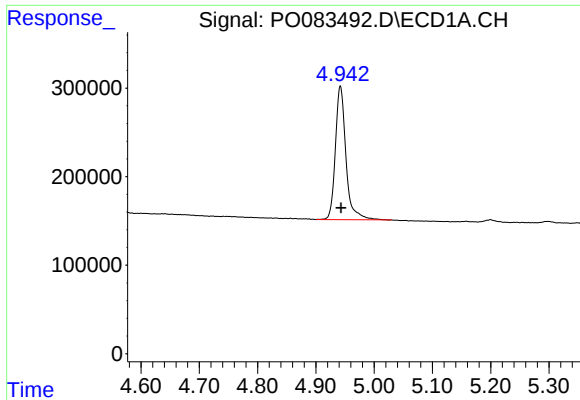

#1 Tetrachloro-m-xylene


R.T.: 4.942 min
Delta R.T.: 0.000 min
Response: 1888981
Conc: 19.80 ng/ml

Instrument :
ECD_O
ClientSampleId :

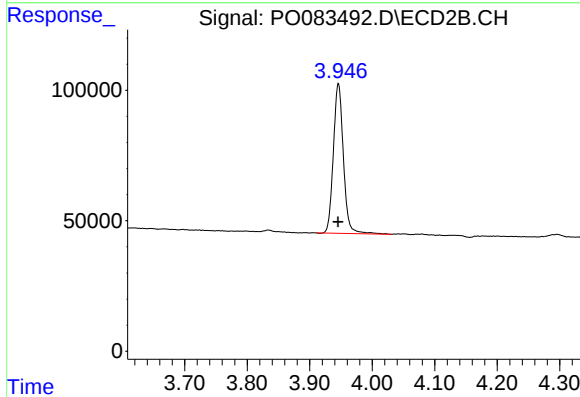


#1 Tetrachloro-m-xylene

R.T.: 3.946 min
Delta R.T.: 0.000 min
Response: 639884
Conc: 20.57 ng/ml

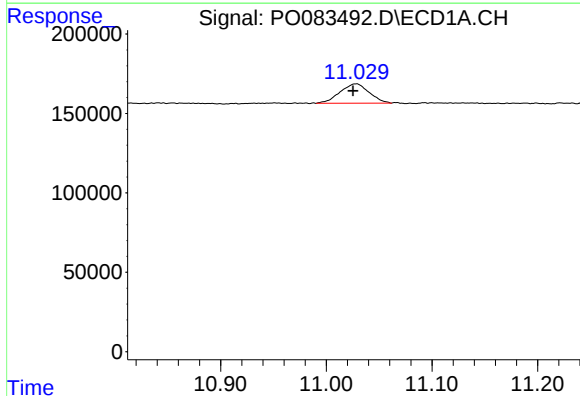


#2 Decachlorobiphenyl

R.T.: 11.029 min
Delta R.T.: 0.003 min
Response: 233875
Conc: 3.27 ng/ml

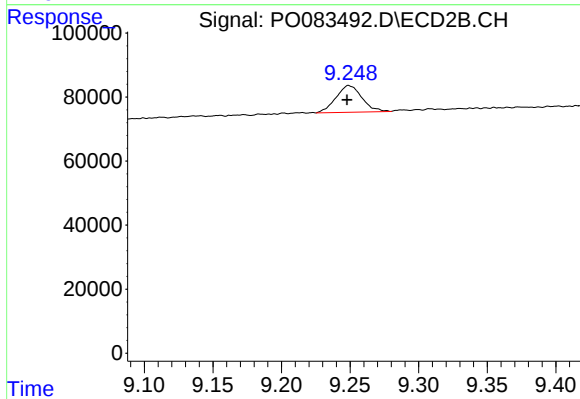

#2 Decachlorobiphenyl


R.T.: 9.249 min
Delta R.T.: 0.001 min
Response: 110204
Conc: 3.38 ng/ml

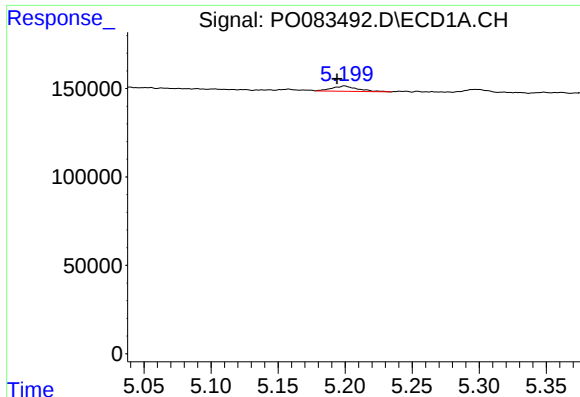

#8 AR-1221-1


R.T.: 5.200 min
Delta R.T.: 0.006 min
Response: 39481
Conc: 39.26 ng/ml

Instrument :
ECD_O
ClientSampleId :

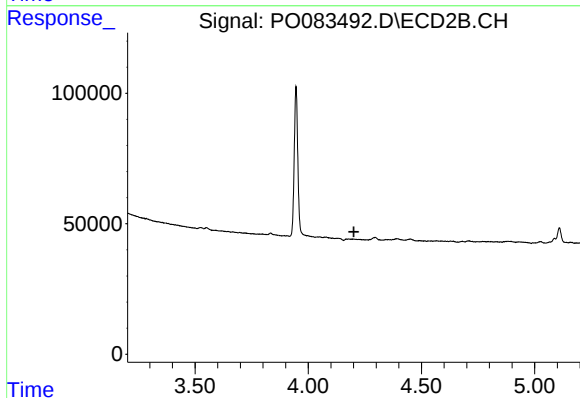


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.202 min
Response: 0
Conc: N.D.

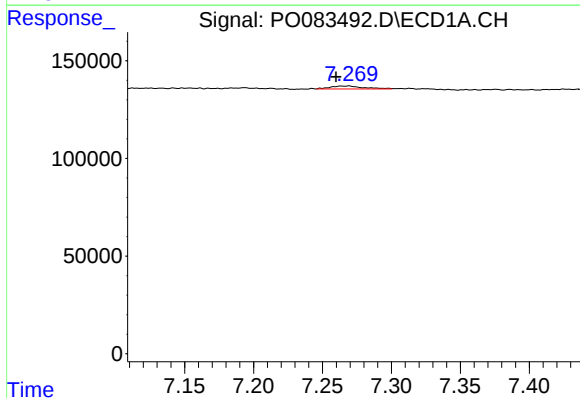


#20 AR-1242-5

R.T.: 7.269 min
Delta R.T.: 0.010 min
Response: 24800
Conc: 14.22 ng/ml

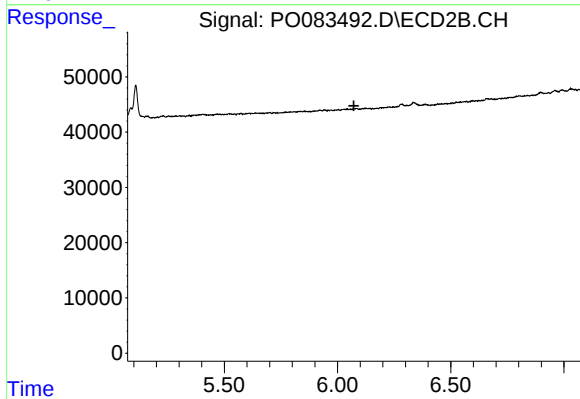

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 6.073 min
Response: 0
Conc: N.D.

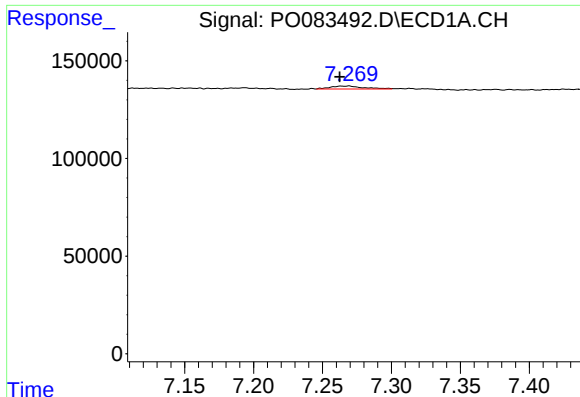

#25 AR-1248-5


R.T.: 7.269 min
Delta R.T.: 0.007 min
Response: 24800
Conc: 8.67 ng/ml

Instrument :
ECD_O
ClientSampleId :

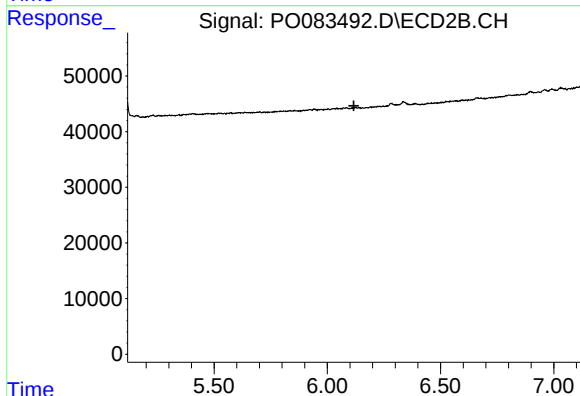


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.117 min
Response: 0
Conc: N.D.

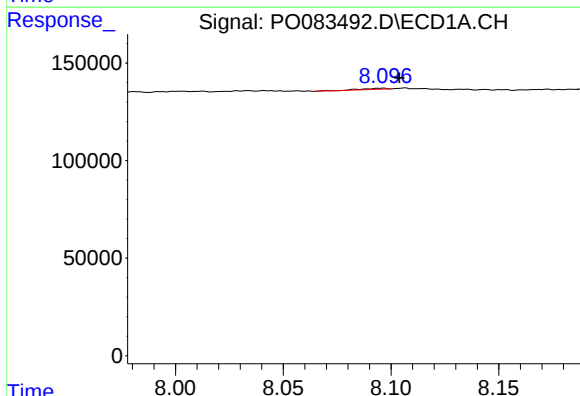


#29 AR-1254-4

R.T.: 8.097 min
Delta R.T.: -0.007 min
Response: 4400
Conc: 1.23 ng/ml

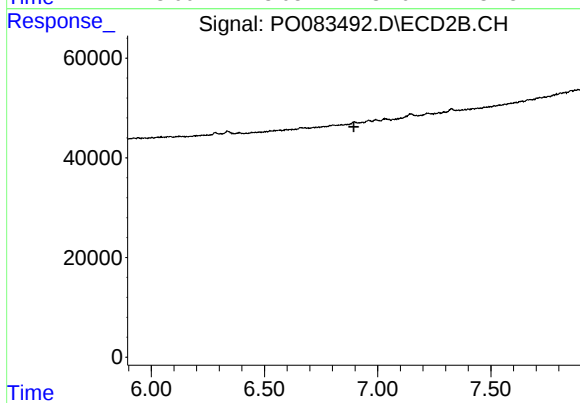

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.895 min
Response: 0
Conc: N.D.

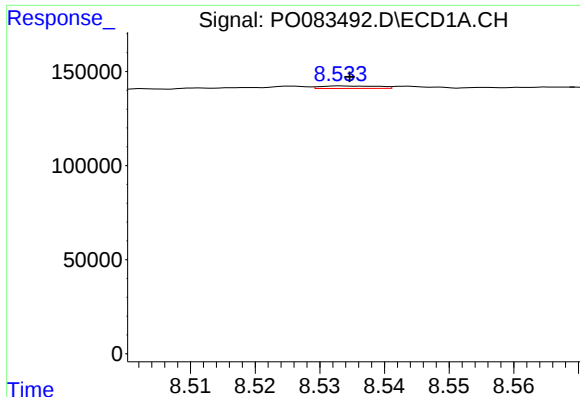

#30 AR-1254-5


R.T.: 8.533 min
Delta R.T.: -0.001 min
Response: 8276
Conc: 2.31 ng/ml

Instrument :
ECD_O
ClientSampleId :

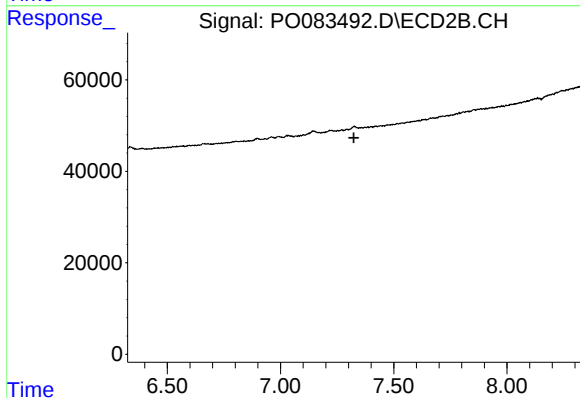


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.324 min
Response: 0
Conc: N.D.

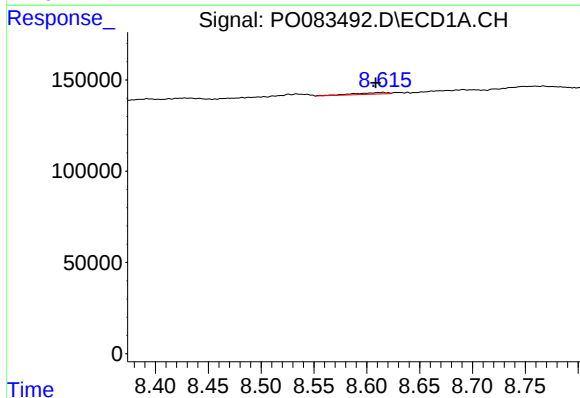


#33 AR-1260-3

R.T.: 8.615 min
Delta R.T.: 0.007 min
Response: 19838
Conc: 6.33 ng/ml

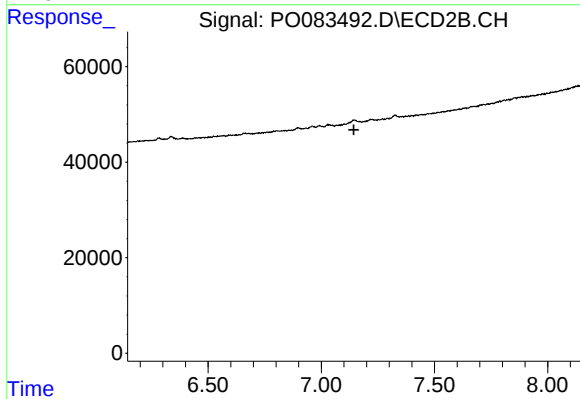

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.144 min
Response: 0
Conc: N.D.

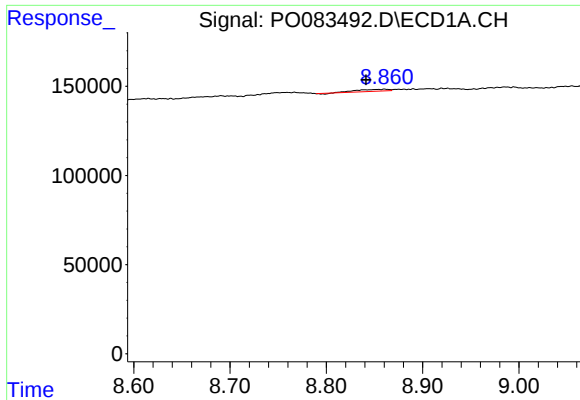

#34 AR-1260-4


R.T.: 8.860 min
Delta R.T.: 0.019 min
Response: 23326
Conc: 6.66 ng/ml

Instrument :
ECD_O
ClientSampleId :

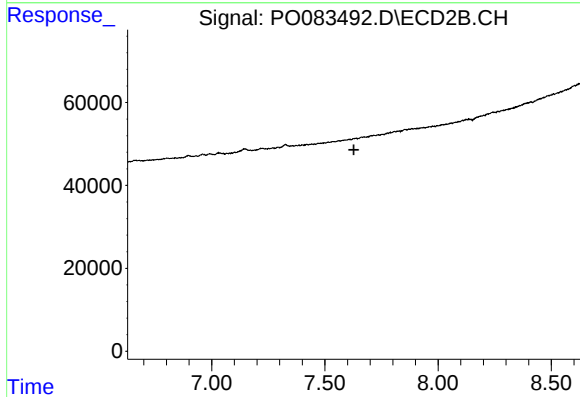


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.628 min
Response: 0
Conc: N.D.

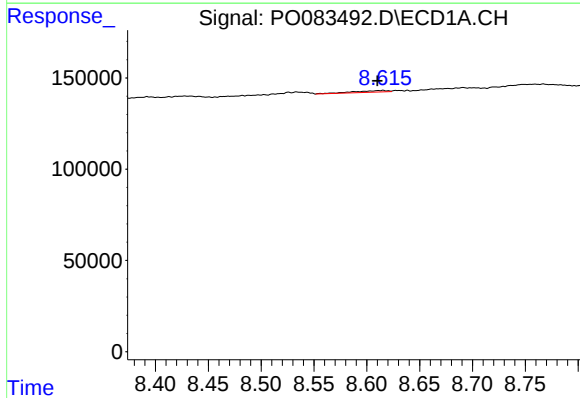

#36 AR-1262-1

R.T.: 8.615 min
Delta R.T.: 0.005 min
Response: 19838
Conc: 4.78 ng/ml

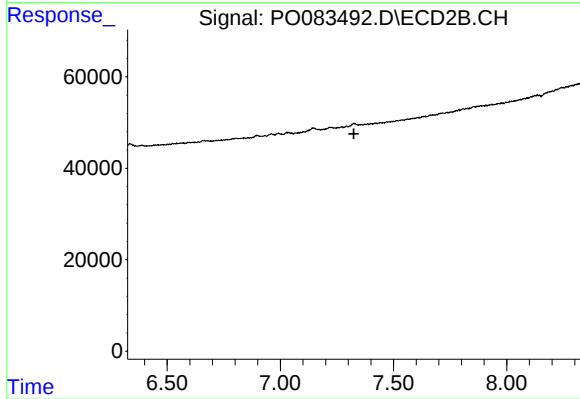

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.324 min
Response: 0
Conc: N.D.