

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120821\
Data File : PO083491.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Dec 2021 16:37
Operator : AJ\MA
Sample : M4953-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
A377

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 00:34:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 07 13:18:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.945	3.949	1711080	575127	17.935	18.489
2) SA Decachlor...	11.030	9.252	178862	81975	2.504	2.513

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120821\
Data File : PO083491.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Dec 2021 16:37
Operator : AJ\MA
Sample : M4953-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
A377

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 00:34:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 07 13:18:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

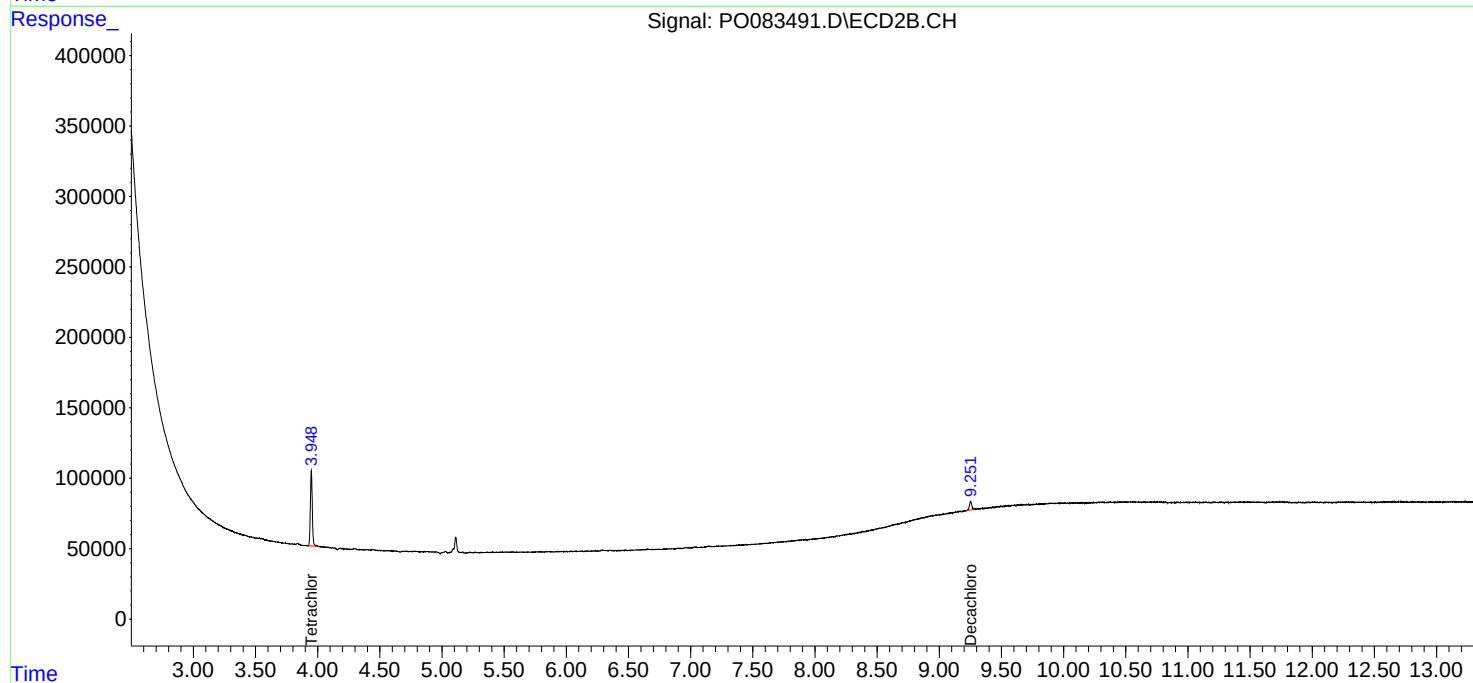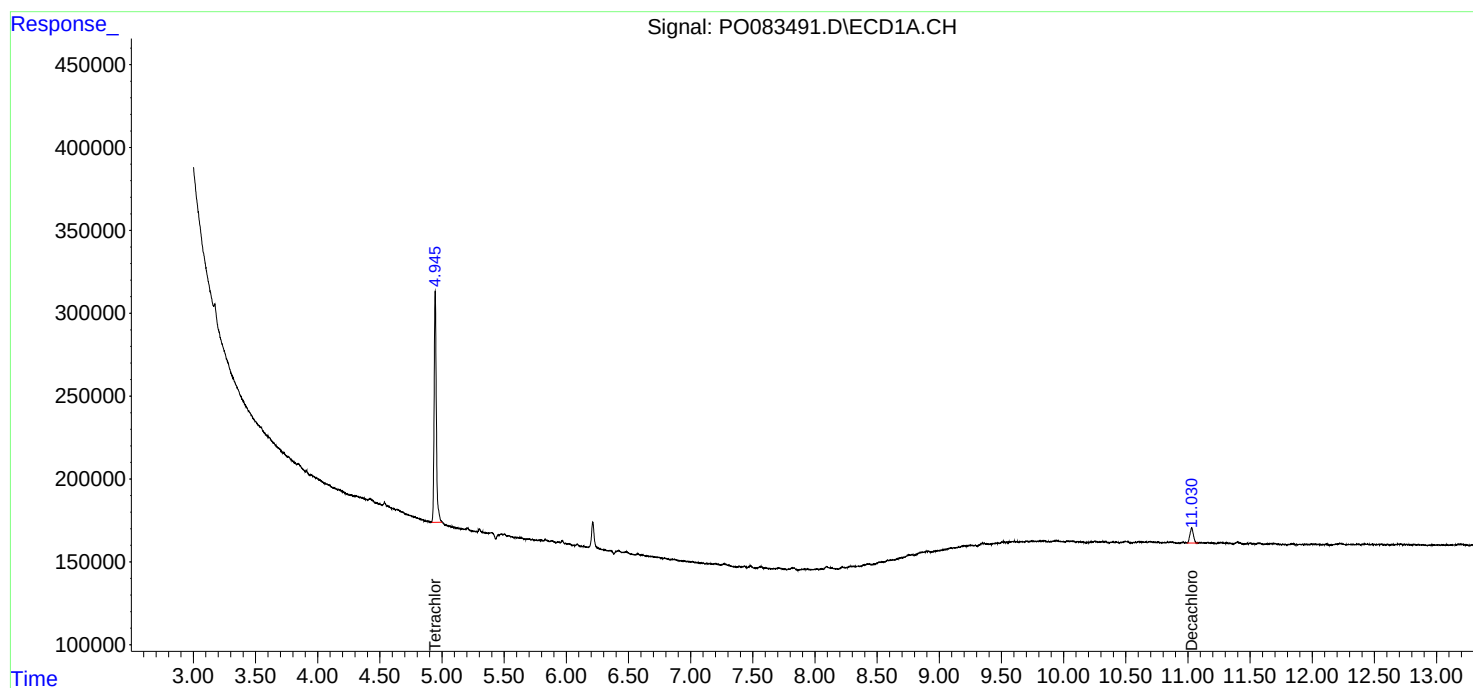


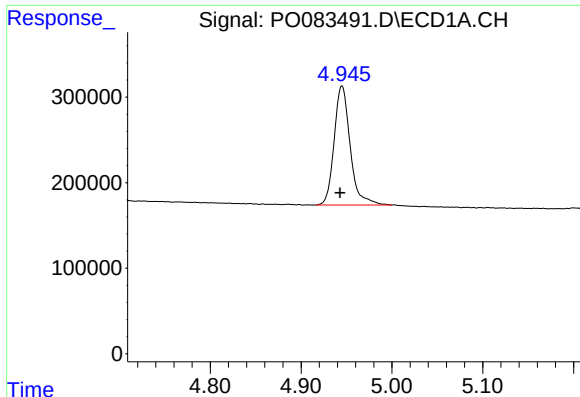

#1 Tetrachloro-m-xylene


R.T.: 4.945 min
Delta R.T.: 0.002 min
Response: 1711080
Conc: 17.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
A377

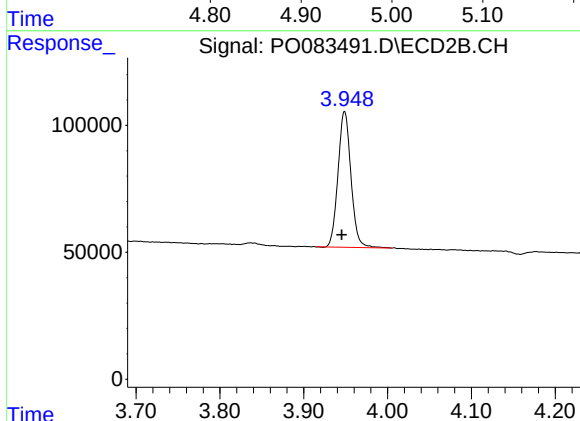


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: 0.003 min
Response: 575127
Conc: 18.49 ng/ml

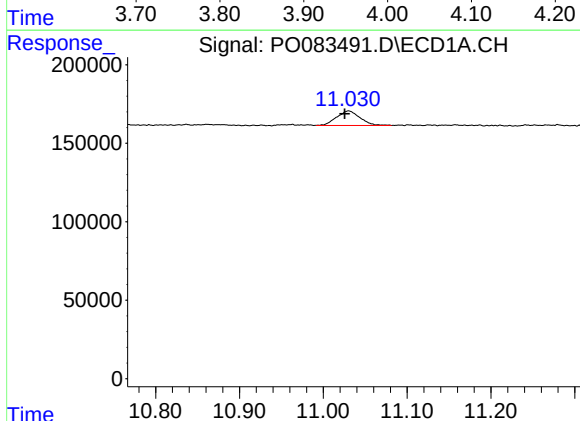

#2 Decachlorobiphenyl

R.T.: 11.030 min
Delta R.T.: 0.005 min
Response: 178862
Conc: 2.50 ng/ml

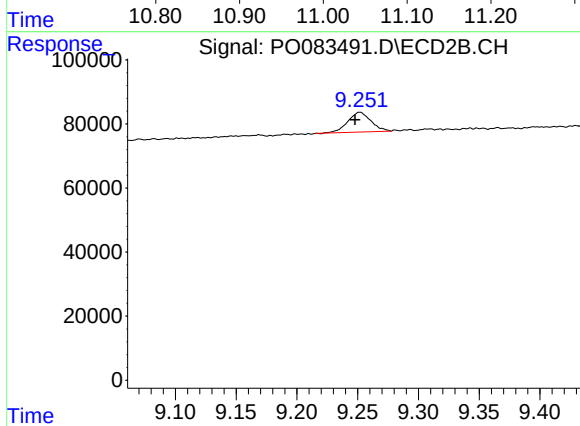

#2 Decachlorobiphenyl

R.T.: 9.252 min
Delta R.T.: 0.004 min
Response: 81975
Conc: 2.51 ng/ml