

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120822\
 Data File : PO091193.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Dec 2022 16:23
 Operator : YP/AJ
 Sample : N5943-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RM-301

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/09/2022
 Supervised By :Ankita Jodhani 12/09/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 08 23:32:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 28 11:25:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.298	3.475	68436713	23195560	20.241	22.100
2) SA Decachlor...	10.046	8.478	48528501	19021179	18.270	19.592

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120822\
Data File : PO091193.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Dec 2022 16:23
Operator : YP/AJ
Sample : N5943-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RM-301


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/09/2022
Supervised By :Ankita Jodhani 12/09/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 08 23:32:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112522.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 28 11:25:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

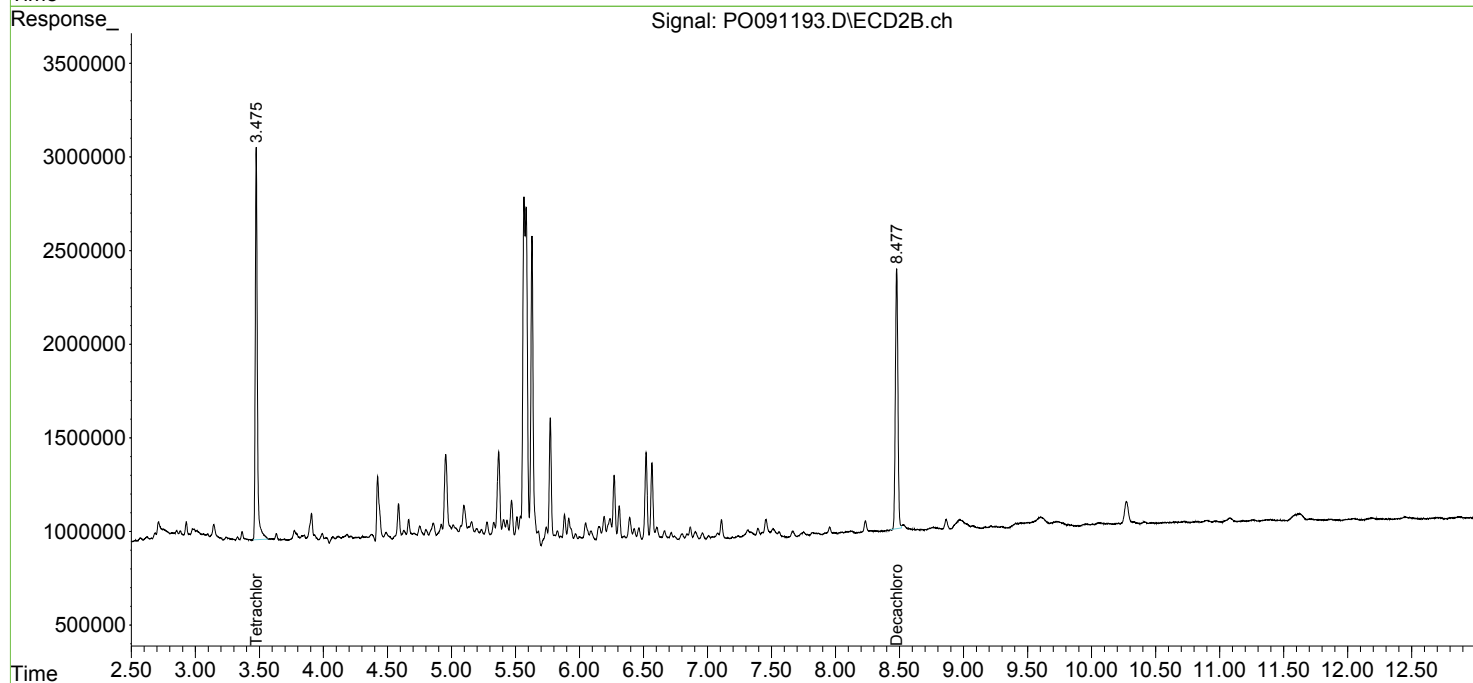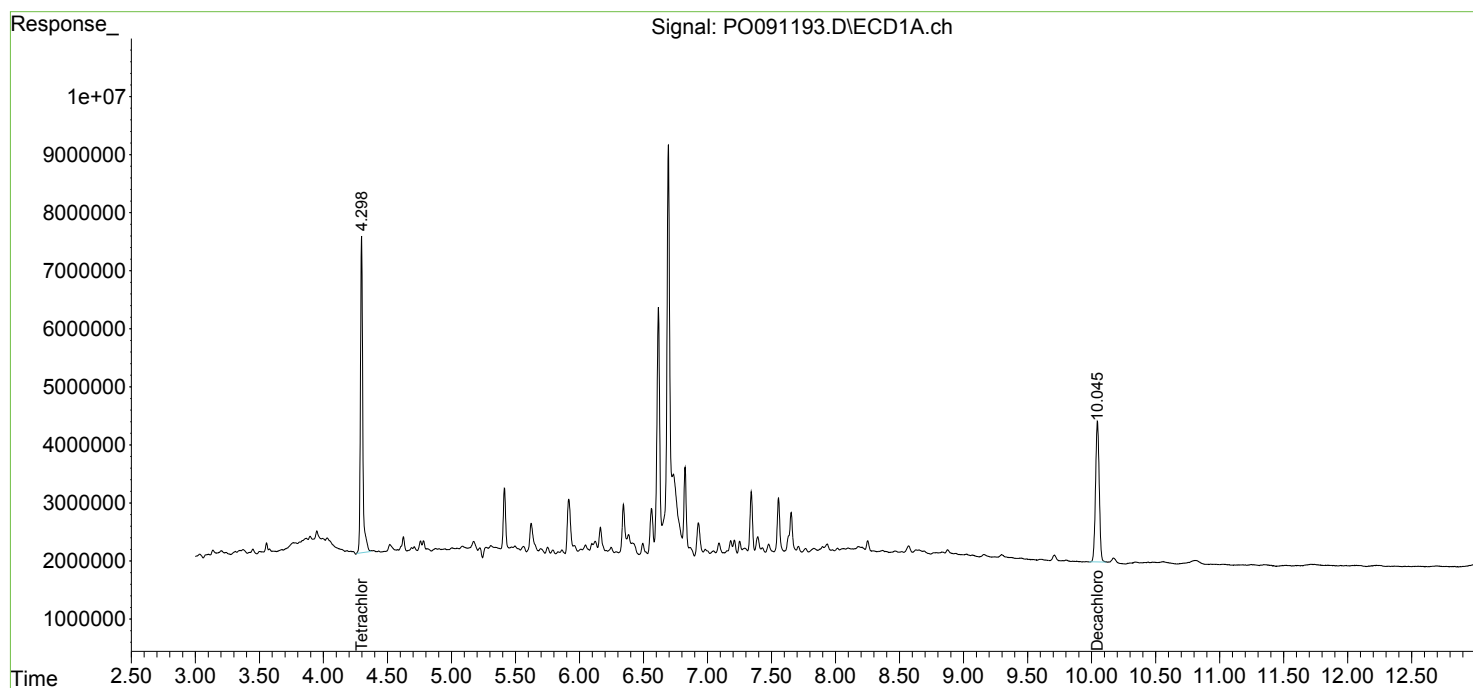

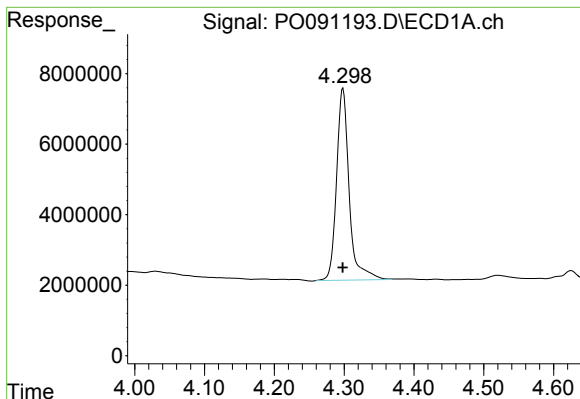


#1 Tetrachloro-m-xylene

R.T.: 4.298 min
Delta R.T.: 0.000 min
Response: 68436713
Conc: 20.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
RM-301


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/09/2022
Supervised By :Ankita Jodhani 12/09/2022

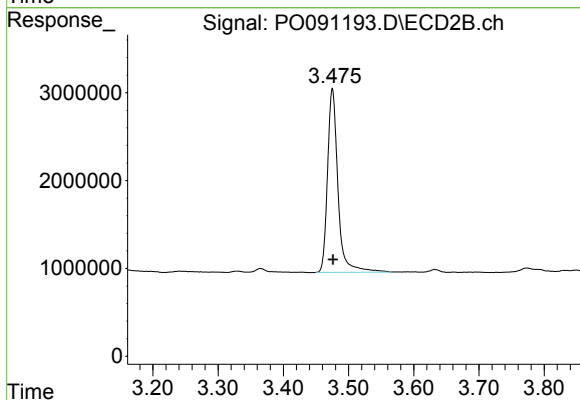


#1 Tetrachloro-m-xylene

R.T.: 3.475 min
Delta R.T.: 0.000 min
Response: 23195560
Conc: 22.10 ng/ml

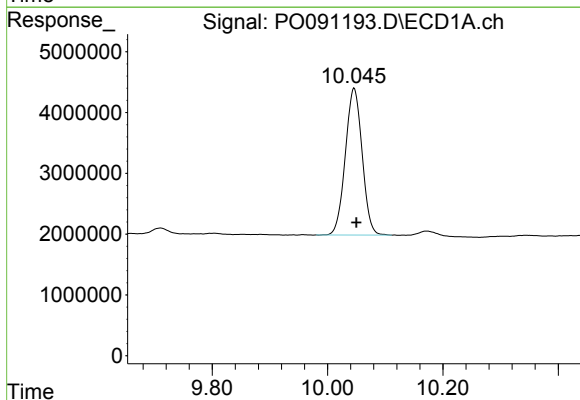

#2 Decachlorobiphenyl

R.T.: 10.046 min
Delta R.T.: -0.004 min
Response: 48528501
Conc: 18.27 ng/ml

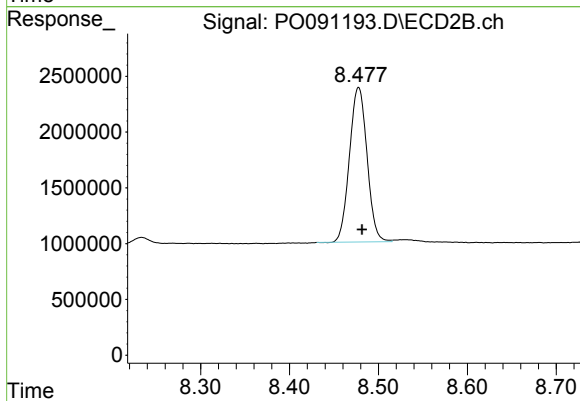

#2 Decachlorobiphenyl

R.T.: 8.478 min
Delta R.T.: -0.004 min
Response: 19021179
Conc: 19.59 ng/ml