

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120822\
 Data File : PO091204.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Dec 2022 19:59
 Operator : YP/AJ
 Sample : N5910-02 (Sig #1); N3910-02 (Sig #2)
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 02-A-02-B-02-C

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/09/2022
 Supervised By :Ankita Jodhani 12/09/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 08 23:38:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 28 11:25:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.297	3.474	73093670	24003016	21.618	22.870
2) SA Decachlor...	10.044	8.476	48412482	20266048	18.226	20.874

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120822\
Data File : PO091204.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Dec 2022 19:59
Operator : YP/AJ
Sample : N5910-02 (Sig #1); N3910-02 (Sig #2)
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
02-A-02-B-02-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/09/2022
Supervised By :Ankita Jodhani 12/09/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 08 23:38:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112522.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 28 11:25:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

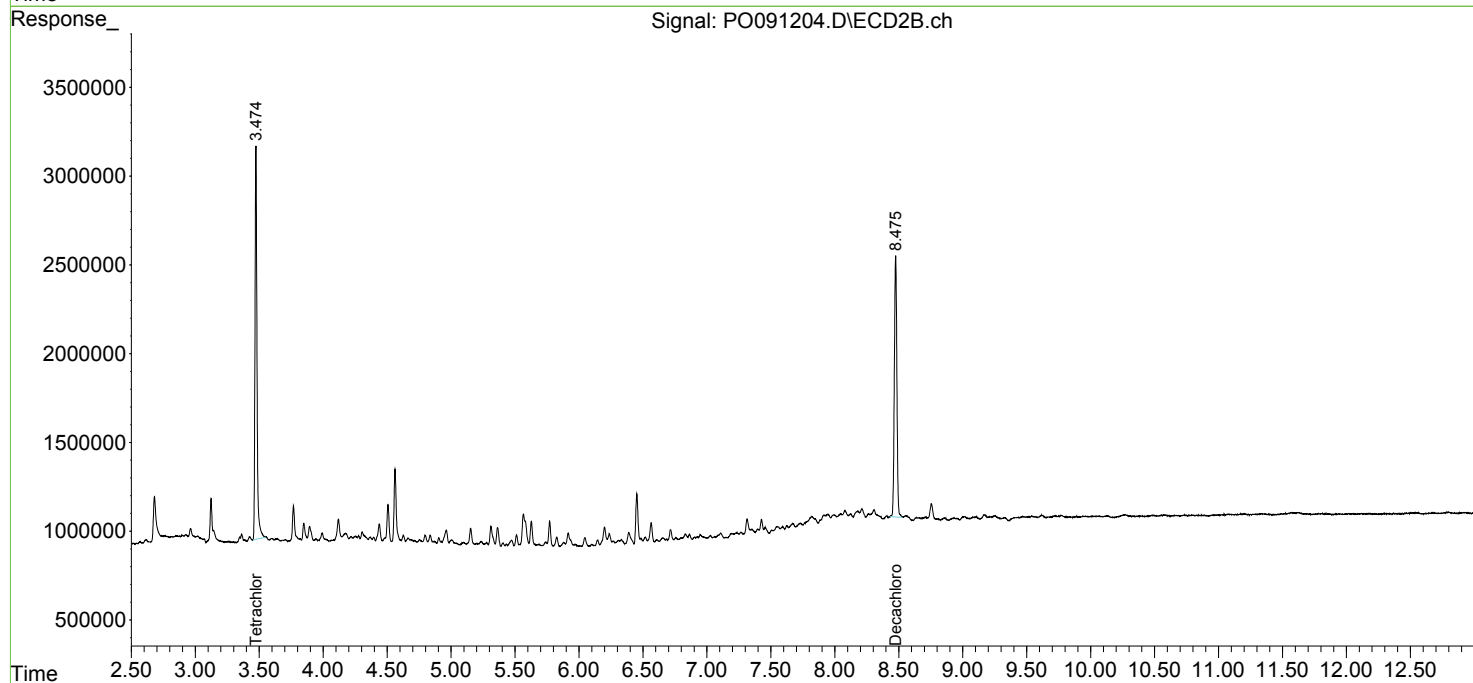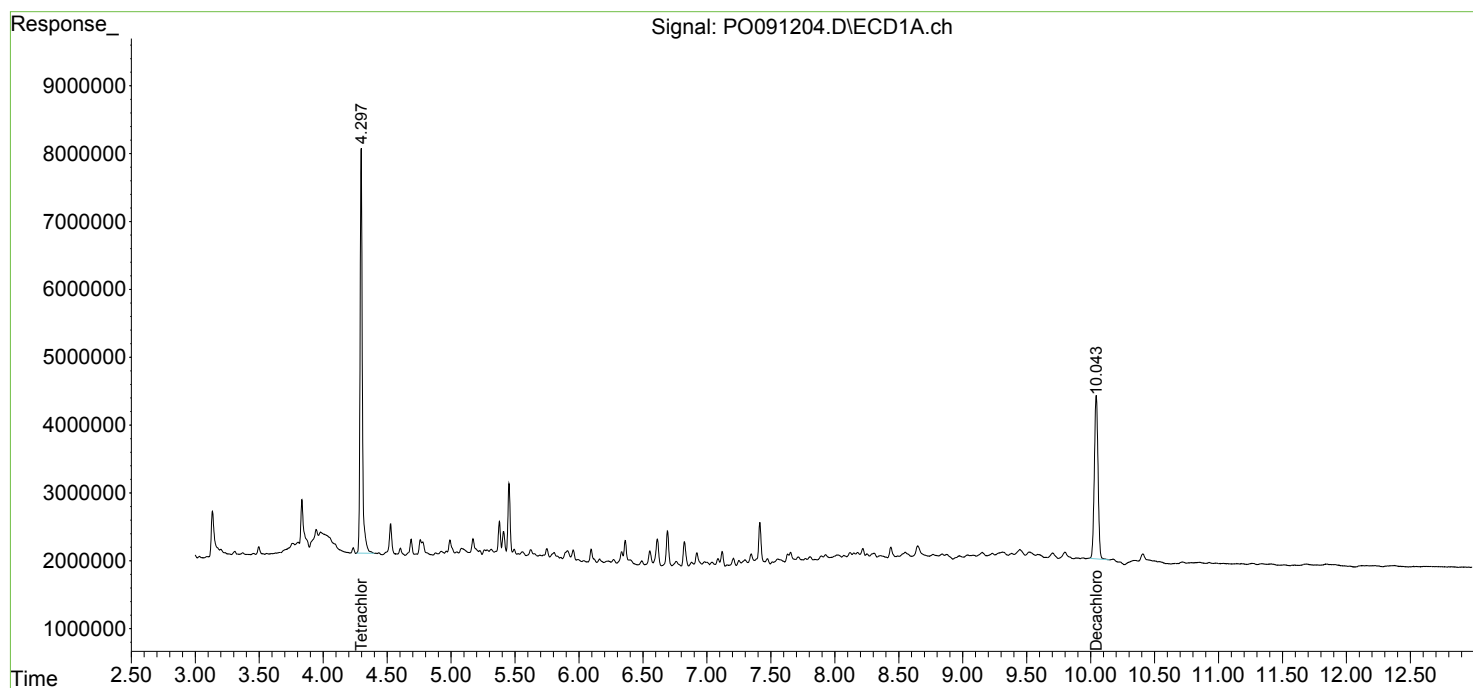

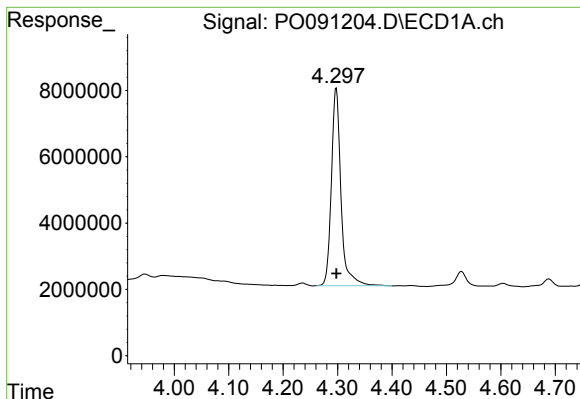

#1 Tetrachloro-m-xylene

R.T.: 4.297 min
Delta R.T.: 0.000 min
Response: 73093670
Conc: 21.62 ng/ml

Instrument :

ECD_O


ClientSampleId :

02-A-02-B-02-C

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 12/09/2022
Supervised By :Ankita Jodhani 12/09/2022

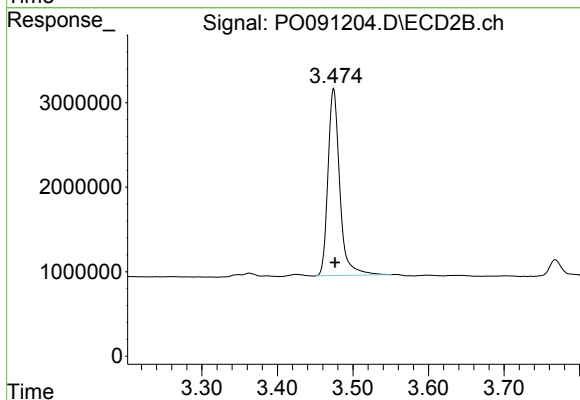


#1 Tetrachloro-m-xylene

R.T.: 3.474 min
Delta R.T.: -0.002 min
Response: 24003016
Conc: 22.87 ng/ml

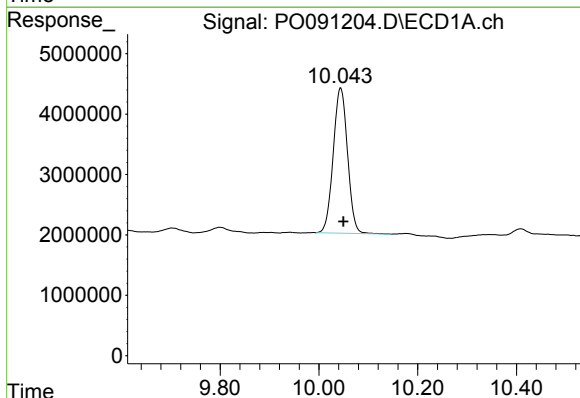

#2 Decachlorobiphenyl

R.T.: 10.044 min
Delta R.T.: -0.006 min
Response: 48412482
Conc: 18.23 ng/ml

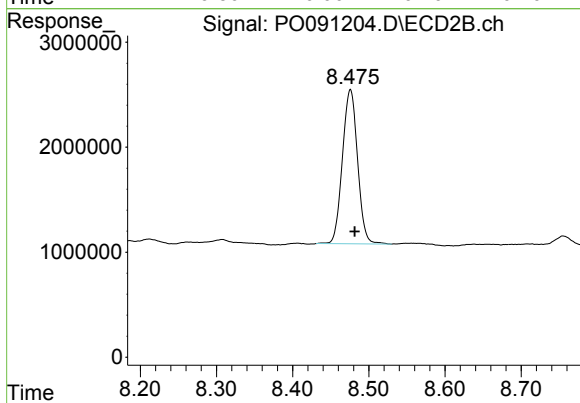

#2 Decachlorobiphenyl

R.T.: 8.476 min
Delta R.T.: -0.006 min
Response: 20266048
Conc: 20.87 ng/ml