

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120919\
 Data File : P0064473.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Dec 2019 13:21
 Operator : SM/AJ
 Sample : PB125311BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB125311BL

Manual Integrations
 APPROVED

Ankita
 12/10/2019 10:09:21 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 13:37:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 28 01:28:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.311	3.560	530919	476301	17.927m	20.025
2) SA Decachlor...	9.934	8.517	721709	743238	17.610	18.194

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120919\
Data File : P0064473.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Dec 2019 13:21
Operator : SM/AJ
Sample : PB125311BL
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB125311BL


Manual Integrations
APPROVED

Ankita
12/10/2019 10:09:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 13:37:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112719.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 28 01:28:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

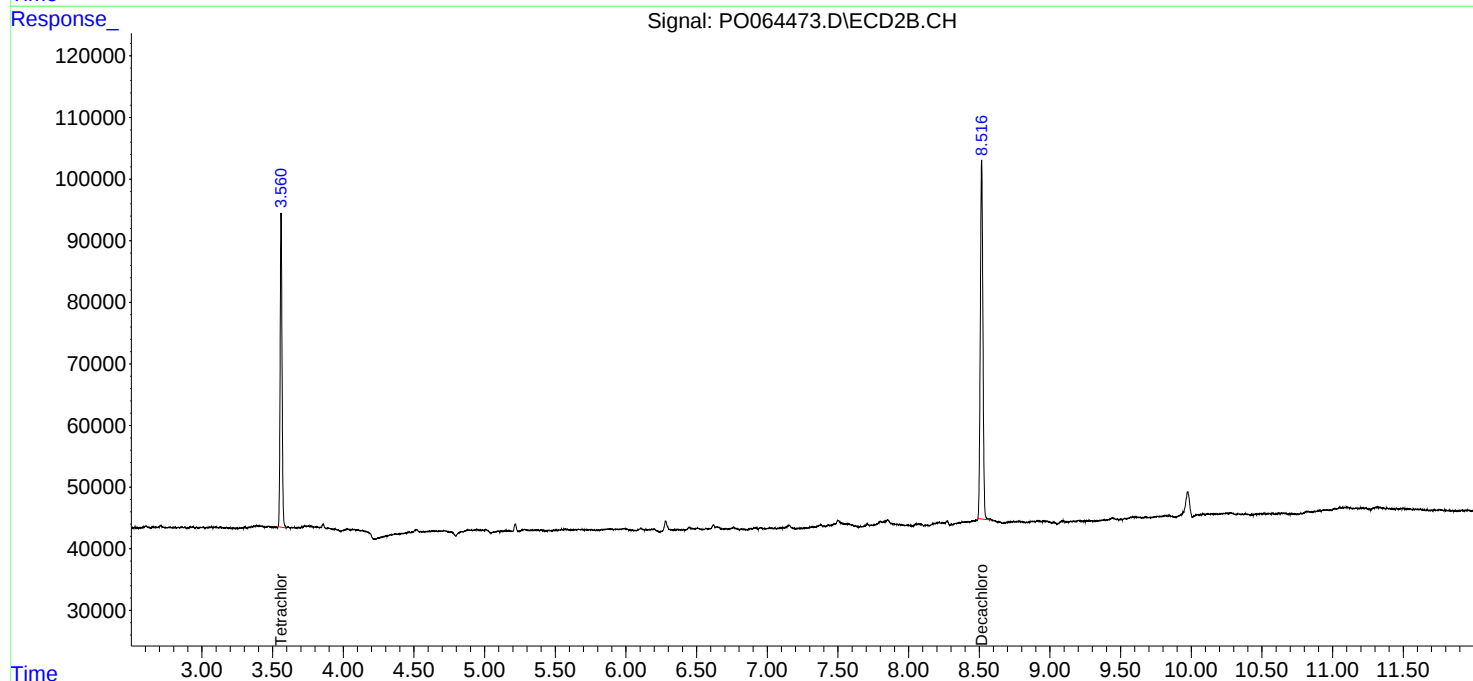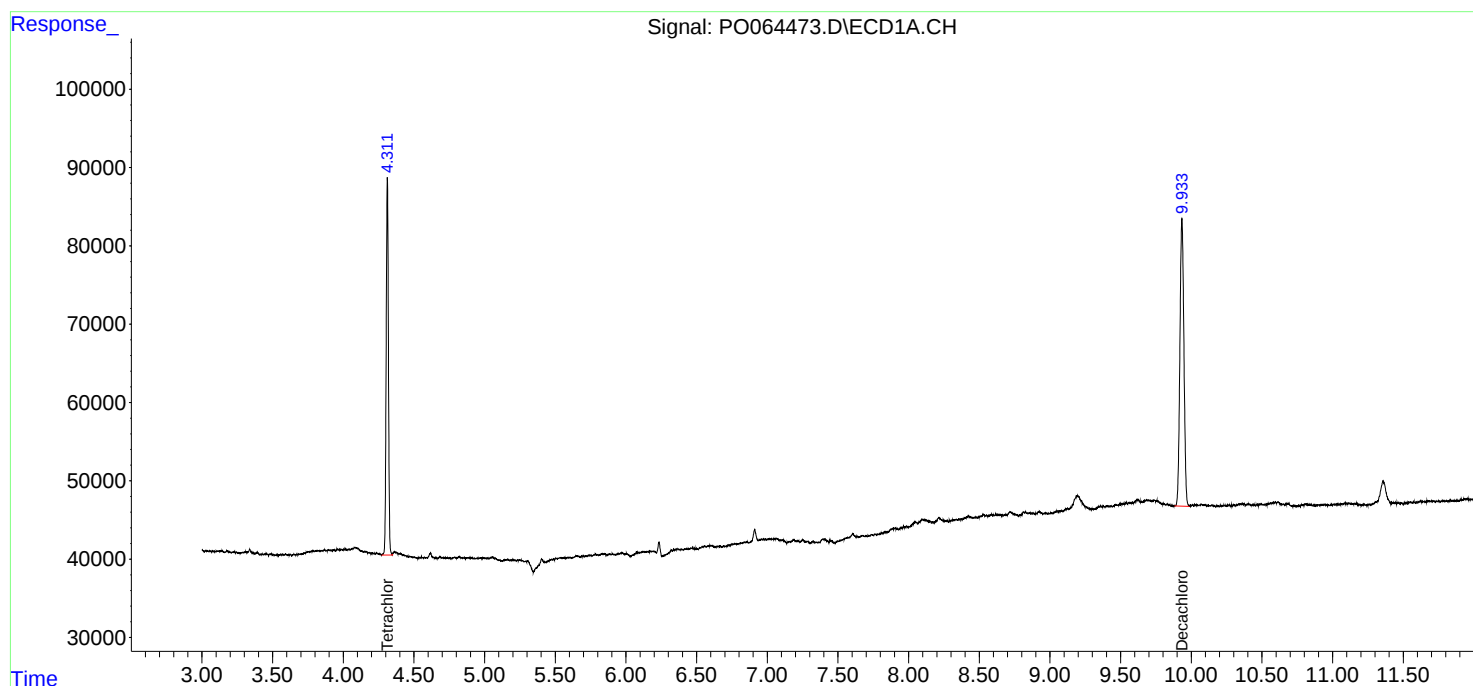

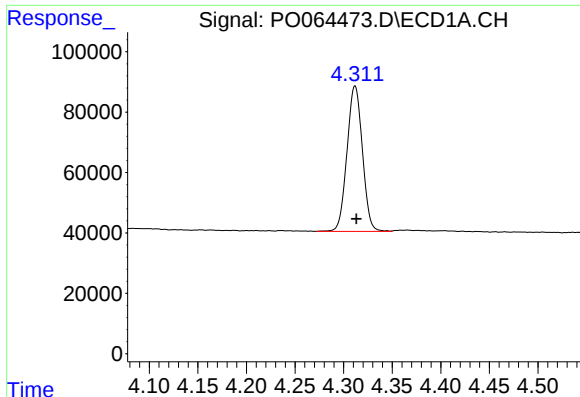


#1 Tetrachloro-m-xylene

R.T.: 4.311 min
Delta R.T.: -0.002 min
Response: 530919
Conc: 17.93 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PB125311BL


Manual Integrations
APPROVED

Ankita
12/10/2019 10:09:21 AM

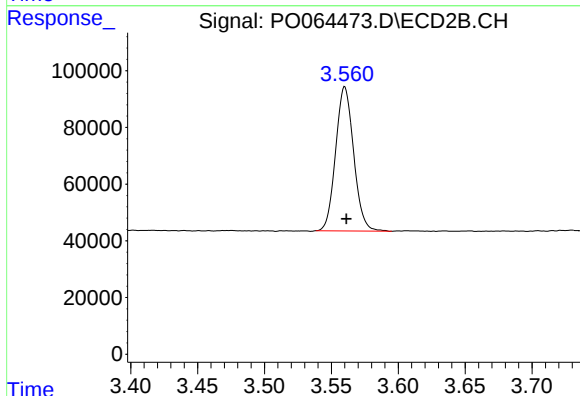


#1 Tetrachloro-m-xylene

R.T.: 3.560 min
Delta R.T.: -0.001 min
Response: 476301
Conc: 20.03 ng/ml

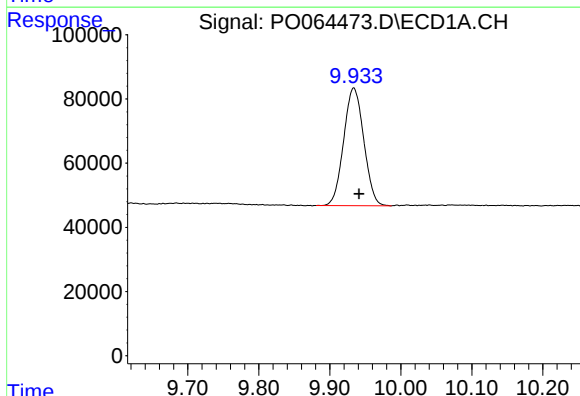

#2 Decachlorobiphenyl

R.T.: 9.934 min
Delta R.T.: -0.007 min
Response: 721709
Conc: 17.61 ng/ml

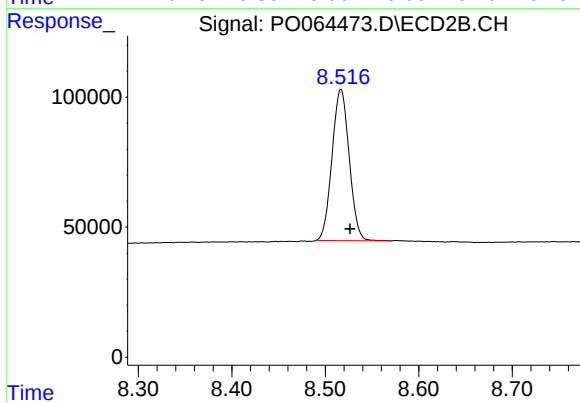

#2 Decachlorobiphenyl

R.T.: 8.517 min
Delta R.T.: -0.010 min
Response: 743238
Conc: 18.19 ng/ml