

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO120921\
 Data File : PO083503.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Dec 2021 9:51
 Operator : AJ\MA
 Sample : M4953-01RE
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 14:08:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO120621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 07 13:18:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.941	3.945	1775501	577389	18.610	18.562
2)	SA Decachlor...	11.019	9.244	179701	81753	2.516	2.506
Target Compounds							
24)	L5 AR-1248-4	7.197f	0.000	15582	0	5.154	N.D. #
26)	L6 AR-1254-1	7.197	0.000	15582	0	4.876	N.D. #
28)	L6 AR-1254-3	7.822f	0.000	14898	0	2.987	N.D. #
30)	L6 AR-1254-5	8.528	0.000	5693	0	1.587	N.D. #
33)	L7 AR-1260-3	8.602	0.000	2919	0	0.931	N.D. #
34)	L7 AR-1260-4	8.850	0.000	3394	0	0.969	N.D. #
36)	L8 AR-1262-1	8.602	0.000	2919	0	0.703	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120921\
Data File : PO083503.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Dec 2021 9:51
Operator : AJ\MA
Sample : M4953-01RE
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 14:08:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 07 13:18:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

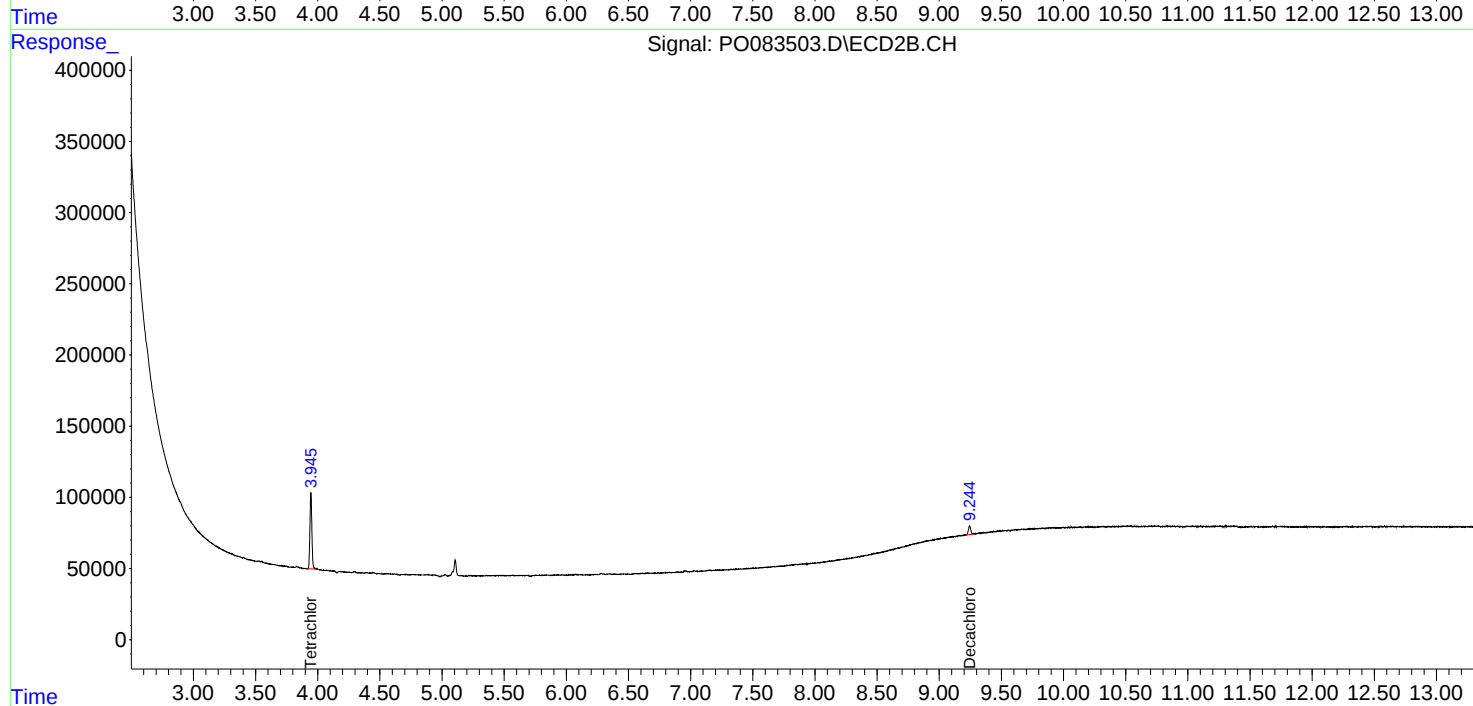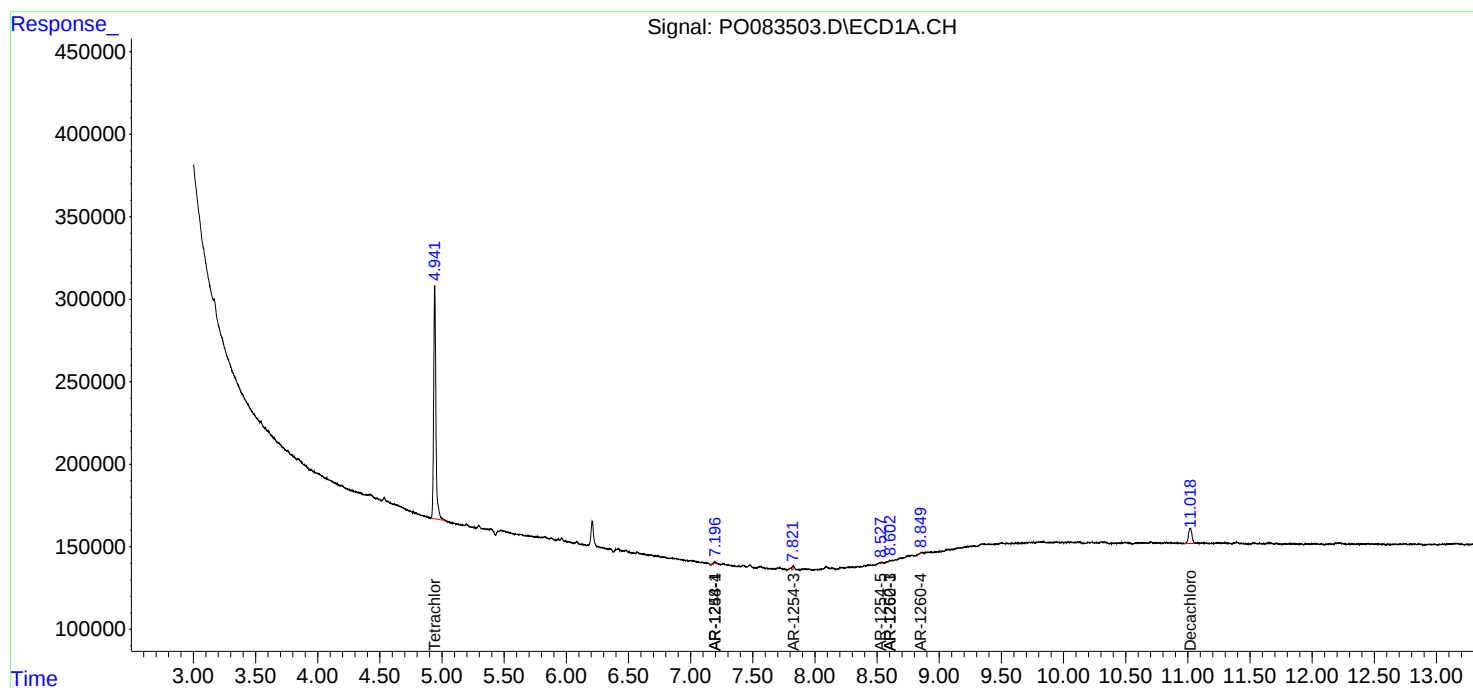


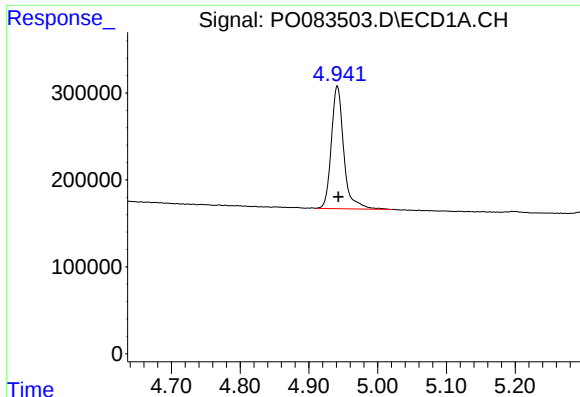

#1 Tetrachloro-m-xylene


R.T.: 4.941 min
Delta R.T.: -0.002 min
Response: 1775501
Conc: 18.61 ng/ml

Instrument :
ECD_O
ClientSampleId :

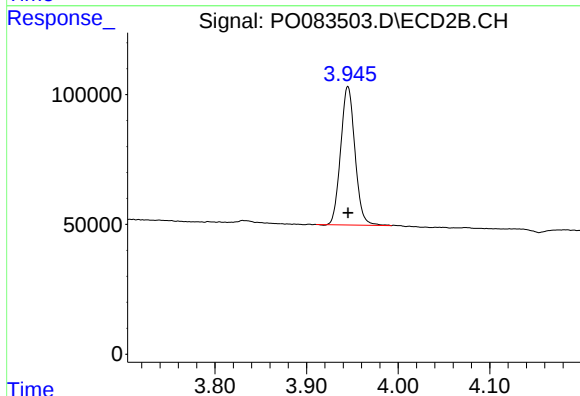


#1 Tetrachloro-m-xylene

R.T.: 3.945 min
Delta R.T.: 0.000 min
Response: 577389
Conc: 18.56 ng/ml

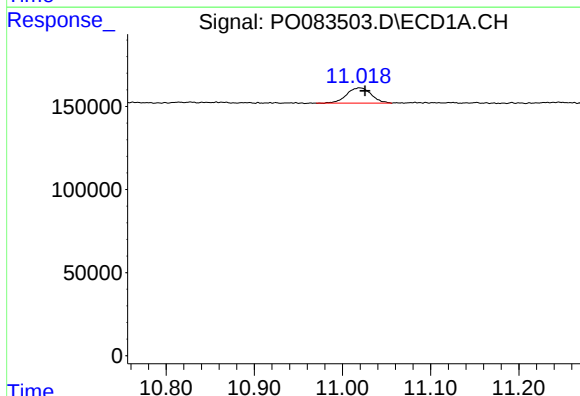


#2 Decachlorobiphenyl

R.T.: 11.019 min
Delta R.T.: -0.006 min
Response: 179701
Conc: 2.52 ng/ml

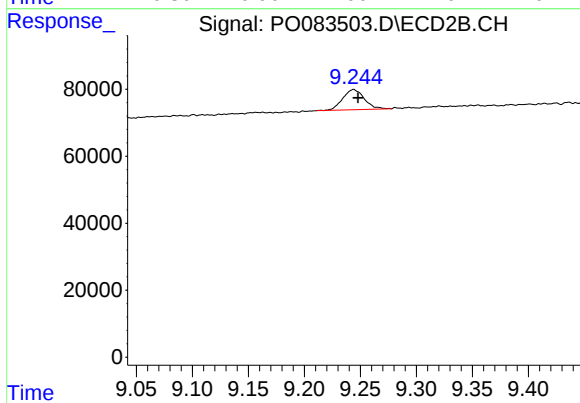

#2 Decachlorobiphenyl


R.T.: 9.244 min
Delta R.T.: -0.004 min
Response: 81753
Conc: 2.51 ng/ml

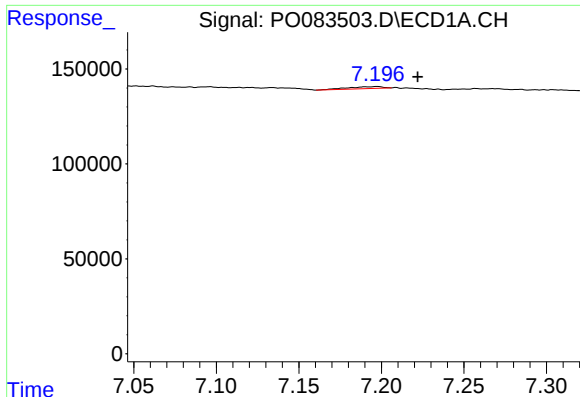

#24 AR-1248-4


R.T.: 7.197 min
Delta R.T.: -0.025 min
Response: 15582
Conc: 5.15 ng/ml

Instrument :
ECD_O
ClientSampleId :

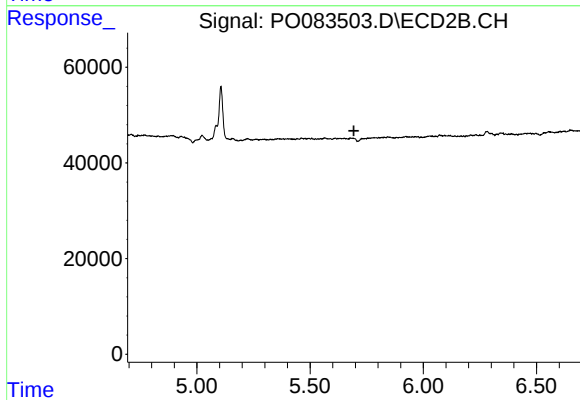


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.693 min
Response: 0
Conc: N.D.

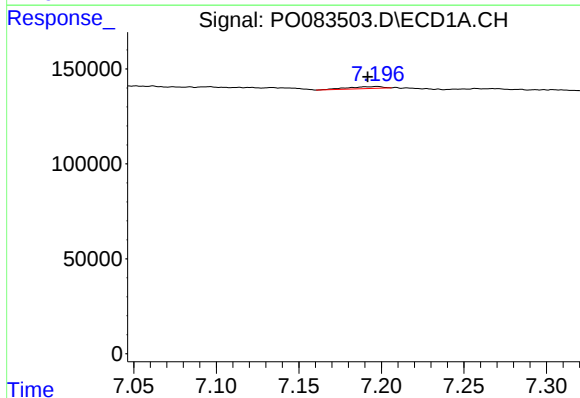


#26 AR-1254-1

R.T.: 7.197 min
Delta R.T.: 0.006 min
Response: 15582
Conc: 4.88 ng/ml

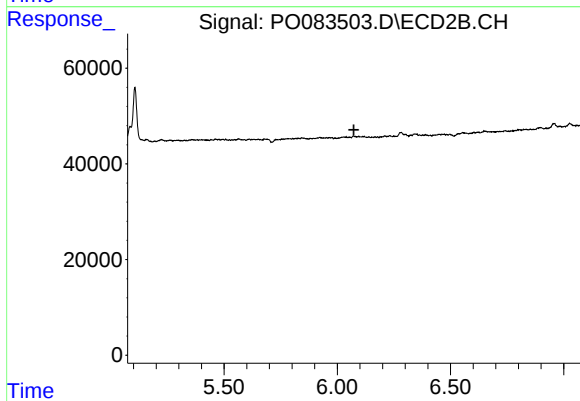

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.073 min
Response: 0
Conc: N.D.

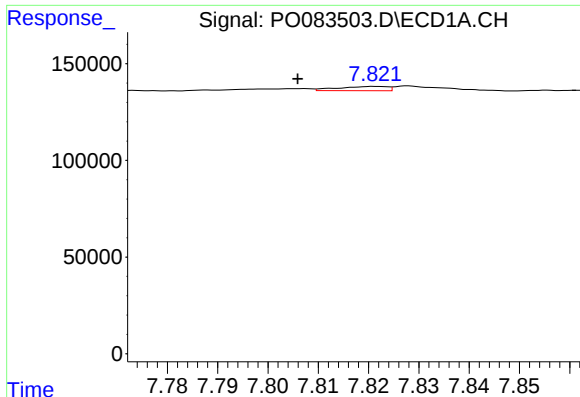

#28 AR-1254-3


R.T.: 7.822 min
Delta R.T.: 0.016 min
Response: 14898
Conc: 2.99 ng/ml

Instrument :
ECD_O
ClientSampleId :

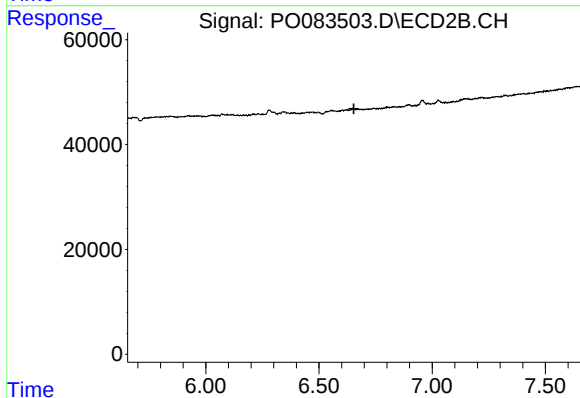


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.654 min
Response: 0
Conc: N.D.

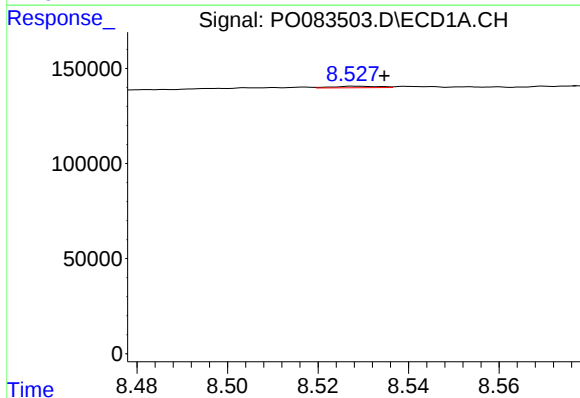


#30 AR-1254-5

R.T.: 8.528 min
Delta R.T.: -0.006 min
Response: 5693
Conc: 1.59 ng/ml

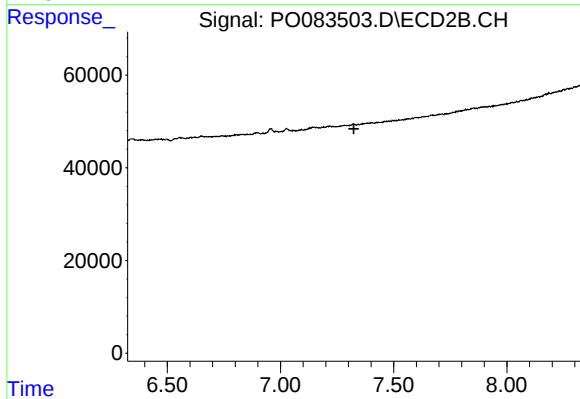

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.324 min
Response: 0
Conc: N.D.

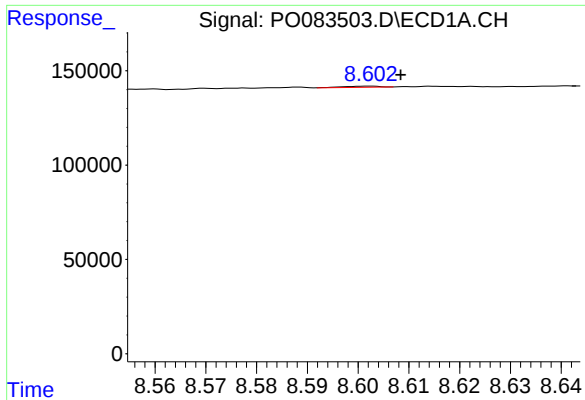

#33 AR-1260-3


R.T.: 8.602 min
Delta R.T.: -0.006 min
Response: 2919
Conc: 0.93 ng/ml

Instrument :
ECD_O
ClientSampleId :

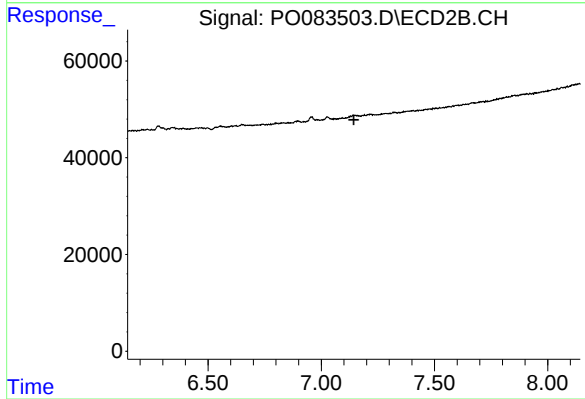


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.144 min
Response: 0
Conc: N.D.

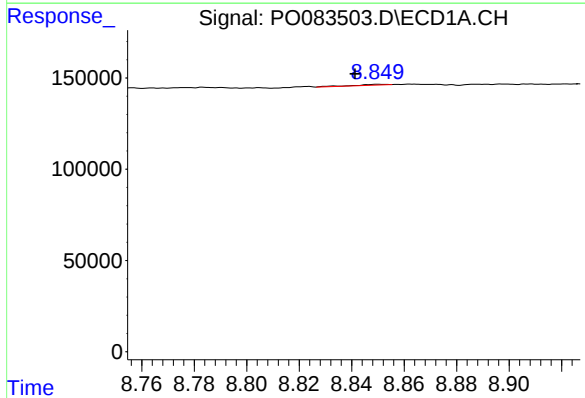


#34 AR-1260-4

R.T.: 8.850 min
Delta R.T.: 0.008 min
Response: 3394
Conc: 0.97 ng/ml

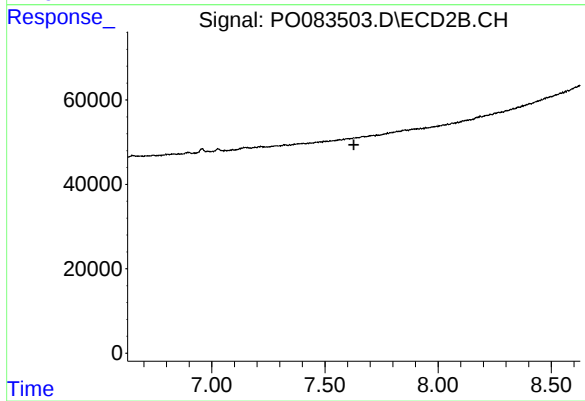

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.628 min
Response: 0
Conc: N.D.

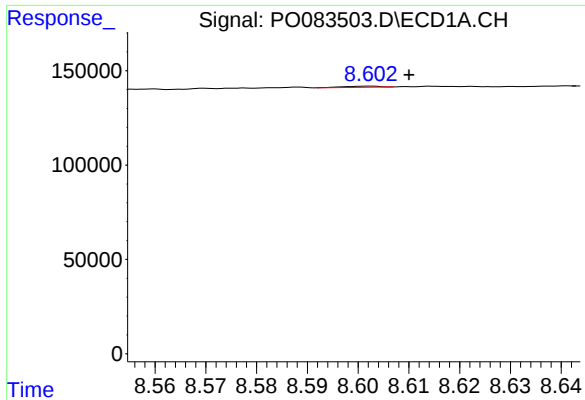

#36 AR-1262-1

R.T.: 8.602 min
Delta R.T.: -0.008 min
Response: 2919
Conc: 0.70 ng/ml

Instrument :
ECD_O
ClientSampleId :

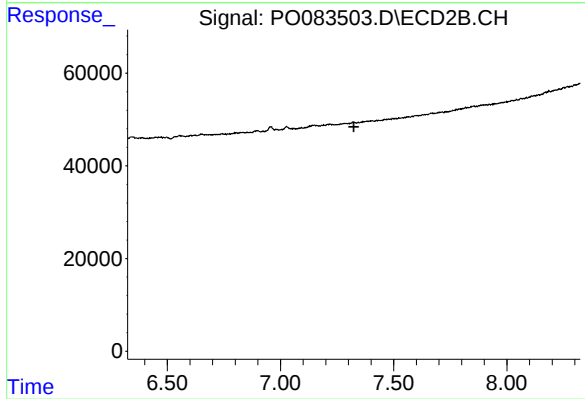

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.324 min
Response: 0
Conc: N.D.